

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022525.D
 Acq On : 02 Oct 2021 20:52
 Operator : SY/MD
 Sample : M4023-09DL 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	106235	105713	15.51%	1.728%
2	1.565	156	163	180	rVB	88708	100428	14.73%	1.642%
3	2.108	322	332	355	rBV2	197957	306974	45.03%	5.019%
4	2.658	500	503	506	rBV2	215	216	0.03%	0.004%
5	2.838	556	559	561	rBV	197	103	0.02%	0.002%
6	2.937	588	590	593	rVB	383	168	0.02%	0.003%
7	2.950	593	594	595	rBV	228	71	0.01%	0.001%
8	2.982	602	604	605	rBV	228	74	0.01%	0.001%
9	3.114	643	645	647	rBV2	131	75	0.01%	0.001%
10	3.269	690	693	696	rVB	210	140	0.02%	0.002%
11	3.291	696	700	703	rBV	193	178	0.03%	0.003%
12	3.410	735	737	739	rVB	256	99	0.01%	0.002%
13	3.433	739	744	747	rBV	252	264	0.04%	0.004%
14	3.494	761	763	764	rBV	180	85	0.01%	0.001%
15	3.548	778	780	782	rBV	238	74	0.01%	0.001%
16	3.658	811	814	815	rBV	268	111	0.02%	0.002%
17	3.722	830	834	835	rBV2	159	137	0.02%	0.002%
18	3.780	848	852	855	rBV2	285	202	0.03%	0.003%
19	3.908	876	892	925	rBV3	43188	174650	25.62%	2.855%
20	4.346	1015	1028	1059	rVB	100207	275509	40.41%	4.504%
21	4.613	1099	1111	1130	rVB3	17190	43967	6.45%	0.719%
22	4.680	1130	1132	1134	rBV2	239	79	0.01%	0.001%
23	4.886	1192	1196	1198	rBV2	228	132	0.02%	0.002%
24	5.047	1229	1246	1271	rBV2	265478	681725	100.00%	11.146%
25	5.407	1355	1358	1360	rBV2	513	305	0.04%	0.005%
26	5.445	1365	1370	1375	rVB2	496	493	0.07%	0.008%
27	5.471	1375	1378	1381	rBV2	298	281	0.04%	0.005%
28	5.490	1382	1384	1385	rBV	273	91	0.01%	0.001%
29	5.558	1402	1405	1406	rBV2	270	149	0.02%	0.002%
30	5.616	1412	1423	1446	rBV	246941	497961	73.04%	8.141%
31	5.915	1503	1516	1542	rBV	292278	577584	84.72%	9.443%
32	6.069	1553	1564	1588	rBV	146291	298133	43.73%	4.874%
33	6.278	1627	1629	1630	rBV	366	164	0.02%	0.003%
34	6.349	1648	1651	1653	rBV2	352	190	0.03%	0.003%
35	6.423	1672	1674	1677	rBV2	204	88	0.01%	0.001%
36	6.558	1713	1716	1719	rVB	335	153	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100221\
 Data File : VW022525.D
 Acq On : 02 Oct 2021 20:52
 Operator : SY/MD
 Sample : M4023-09DL 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	6.577	1719	1722	1723	rBV	322	210	0.03%	0.003%
38	6.838	1801	1803	1804	rBV	157	83	0.01%	0.001%
39	6.941	1831	1835	1838	rBV	247	248	0.04%	0.004%
40	6.989	1839	1850	1874	rVV	78523	141145	20.70%	2.308%
41	7.227	1921	1924	1926	rBV2	296	215	0.03%	0.004%
42	7.317	1940	1952	1971	rBV	315738	557113	81.72%	9.108%
43	7.625	2037	2048	2070	rBV	53715	94475	13.86%	1.545%
44	7.825	2108	2110	2111	rBV	245	122	0.02%	0.002%
45	7.834	2111	2113	2117	rVB2	506	339	0.05%	0.006%
46	7.860	2117	2121	2123	rBV2	189	160	0.02%	0.003%
47	7.931	2139	2143	2144	rBV2	199	141	0.02%	0.002%
48	7.979	2156	2158	2160	rBV	232	95	0.01%	0.002%
49	8.092	2183	2193	2223	rBV	129696	290714	42.64%	4.753%
50	8.349	2271	2273	2278	rVB3	614	446	0.07%	0.007%
51	8.371	2278	2280	2282	rBV2	253	180	0.03%	0.003%
52	8.429	2295	2298	2300	rBV2	406	295	0.04%	0.005%
53	8.603	2350	2352	2354	rBV2	215	98	0.01%	0.002%
54	8.638	2360	2363	2364	rBV	348	187	0.03%	0.003%
55	8.854	2419	2430	2449	rBV	367715	597521	87.65%	9.769%
56	9.092	2501	2504	2508	rBV	261	252	0.04%	0.004%
57	9.149	2516	2522	2531	rVB5	1799	2297	0.34%	0.038%
58	9.220	2540	2544	2548	rVB3	431	242	0.04%	0.004%
59	9.358	2582	2587	2590	rBV	217	211	0.03%	0.003%
60	9.413	2601	2604	2605	rBV2	176	108	0.02%	0.002%
61	9.516	2632	2636	2637	rBV	313	178	0.03%	0.003%
62	9.558	2641	2649	2657	rBV5	1315	2219	0.33%	0.036%
63	9.600	2660	2662	2666	rBV2	152	147	0.02%	0.002%
64	9.741	2700	2706	2712	rBV3	310	419	0.06%	0.007%
65	9.789	2719	2721	2725	rBV2	342	211	0.03%	0.003%
66	10.005	2786	2788	2789	rBV	228	86	0.01%	0.001%
67	10.085	2810	2813	2815	rBV	182	151	0.02%	0.002%
68	10.127	2821	2826	2835	rBV3	1694	1945	0.29%	0.032%
69	10.217	2843	2854	2871	rBV2	198075	308580	45.26%	5.045%
70	10.320	2881	2886	2891	rBV2	517	581	0.09%	0.009%
71	10.387	2904	2907	2909	rBV2	343	176	0.03%	0.003%
72	10.464	2925	2931	2935	rBV3	497	467	0.07%	0.008%
73	10.690	2997	3001	3004	rBV2	317	222	0.03%	0.004%
74	10.731	3011	3014	3016	rVB	276	131	0.02%	0.002%
75	10.831	3042	3045	3052	rVB	453	407	0.06%	0.007%
76	11.043	3109	3111	3114	rVB2	258	103	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022525.D
 Acq On : 02 Oct 2021 20:52
 Operator : SY/MD
 Sample : M4023-09DL 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.143	3138	3142	3144	rBV2	705	631	0.09%	0.010%
78	11.249	3164	3175	3196	rBV	362008	555683	81.51%	9.085%
79	11.429	3225	3231	3234	rBV3	872	962	0.14%	0.016%
80	11.625	3280	3292	3308	rBV	313854	485723	71.25%	7.941%
81	11.940	3386	3390	3391	rBV	247	137	0.02%	0.002%
82	11.966	3395	3398	3400	rVB	386	196	0.03%	0.003%
83	12.043	3418	3422	3425	rBV2	215	182	0.03%	0.003%
84	12.342	3511	3515	3517	rBV	429	302	0.04%	0.005%
85	12.419	3537	3539	3542	rBV2	232	136	0.02%	0.002%
86	12.574	3585	3587	3592	rVB2	174	113	0.02%	0.002%
87	12.603	3592	3596	3597	rBV	402	227	0.03%	0.004%
88	12.683	3619	3621	3623	rBV	206	108	0.02%	0.002%
89	12.889	3680	3685	3687	rBV2	369	285	0.04%	0.005%
90	12.976	3709	3712	3717	rBV2	194	231	0.03%	0.004%
91	13.059	3736	3738	3740	rBV	128	75	0.01%	0.001%
92	13.124	3756	3758	3759	rBV	267	113	0.02%	0.002%
93	13.194	3779	3780	3783	rVB	231	104	0.02%	0.002%
94	13.378	3833	3837	3840	rBV	243	227	0.03%	0.004%
95	13.451	3856	3860	3861	rBV	237	198	0.03%	0.003%
96	13.477	3865	3868	3875	rVB4	404	409	0.06%	0.007%
97	13.770	3956	3959	3960	rVB	388	172	0.03%	0.003%
98	14.098	4060	4061	4064	rVB2	394	150	0.02%	0.002%
99	14.423	4160	4162	4168	rBV3	355	390	0.06%	0.006%
100	14.554	4202	4203	4204	rBV	276	73	0.01%	0.001%




Sum of corrected areas: 6116513

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022525.D
Acq On : 02 Oct 2021 20:52
Operator : SY/MD
Sample : M4023-09DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

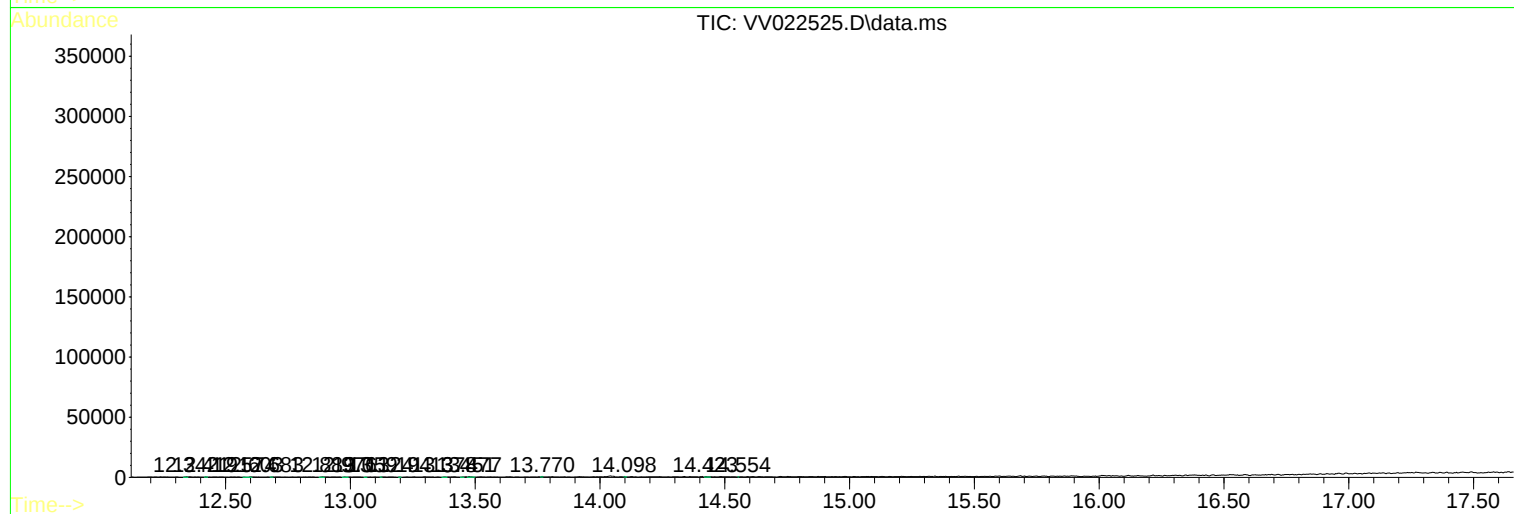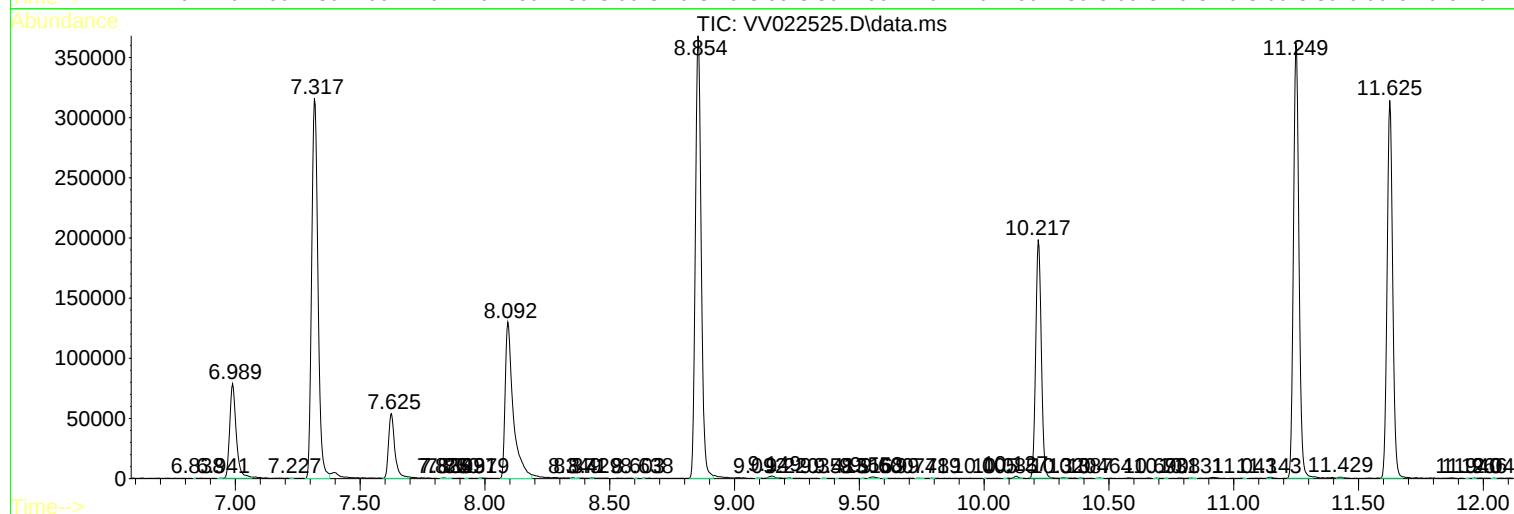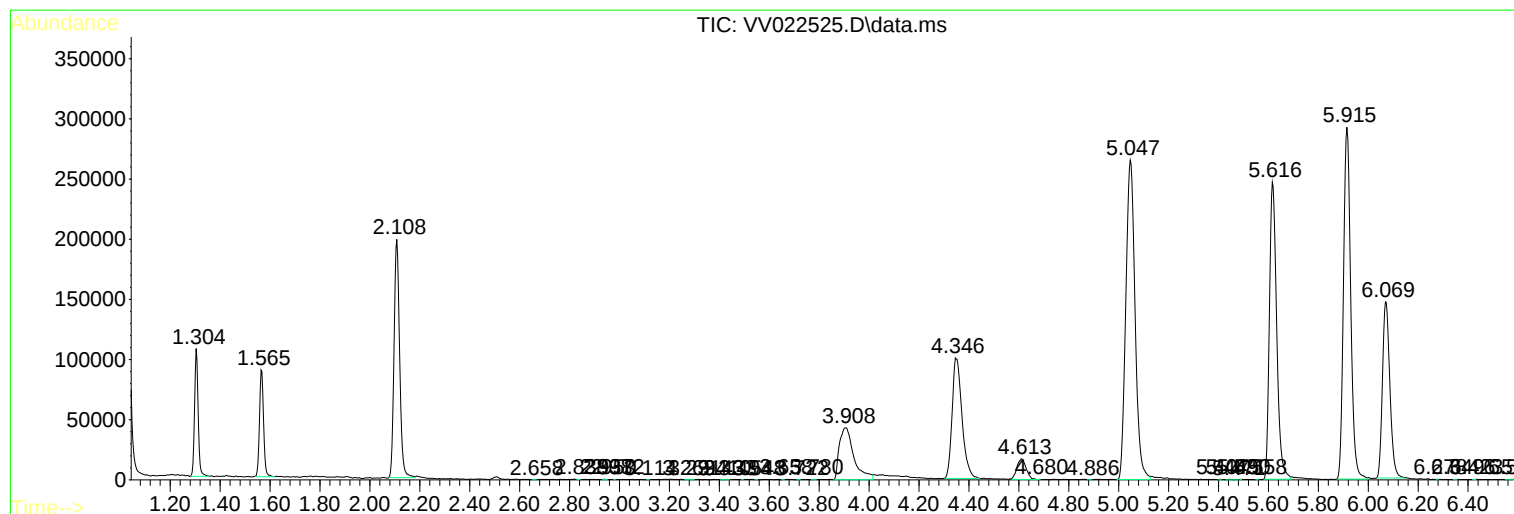

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022525.D
Acq On : 02 Oct 2021 20:52
Operator : SY/MD
Sample : M4023-09DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022525.D
Acq On : 02 Oct 2021 20:52
Operator : SY/MD
Sample : M4023-09DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
