

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022528.D
 Acq On : 02 Oct 2021 22:50
 Operator : SY/MD
 Sample : VV1002MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK274

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

Signal : TIC: VV022528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	105592	109610	16.02%	2.015%
2	1.564	157	163	179	rVB	87210	101342	14.81%	1.863%
3	2.053	313	315	317	rBV2	756	448	0.07%	0.008%
4	2.108	322	332	349	rVV	186423	274714	40.14%	5.049%
5	2.555	464	471	474	rVB3	300	351	0.05%	0.006%
6	2.683	507	511	516	rVB2	374	330	0.05%	0.006%
7	2.818	551	553	555	rBV2	608	174	0.03%	0.003%
8	2.850	561	563	565	rBV	228	108	0.02%	0.002%
9	2.998	605	609	613	rVB	357	284	0.04%	0.005%
10	3.079	631	634	635	rBV	230	105	0.02%	0.002%
11	3.101	639	641	642	rBV	375	175	0.03%	0.003%
12	3.191	665	669	672	rBV2	149	124	0.02%	0.002%
13	3.265	690	692	694	rBV	397	145	0.02%	0.003%
14	3.349	717	718	722	rVB	417	165	0.02%	0.003%
15	3.407	735	736	742	rVB2	369	261	0.04%	0.005%
16	3.471	755	756	759	rVB	499	147	0.02%	0.003%
17	3.493	759	763	766	rBV2	235	203	0.03%	0.004%
18	3.519	766	771	776	rVB2	246	289	0.04%	0.005%
19	3.558	779	783	788	rBV2	160	149	0.02%	0.003%
20	3.583	788	791	795	rBV	181	189	0.03%	0.003%
21	3.619	795	802	805	rBV	252	266	0.04%	0.005%
22	3.747	839	842	843	rBV	191	114	0.02%	0.002%
23	3.776	847	851	853	rBV2	183	156	0.02%	0.003%
24	3.850	872	874	877	rBV	233	156	0.02%	0.003%
25	3.892	877	887	917	rBV	27909	96768	14.14%	1.779%
26	4.349	1017	1029	1058	rVB	104302	273045	39.90%	5.018%
27	4.641	1117	1120	1122	rVB2	352	175	0.03%	0.003%
28	4.709	1139	1141	1143	rBV2	404	245	0.04%	0.005%
29	4.857	1184	1187	1188	rBV	254	164	0.02%	0.003%
30	4.963	1216	1220	1225	rBV2	444	456	0.07%	0.008%
31	5.046	1230	1246	1272	rBV2	269423	684362	100.00%	12.578%
32	5.362	1339	1344	1347	rBV2	358	366	0.05%	0.007%
33	5.516	1389	1392	1397	rVB2	341	255	0.04%	0.005%
34	5.542	1397	1400	1401	rBV	262	133	0.02%	0.002%
35	5.619	1411	1424	1451	rBV	248930	503192	73.53%	9.248%
36	5.847	1492	1495	1497	rBV2	265	184	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022528.D
 Acq On : 02 Oct 2021 22:50
 Operator : SY/MD
 Sample : VV1002MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK274

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	5.911	1505	1515	1532	rVB5	12911	30792	4.50%	0.566%
38	6.072	1549	1565	1588	rBV	149915	307460	44.93%	5.651%
39	6.355	1649	1653	1656	rBV2	408	392	0.06%	0.007%
40	6.461	1682	1686	1689	rVB2	324	290	0.04%	0.005%
41	6.487	1689	1694	1696	rBV2	462	400	0.06%	0.007%
42	6.638	1736	1741	1746	rVB2	485	539	0.08%	0.010%
43	6.664	1746	1749	1750	rBV	241	138	0.02%	0.003%
44	6.677	1750	1753	1755	rBV3	301	200	0.03%	0.004%
45	6.751	1774	1776	1779	rBV	289	151	0.02%	0.003%
46	6.815	1792	1796	1799	rVB	406	248	0.04%	0.005%
47	6.989	1839	1850	1877	rBV	76263	140432	20.52%	2.581%
48	7.165	1903	1905	1908	rBV	224	110	0.02%	0.002%
49	7.198	1913	1915	1917	rBV	297	160	0.02%	0.003%
50	7.316	1940	1952	1972	rBV	317443	555342	81.15%	10.207%
51	7.545	2020	2023	2024	rBV	335	182	0.03%	0.003%
52	7.625	2038	2048	2065	rBV2	50962	90590	13.24%	1.665%
53	7.876	2122	2126	2128	rBV2	190	159	0.02%	0.003%
54	7.979	2156	2158	2160	rBV	279	164	0.02%	0.003%
55	8.030	2170	2174	2176	rBV	185	146	0.02%	0.003%
56	8.091	2183	2193	2228	rBV	124542	295684	43.21%	5.434%
57	8.416	2291	2294	2300	rBV3	576	494	0.07%	0.009%
58	8.442	2300	2302	2305	rBV2	274	174	0.03%	0.003%
59	8.615	2351	2356	2359	rBV2	327	313	0.05%	0.006%
60	8.657	2366	2369	2370	rBV	226	129	0.02%	0.002%
61	8.696	2378	2381	2383	rVB3	252	141	0.02%	0.003%
62	8.757	2397	2400	2403	rBV2	173	128	0.02%	0.002%
63	8.853	2418	2430	2462	rBV	367483	605985	88.55%	11.138%
64	9.075	2496	2499	2501	rBV	312	263	0.04%	0.005%
65	9.297	2564	2568	2570	rVB3	354	273	0.04%	0.005%
66	9.558	2644	2649	2656	rVB3	345	448	0.07%	0.008%
67	9.596	2656	2661	2663	rBV2	289	287	0.04%	0.005%
68	9.844	2734	2738	2740	rBV2	285	225	0.03%	0.004%
69	9.985	2779	2782	2785	rVV2	309	152	0.02%	0.003%
70	10.011	2788	2790	2797	rVB2	267	296	0.04%	0.005%
71	10.043	2797	2800	2803	rBV	302	166	0.02%	0.003%
72	10.130	2822	2827	2835	rVB2	1340	1752	0.26%	0.032%
73	10.217	2842	2854	2870	rBV	196147	310466	45.37%	5.706%
74	10.458	2926	2929	2932	rBV	183	145	0.02%	0.003%
75	10.545	2952	2956	2958	rBV2	499	333	0.05%	0.006%
76	10.583	2965	2968	2970	rBV	433	245	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022528.D
 Acq On : 02 Oct 2021 22:50
 Operator : SY/MD
 Sample : VV1002MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK274

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	10.644	2984	2987	2989	rBV2	177	128	0.02%	0.002%
78	10.770	3023	3026	3031	rBV	270	148	0.02%	0.003%
79	11.111	3130	3132	3135	rVB	219	125	0.02%	0.002%
80	11.249	3164	3175	3193	rBV	354706	552981	80.80%	10.163%
81	11.393	3215	3220	3223	rBV5	930	818	0.12%	0.015%
82	11.519	3256	3259	3261	rBV	191	119	0.02%	0.002%
83	11.625	3280	3292	3310	rBV	308628	485873	71.00%	8.930%
84	11.728	3321	3324	3327	rBV2	549	423	0.06%	0.008%
85	11.950	3390	3393	3394	rBV	308	182	0.03%	0.003%
86	12.011	3408	3412	3414	rBV2	285	202	0.03%	0.004%
87	12.104	3439	3441	3443	rBV	290	152	0.02%	0.003%
88	12.274	3490	3494	3496	rBV	268	210	0.03%	0.004%
89	12.477	3555	3557	3560	rBV	265	160	0.02%	0.003%
90	12.657	3607	3613	3619	rVB2	598	749	0.11%	0.014%
91	12.696	3619	3625	3629	rBV3	425	354	0.05%	0.007%
92	12.856	3672	3675	3678	rBV2	231	199	0.03%	0.004%
93	13.152	3763	3767	3769	rBV2	434	262	0.04%	0.005%
94	13.268	3796	3803	3805	rBV4	851	810	0.12%	0.015%
95	13.503	3873	3876	3877	rBV4	434	273	0.04%	0.005%
96	13.635	3914	3917	3920	rBV2	313	216	0.03%	0.004%
97	13.725	3942	3945	3948	rBV2	332	214	0.03%	0.004%
98	13.979	4021	4024	4029	rBV2	263	252	0.04%	0.005%
99	14.866	4296	4300	4302	rBV2	418	340	0.05%	0.006%
100	15.204	4401	4405	4407	rBV2	429	363	0.05%	0.007%




Sum of corrected areas: 5440897

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022528.D
Acq On : 02 Oct 2021 22:50
Operator : SY/MD
Sample : VV1002MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK274

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

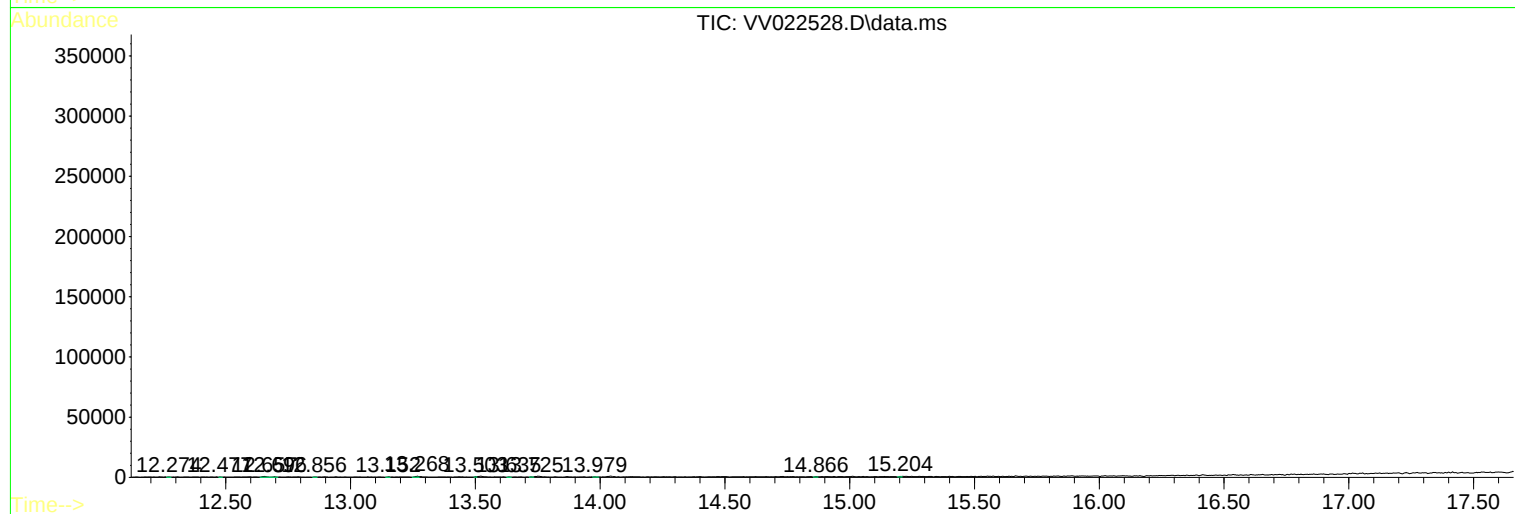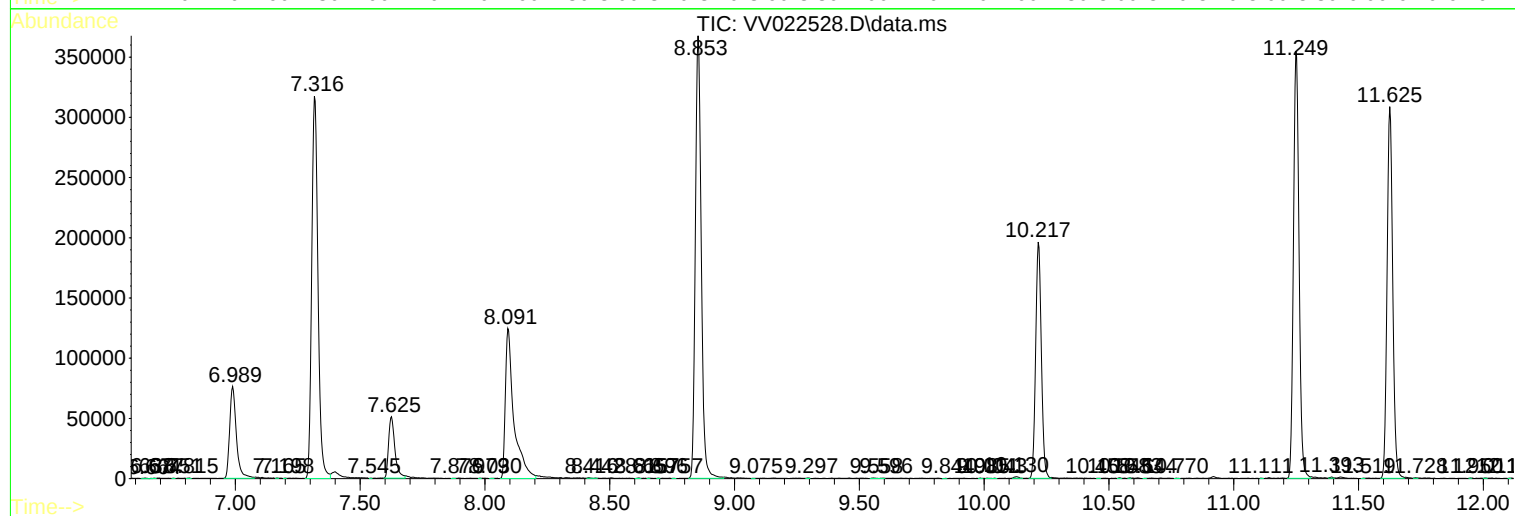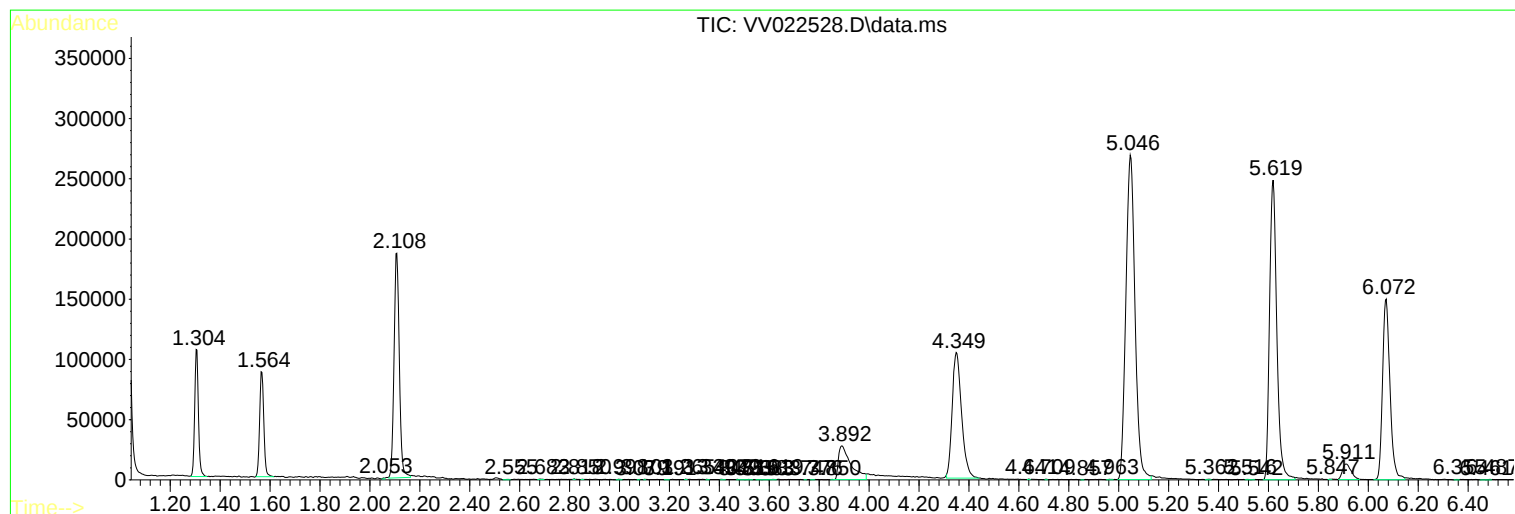

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022528.D
Acq On : 02 Oct 2021 22:50
Operator : SY/MD
Sample : VV1002MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK274

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022528.D
Acq On : 02 Oct 2021 22:50
Operator : SY/MD
Sample : VV1002MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK274

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
