

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022531.D
 Acq On : 03 Oct 2021 00:01
 Operator : SY/MD
 Sample : M3973-08ME
 Misc : 5.01g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8X4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rVB	68305	102690	13.89%	1.865%
2	1.568	158	164	192	rVB	35931	79647	10.77%	1.446%
3	2.092	319	327	344	rVB	176029	248065	33.55%	4.505%
4	2.725	521	524	526	rBV	440	233	0.03%	0.004%
5	2.934	587	589	593	rVB2	276	130	0.02%	0.002%
6	3.063	627	629	631	rBV2	233	126	0.02%	0.002%
7	3.429	739	743	746	rBV2	217	264	0.04%	0.005%
8	3.497	762	764	766	rBV	161	65	0.01%	0.001%
9	3.552	779	781	785	rVB2	287	106	0.01%	0.002%
10	3.593	791	794	796	rBV2	192	114	0.02%	0.002%
11	3.610	797	799	802	rBV2	256	145	0.02%	0.003%
12	3.934	889	900	902	rBV2	14799	24845	3.36%	0.451%
13	4.664	1124	1127	1130	rBV3	353	239	0.03%	0.004%
14	4.745	1148	1152	1156	rBV2	233	220	0.03%	0.004%
15	4.806	1165	1171	1172	rBV2	451	364	0.05%	0.007%
16	4.880	1191	1194	1196	rVB3	301	185	0.03%	0.003%
17	4.982	1223	1226	1229	rBV2	415	310	0.04%	0.006%
18	5.044	1229	1245	1277	rBV3	293841	739475	100.00%	13.428%
19	5.355	1331	1342	1347	rBV7	2526	5573	0.75%	0.101%
20	5.494	1383	1385	1388	rVB2	586	310	0.04%	0.006%
21	5.516	1388	1392	1394	rBV2	385	241	0.03%	0.004%
22	5.616	1411	1423	1455	rBV	266882	572502	77.42%	10.396%
23	5.915	1503	1516	1535	rBV5	22629	55335	7.48%	1.005%
24	6.072	1553	1565	1592	rVB	146717	322438	43.60%	5.855%
25	6.484	1689	1693	1696	rBV2	225	241	0.03%	0.004%
26	6.661	1745	1748	1750	rBV3	556	324	0.04%	0.006%
27	6.696	1757	1759	1760	rBV3	242	80	0.01%	0.001%
28	6.716	1763	1765	1767	rBV	162	82	0.01%	0.001%
29	6.741	1771	1773	1776	rBV2	304	212	0.03%	0.004%
30	6.806	1791	1793	1795	rBV	364	217	0.03%	0.004%
31	6.873	1811	1814	1819	rBV	273	193	0.03%	0.004%
32	6.989	1837	1850	1877	rBV	71443	149427	20.21%	2.713%
33	7.159	1900	1903	1905	rBV3	396	278	0.04%	0.005%
34	7.224	1921	1923	1928	rVB	521	334	0.05%	0.006%
35	7.249	1928	1931	1933	rBV	197	160	0.02%	0.003%
36	7.317	1940	1952	1971	rBV	330390	600147	81.16%	10.898%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022531.D
 Acq On : 03 Oct 2021 00:01
 Operator : SY/MD
 Sample : M3973-08ME
 Misc : 5.01g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8X4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	7.539	2019	2021	2023	rVB	279	103	0.01%	0.002%
38	7.555	2023	2026	2027	rBV	402	202	0.03%	0.004%
39	7.629	2039	2049	2076	rBV	47449	98563	13.33%	1.790%
40	7.834	2108	2113	2116	rBV2	457	428	0.06%	0.008%
41	7.937	2143	2145	2146	rBV2	204	92	0.01%	0.002%
42	7.963	2151	2153	2155	rBV	119	70	0.01%	0.001%
43	8.040	2175	2177	2179	rVB	272	133	0.02%	0.002%
44	8.063	2179	2184	2187	rBV2	358	302	0.04%	0.005%
45	8.130	2187	2205	2236	rBV2	76856	290842	39.33%	5.281%
46	8.474	2308	2312	2317	rBV3	288	310	0.04%	0.006%
47	8.558	2336	2338	2343	rVB3	448	356	0.05%	0.006%
48	8.596	2348	2350	2353	rVB	341	147	0.02%	0.003%
49	8.760	2399	2401	2404	rBV	200	107	0.01%	0.002%
50	8.857	2419	2431	2464	rBV	371352	698080	94.40%	12.676%
51	9.223	2540	2545	2547	rBV2	454	455	0.06%	0.008%
52	9.297	2567	2568	2569	rBV2	207	69	0.01%	0.001%
53	9.442	2610	2613	2614	rBV	381	160	0.02%	0.003%
54	9.484	2624	2626	2629	rBV	160	53	0.01%	0.001%
55	9.500	2629	2631	2633	rBV2	165	48	0.01%	0.001%
56	9.526	2637	2639	2641	rBV	181	61	0.01%	0.001%
57	9.535	2641	2642	2643	rBV	202	65	0.01%	0.001%
58	9.609	2659	2665	2667	rBV2	354	355	0.05%	0.006%
59	9.680	2685	2687	2690	rBV2	422	222	0.03%	0.004%
60	9.809	2722	2727	2730	rBV	215	205	0.03%	0.004%
61	9.934	2763	2766	2767	rBV	147	81	0.01%	0.001%
62	9.944	2767	2769	2770	rBV	252	126	0.02%	0.002%
63	10.127	2819	2826	2834	rVB3	2510	3292	0.45%	0.060%
64	10.227	2843	2857	2877	rBV	186532	322152	43.56%	5.850%
65	10.397	2909	2910	2912	rBV	222	91	0.01%	0.002%
66	10.513	2944	2946	2949	rBV2	232	117	0.02%	0.002%
67	10.661	2989	2992	2996	rBV2	366	341	0.05%	0.006%
68	10.703	3001	3005	3007	rBV2	158	115	0.02%	0.002%
69	10.719	3007	3010	3012	rBV2	181	115	0.02%	0.002%
70	10.735	3013	3015	3016	rBV	209	70	0.01%	0.001%
71	10.831	3043	3045	3047	rBV	303	95	0.01%	0.002%
72	10.918	3066	3072	3081	rVB6	2384	3968	0.54%	0.072%
73	11.256	3165	3177	3200	rBV	418809	649186	87.79%	11.789%
74	11.629	3282	3293	3309	rBV	329408	523765	70.83%	9.511%
75	11.760	3332	3334	3336	rBV	232	100	0.01%	0.002%
76	11.789	3337	3343	3350	rVV6	1536	1941	0.26%	0.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022531.D
 Acq On : 03 Oct 2021 00:01
 Operator : SY/MD
 Sample : M3973-08ME
 Misc : 5.01g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8X4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

77	11.841	3353	3359	3360	rBV3	642	576	0.08%	0.010%
78	11.924	3383	3385	3387	rVB3	249	82	0.01%	0.001%
79	11.940	3387	3390	3392	rBV2	250	150	0.02%	0.003%
80	12.101	3435	3440	3443	rBV2	547	641	0.09%	0.012%
81	12.256	3486	3488	3494	rVB4	668	467	0.06%	0.008%
82	12.368	3522	3523	3525	rBV4	305	103	0.01%	0.002%
83	12.445	3546	3547	3552	rVB2	396	168	0.02%	0.003%
84	12.471	3552	3555	3558	rVB	369	217	0.03%	0.004%
85	12.680	3616	3620	3622	rBV2	330	256	0.03%	0.005%
86	12.773	3647	3649	3650	rBV	278	74	0.01%	0.001%
87	12.882	3680	3683	3689	rBV5	647	664	0.09%	0.012%
88	13.114	3753	3755	3759	rBV2	270	174	0.02%	0.003%
89	13.207	3782	3784	3787	rBV	266	152	0.02%	0.003%
90	13.493	3870	3873	3874	rBV	295	177	0.02%	0.003%
91	14.323	4128	4131	4135	rBV4	351	276	0.04%	0.005%
92	14.606	4213	4219	4220	rBV2	515	463	0.06%	0.008%




Sum of corrected areas: 5506940

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022531.D
Acq On : 03 Oct 2021 00:01
Operator : SY/MD
Sample : M3973-08ME
Misc : 5.01g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8X4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

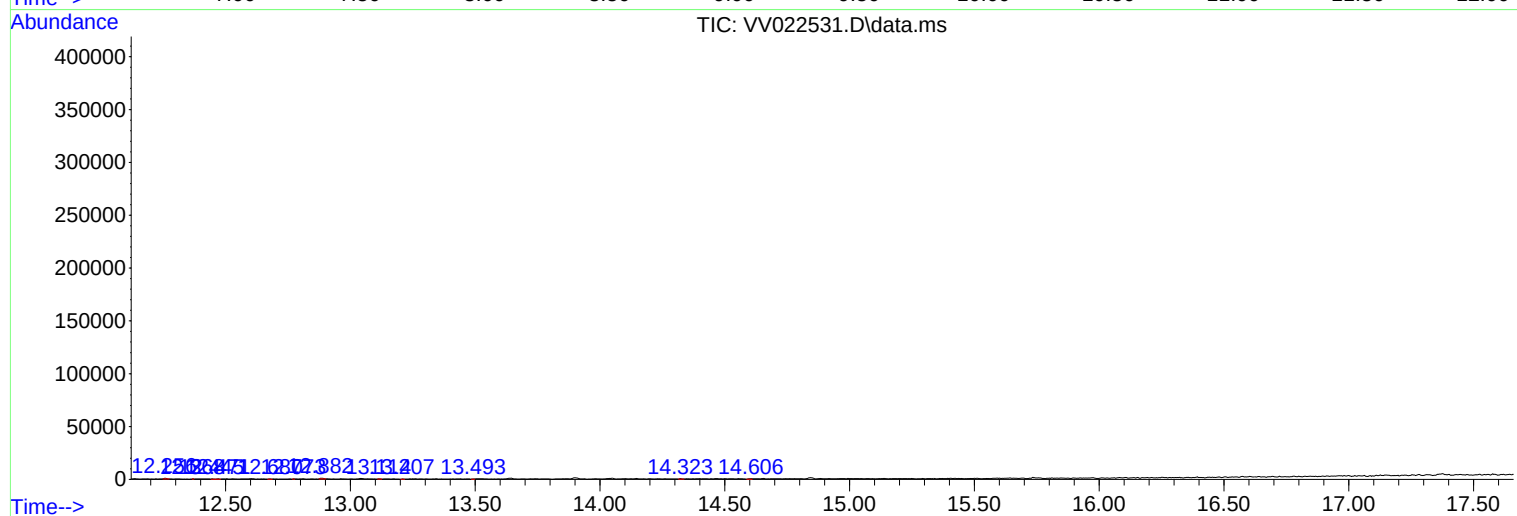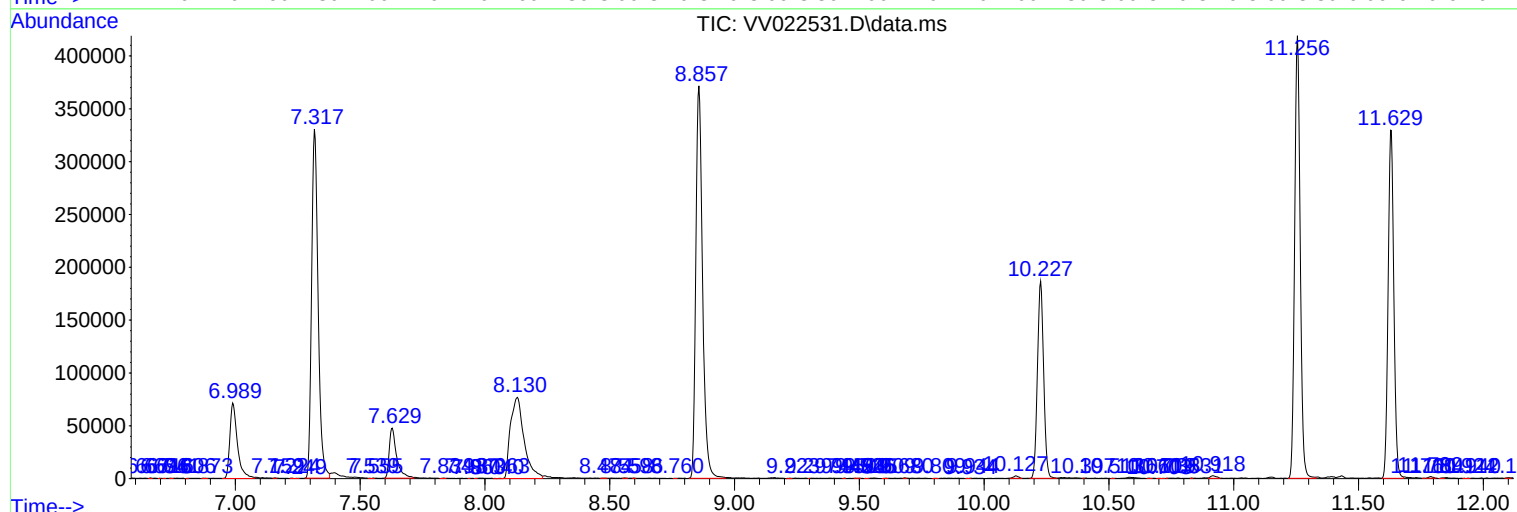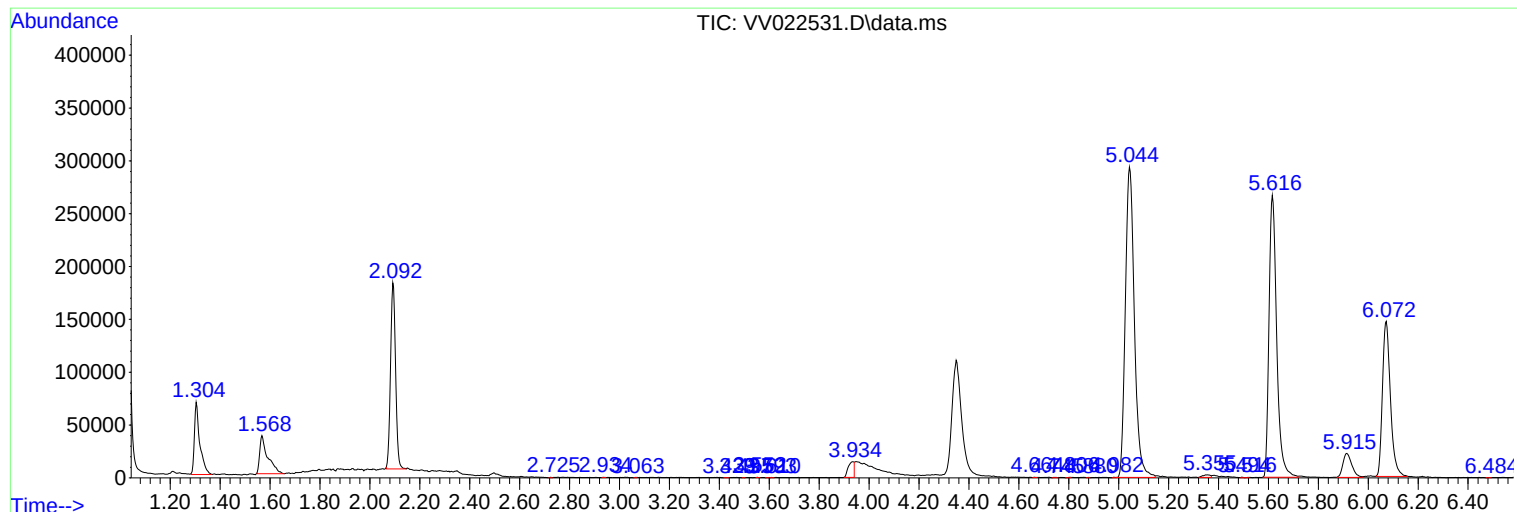

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022531.D
Acq On : 03 Oct 2021 00:01
Operator : SY/MD
Sample : M3973-08ME
Misc : 5.01g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8X4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022531.D
Acq On : 03 Oct 2021 00:01
Operator : SY/MD
Sample : M3973-08ME
Misc : 5.01g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8X4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc