

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022545.D
 Acq On : 03 Oct 2021 05:33
 Operator : SY/MD
 Sample : M3974-09ME 10X
 Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Z3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

Signal : TIC: VV022545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	112406	116258	13.95%	1.663%
2	1.564	157	163	174	rVB	87523	97739	11.73%	1.398%
3	2.101	321	330	350	rVB	188884	271180	32.55%	3.879%
4	2.780	538	541	543	rBV	303	201	0.02%	0.003%
5	2.931	584	588	591	rBV2	288	203	0.02%	0.003%
6	3.130	646	650	652	rBV2	266	236	0.03%	0.003%
7	3.175	658	664	667	rBV2	226	277	0.03%	0.004%
8	3.445	745	748	749	rBV	194	108	0.01%	0.002%
9	3.632	804	806	809	rVB2	219	83	0.01%	0.001%
10	3.754	841	844	845	rBV	402	180	0.02%	0.003%
11	3.854	873	875	877	rBV2	161	53	0.01%	0.001%
12	3.899	879	889	920	rBV2	45807	156149	18.74%	2.234%
13	4.349	1016	1029	1050	rVB	130771	317890	38.16%	4.547%
14	4.593	1104	1105	1107	rBV	334	168	0.02%	0.002%
15	4.674	1128	1130	1131	rBV	314	132	0.02%	0.002%
16	4.870	1187	1191	1195	rVB2	376	277	0.03%	0.004%
17	4.892	1195	1198	1200	rBV2	193	132	0.02%	0.002%
18	4.947	1212	1215	1221	rVB2	352	357	0.04%	0.005%
19	4.976	1221	1224	1226	rBV	211	148	0.02%	0.002%
20	5.043	1229	1245	1280	rBV2	334965	833108	100.00%	11.918%
21	5.330	1332	1334	1338	rBV2	392	304	0.04%	0.004%
22	5.397	1354	1355	1356	rBV2	389	103	0.01%	0.001%
23	5.426	1363	1364	1366	rVB	162	57	0.01%	0.001%
24	5.503	1384	1388	1390	rBV3	298	169	0.02%	0.002%
25	5.616	1411	1423	1455	rBV	331540	671956	80.66%	9.612%
26	5.915	1503	1516	1538	rBV3	94879	196508	23.59%	2.811%
27	6.072	1552	1565	1590	rBV	179546	371195	44.56%	5.310%
28	6.265	1623	1625	1628	rVB4	295	118	0.01%	0.002%
29	6.281	1628	1630	1632	rBV2	326	130	0.02%	0.002%
30	6.371	1655	1658	1659	rBV	381	159	0.02%	0.002%
31	6.423	1672	1674	1675	rBV	177	57	0.01%	0.001%
32	6.477	1687	1691	1694	rVB2	258	153	0.02%	0.002%
33	6.516	1702	1703	1704	rBV2	216	75	0.01%	0.001%
34	6.555	1713	1715	1719	rVB3	345	149	0.02%	0.002%
35	6.583	1719	1724	1726	rBV	244	193	0.02%	0.003%
36	6.609	1731	1732	1735	rVB	291	85	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100221\
 Data File : VW022545.D
 Acq On : 03 Oct 2021 05:33
 Operator : SY/MD
 Sample : M3974-09ME 10X
 Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Z3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	6.683	1747	1755	1764	rBV6	2018	3897	0.47%	0.056%
38	6.834	1801	1802	1806	rVB2	235	116	0.01%	0.002%
39	6.989	1839	1850	1872	rBV	92124	170281	20.44%	2.436%
40	7.172	1905	1907	1910	rBV	357	166	0.02%	0.002%
41	7.317	1940	1952	1971	rBV	396932	686186	82.36%	9.816%
42	7.625	2038	2048	2076	rBV	60393	110508	13.26%	1.581%
43	7.764	2090	2091	2095	rVB2	417	198	0.02%	0.003%
44	7.786	2095	2098	2100	rBV2	283	205	0.02%	0.003%
45	7.802	2100	2103	2105	rVB	443	205	0.02%	0.003%
46	7.857	2118	2120	2123	rBV	217	98	0.01%	0.001%
47	7.911	2131	2137	2138	rBV2	221	206	0.02%	0.003%
48	7.989	2156	2161	2163	rBV3	402	392	0.05%	0.006%
49	8.037	2174	2176	2178	rBV3	268	113	0.01%	0.002%
50	8.095	2184	2194	2233	rBV	165433	374836	44.99%	5.362%
51	8.567	2338	2341	2344	rBV2	259	197	0.02%	0.003%
52	8.622	2355	2358	2360	rBV	276	141	0.02%	0.002%
53	8.641	2360	2364	2365	rBV2	427	269	0.03%	0.004%
54	8.677	2372	2375	2385	rVB3	361	442	0.05%	0.006%
55	8.747	2391	2397	2400	rBV2	268	293	0.04%	0.004%
56	8.853	2418	2430	2464	rBV	491525	797594	95.74%	11.410%
57	9.101	2501	2507	2510	rBV2	341	317	0.04%	0.005%
58	9.127	2512	2515	2518	rVV	319	284	0.03%	0.004%
59	9.146	2518	2521	2533	rVV4	835	1240	0.15%	0.018%
60	9.233	2545	2548	2556	rBV2	153	193	0.02%	0.003%
61	9.323	2574	2576	2577	rBV2	225	104	0.01%	0.001%
62	9.368	2586	2590	2596	rVB2	218	271	0.03%	0.004%
63	9.394	2596	2598	2599	rBV2	236	79	0.01%	0.001%
64	9.554	2644	2648	2652	rBV2	666	600	0.07%	0.009%
65	9.667	2681	2683	2685	rBV2	149	63	0.01%	0.001%
66	9.940	2763	2768	2773	rBV2	297	429	0.05%	0.006%
67	10.001	2785	2787	2790	rVB	238	87	0.01%	0.001%
68	10.127	2819	2826	2834	rBV4	2090	2757	0.33%	0.039%
69	10.217	2842	2854	2874	rBV	236456	386889	46.44%	5.534%
70	10.426	2917	2919	2922	rBV	182	59	0.01%	0.001%
71	10.448	2923	2926	2928	rBV2	295	171	0.02%	0.002%
72	10.542	2949	2955	2957	rBV3	736	675	0.08%	0.010%
73	10.606	2971	2975	2979	rVB3	565	402	0.05%	0.006%
74	10.921	3064	3073	3086	rVB6	2266	3715	0.45%	0.053%
75	11.030	3105	3107	3109	rBV	273	146	0.02%	0.002%
76	11.098	3123	3128	3135	rVB3	433	507	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022545.D
 Acq On : 03 Oct 2021 05:33
 Operator : SY/MD
 Sample : M3974-09ME 10X
 Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Z3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.252	3164	3176	3193	rBV	505124	773406	92.83%	11.064%
78	11.413	3224	3226	3227	rBV2	714	308	0.04%	0.004%
79	11.532	3256	3263	3265	rBV3	1693	1613	0.19%	0.023%
80	11.625	3281	3292	3314	rBV	390041	613151	73.60%	8.771%
81	11.747	3328	3330	3331	rVB	370	85	0.01%	0.001%
82	11.837	3356	3358	3361	rBV2	249	138	0.02%	0.002%
83	11.876	3368	3370	3374	rBV2	198	84	0.01%	0.001%
84	12.024	3411	3416	3421	rVB3	719	849	0.10%	0.012%
85	12.120	3437	3446	3450	rBV5	1971	2673	0.32%	0.038%
86	12.320	3503	3508	3510	rBV2	468	376	0.05%	0.005%
87	12.558	3581	3582	3583	rVB	307	59	0.01%	0.001%
88	12.590	3590	3592	3594	rBV	556	321	0.04%	0.005%
89	12.651	3607	3611	3612	rBV2	536	345	0.04%	0.005%
90	12.689	3621	3623	3624	rBV2	273	87	0.01%	0.001%
91	12.734	3631	3637	3645	rVB4	899	1273	0.15%	0.018%
92	12.767	3645	3647	3650	rBV2	388	259	0.03%	0.004%
93	12.885	3677	3684	3696	rVB7	4906	7410	0.89%	0.106%
94	13.246	3793	3796	3797	rBV	181	77	0.01%	0.001%
95	13.271	3801	3804	3809	rVB4	604	606	0.07%	0.009%
96	13.455	3859	3861	3864	rBV2	221	113	0.01%	0.002%
97	13.628	3909	3915	3918	rBV3	838	819	0.10%	0.012%
98	13.725	3943	3945	3947	rBV	415	186	0.02%	0.003%
99	13.969	4019	4021	4024	rBV	216	127	0.02%	0.002%
100	14.824	4279	4287	4299	rVB6	2446	4541	0.55%	0.065%

Sum of corrected areas: 6990527




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022545.D
Acq On : 03 Oct 2021 05:33
Operator : SY/MD
Sample : M3974-09ME 10X
Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8Z3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

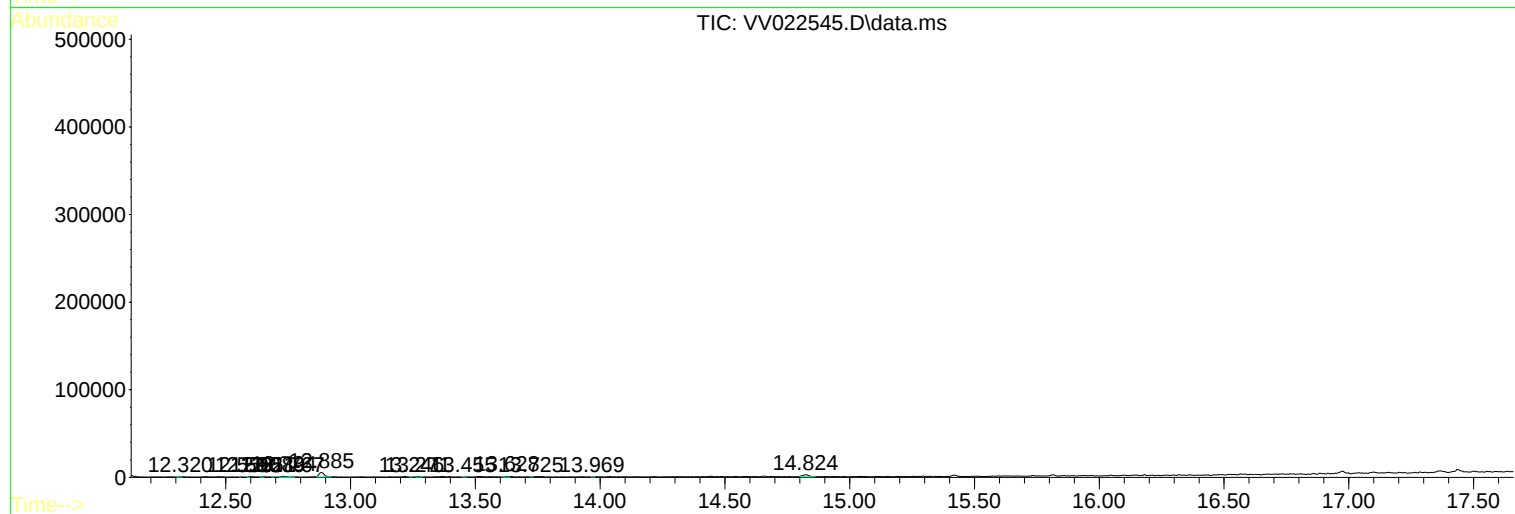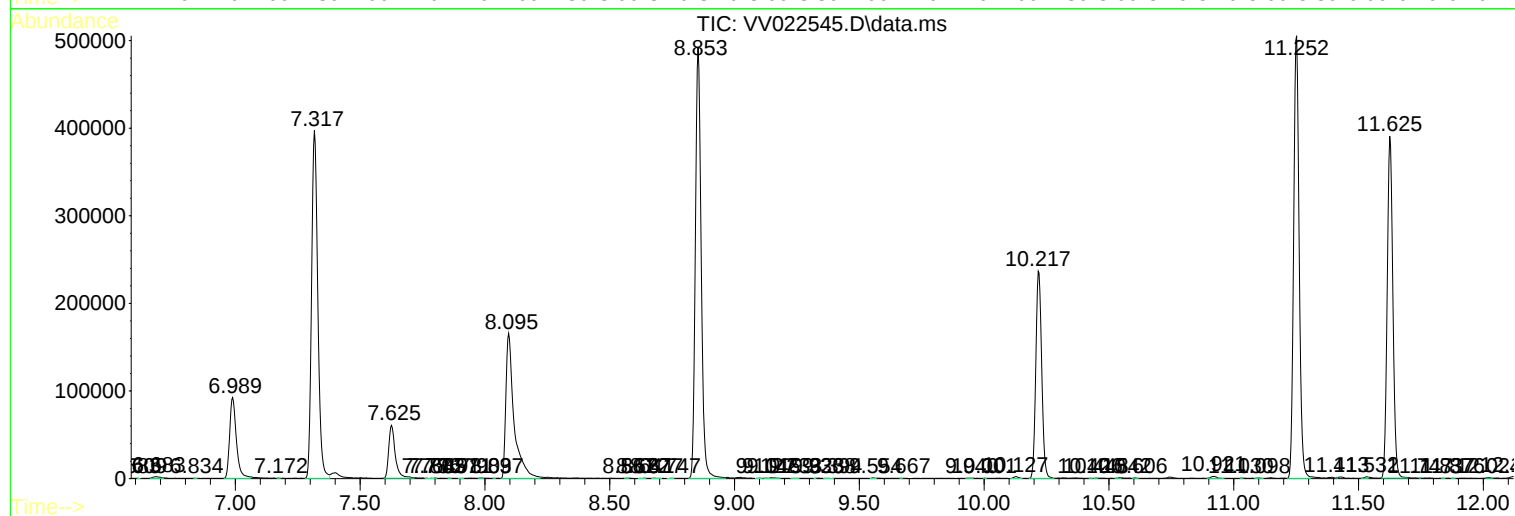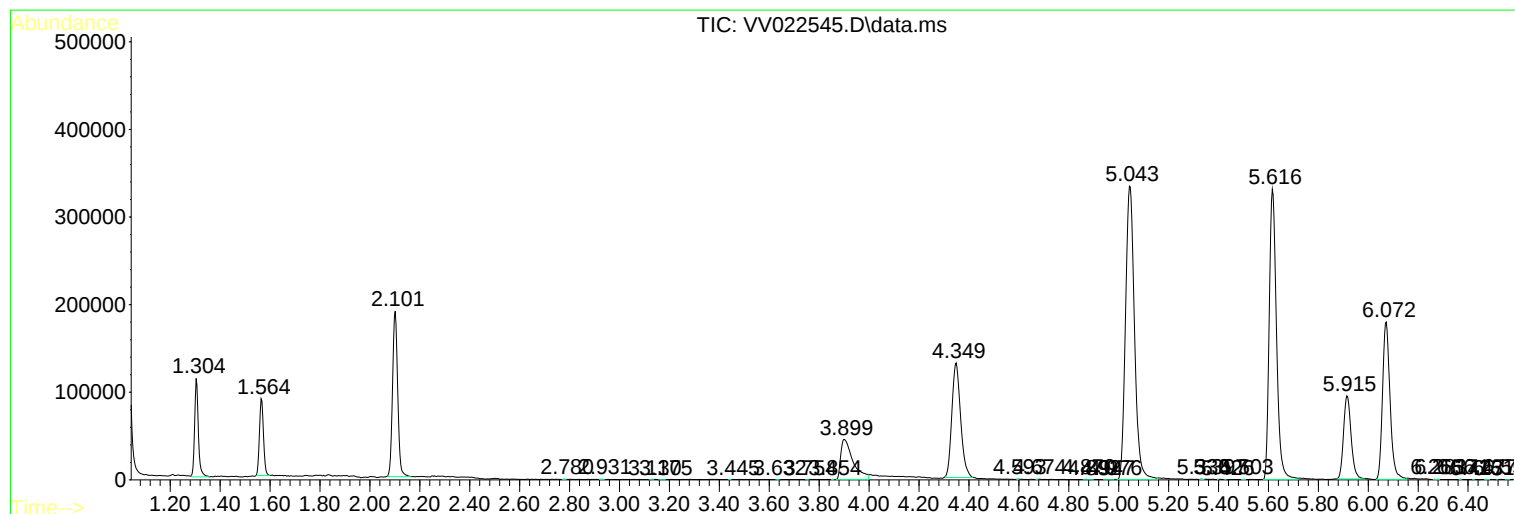

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022545.D
Acq On : 03 Oct 2021 05:33
Operator : SY/MD
Sample : M3974-09ME 10X
Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8Z3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022545.D
Acq On : 03 Oct 2021 05:33
Operator : SY/MD
Sample : M3974-09ME 10X
Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8Z3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
