


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022502.D
Acq On : 02 Oct 2021 10:45
Operator : SY/MD
Sample : BFB240
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB240

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Title : VOC Analysis
Last Update : Wed Oct 13 01:15:35 2021

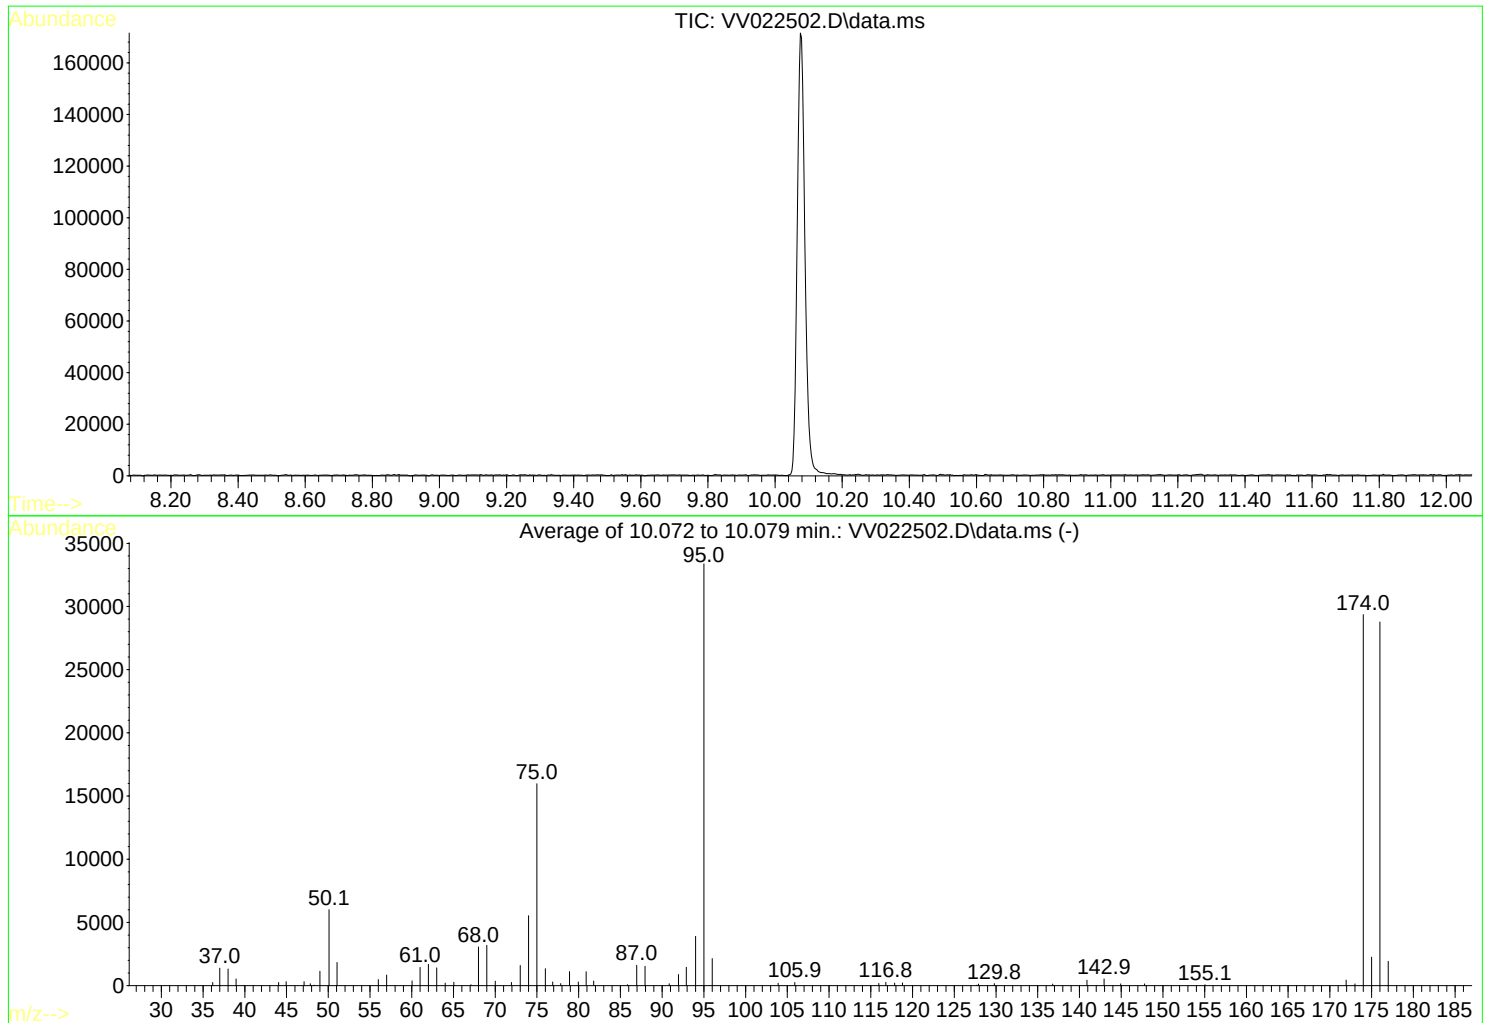

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	6008	PASS
75	95	30	80	47.9	15981	PASS
95	95	100	100	100.0	33376	PASS
96	95	5	9	6.4	2141	PASS
173	174	0.00	2	0.5	137	PASS
174	95	50	120	88.0	29360	PASS
175	174	5	9	7.7	2259	PASS
176	174	95	105	98.0	28773	PASS
177	176	5	10	6.7	1930	PASS

Scan 2799 (10.040 min): VV022502.D\data.ms
BFB240

m/z	Abundance
35.30	102.0
39.90	146.0
44.10	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
36.10	225.0
37.00	1283.0
38.00	1278.0
38.90	469.0
39.90	173.0
44.00	316.0
44.90	308.0
47.10	318.0
47.80	155.0
49.00	1102.0
50.10	5911.0
51.10	1761.0
56.00	429.0
57.00	798.0
60.10	376.0
61.00	1486.0
62.00	1610.0
63.00	1400.0
64.00	213.0
65.00	249.0
68.00	2949.0
69.00	3128.0
70.00	312.0
72.00	238.0
73.00	1550.0
74.00	5278.0
75.00	15218.0
76.00	1438.0
76.90	285.0
77.90	152.0
78.90	1012.0
80.00	331.0
80.90	1077.0
81.80	335.0
85.90	111.0
87.00	1395.0
87.90	1464.0
90.80	146.0
92.00	833.0
92.90	1301.0
94.00	3600.0
95.00	32120.0
96.00	2142.0
104.00	199.0
105.90	246.0
115.90	147.0
116.80	271.0
117.90	217.0
118.80	210.0
127.70	131.0
129.80	143.0
136.80	123.0
140.90	379.0
142.90	516.0
145.00	153.0
147.80	122.0
155.10	108.0
172.00	419.0
173.00	410.0
174.00	27344.0
175.00	2244.0
176.00	26424.0
177.00	1908.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
36.10	270.0
37.00	1417.0
38.00	1365.0
38.90	544.0
39.90	179.0
44.00	375.0
44.90	334.0
47.10	343.0
47.80	143.0
49.00	1146.0
50.10	6266.0
51.10	1906.0
56.00	497.0
57.00	855.0
60.00	366.0
61.00	1457.0
62.00	1724.0
63.00	1433.0
64.00	211.0
65.00	251.0
67.10	107.0
68.00	3132.0
69.00	3271.0
70.00	364.0
72.00	267.0
73.00	1648.0
74.00	5706.0
75.00	16456.0
76.00	1374.0
76.90	305.0
77.90	176.0
78.90	1132.0
79.90	282.0
80.90	1107.0
81.80	379.0
85.80	104.0
87.00	1648.0
88.00	1577.0
90.90	168.0
91.90	876.0
92.90	1534.0
94.00	4024.0
95.00	34480.0
96.00	2227.0
103.90	177.0
105.90	274.0
116.00	188.0
116.80	270.0
117.90	205.0
118.80	228.0
127.90	183.0
129.80	173.0
136.80	136.0
140.90	465.0
142.90	546.0
145.00	150.0
147.80	150.0
155.00	113.0
172.00	438.0
174.00	30360.0
175.00	2344.0
176.00	29744.0
177.00	1984.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
36.20	282.0
37.00	1432.0
38.00	1325.0
39.00	589.0
39.90	164.0
44.10	432.0
45.00	318.0
47.10	286.0
47.90	141.0
48.30	117.0
49.00	1154.0
50.10	5847.0
51.00	1854.0
56.00	536.0
57.00	866.0
60.00	379.0
61.00	1402.0
62.00	1739.0
63.00	1380.0
64.00	192.0
65.10	306.0
67.10	123.0
68.00	3131.0
69.00	3174.0
70.00	380.0
71.90	265.0
73.00	1594.0
74.00	5604.0
75.00	16269.0
76.00	1229.0
76.90	275.0
77.80	177.0
78.90	1203.0
80.00	254.0
80.90	1134.0
81.80	387.0
86.90	1802.0
88.00	1544.0
90.90	154.0
91.90	911.0
92.90	1553.0
94.00	4070.0
95.00	33528.0
96.00	2055.0
103.80	183.0
105.90	250.0
115.90	212.0
116.80	255.0
117.80	176.0
118.80	220.0
127.90	184.0
129.80	189.0
136.80	117.0
140.90	451.0
143.00	526.0
144.90	129.0
147.80	135.0
171.90	457.0
174.00	30376.0
175.00	2188.0
176.00	30152.0
177.00	1898.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240