

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032203.D
 Acq On : 02 Oct 2023 16:59
 Operator : SY/MD
 Sample : 04592-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 03 02:01:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 03 01:57:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	211042	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	199820	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	99706	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	44244	33.877	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	67.760%		
7) Chloroethane-d5	1.529	69	42345	37.590	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	75.180%		
11) 1,1-Dichloroethene-d2	2.060	65	19908	34.908	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.820%		
21) 2-Butanone-d5	3.786	46	116876	99.524	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	99.520%		
24) Chloroform-d	4.253	84	110616	40.474	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.940%		
26) 1,2-Dichloroethane-d4	4.947	65	70394	42.808	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.620%		
32) Benzene-d6	4.963	84	205085	39.042	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	78.080%		
36) 1,2-Dichloropropane-d6	5.992	67	75838	43.264	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	86.520%		
41) Toluene-d8	7.246	98	173815	36.271	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	72.540%#		
43) trans-1,3-Dichloroprop...	7.558	79	30081	36.072	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	72.140%		
47) 2-Hexanone-d5	8.027	63	68569	90.583	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	90.580%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	115082	46.159	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.320%		
66) 1,2-Dichlorobenzene-d4	11.564	152	79817	44.143	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.280%		
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.188	75	12870	6.640	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032203.D
Acq On : 02 Oct 2023 16:59
Operator : SY/MD
Sample : 04592-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 03 02:01:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 03 01:57:58 2023
Response via : Initial Calibration

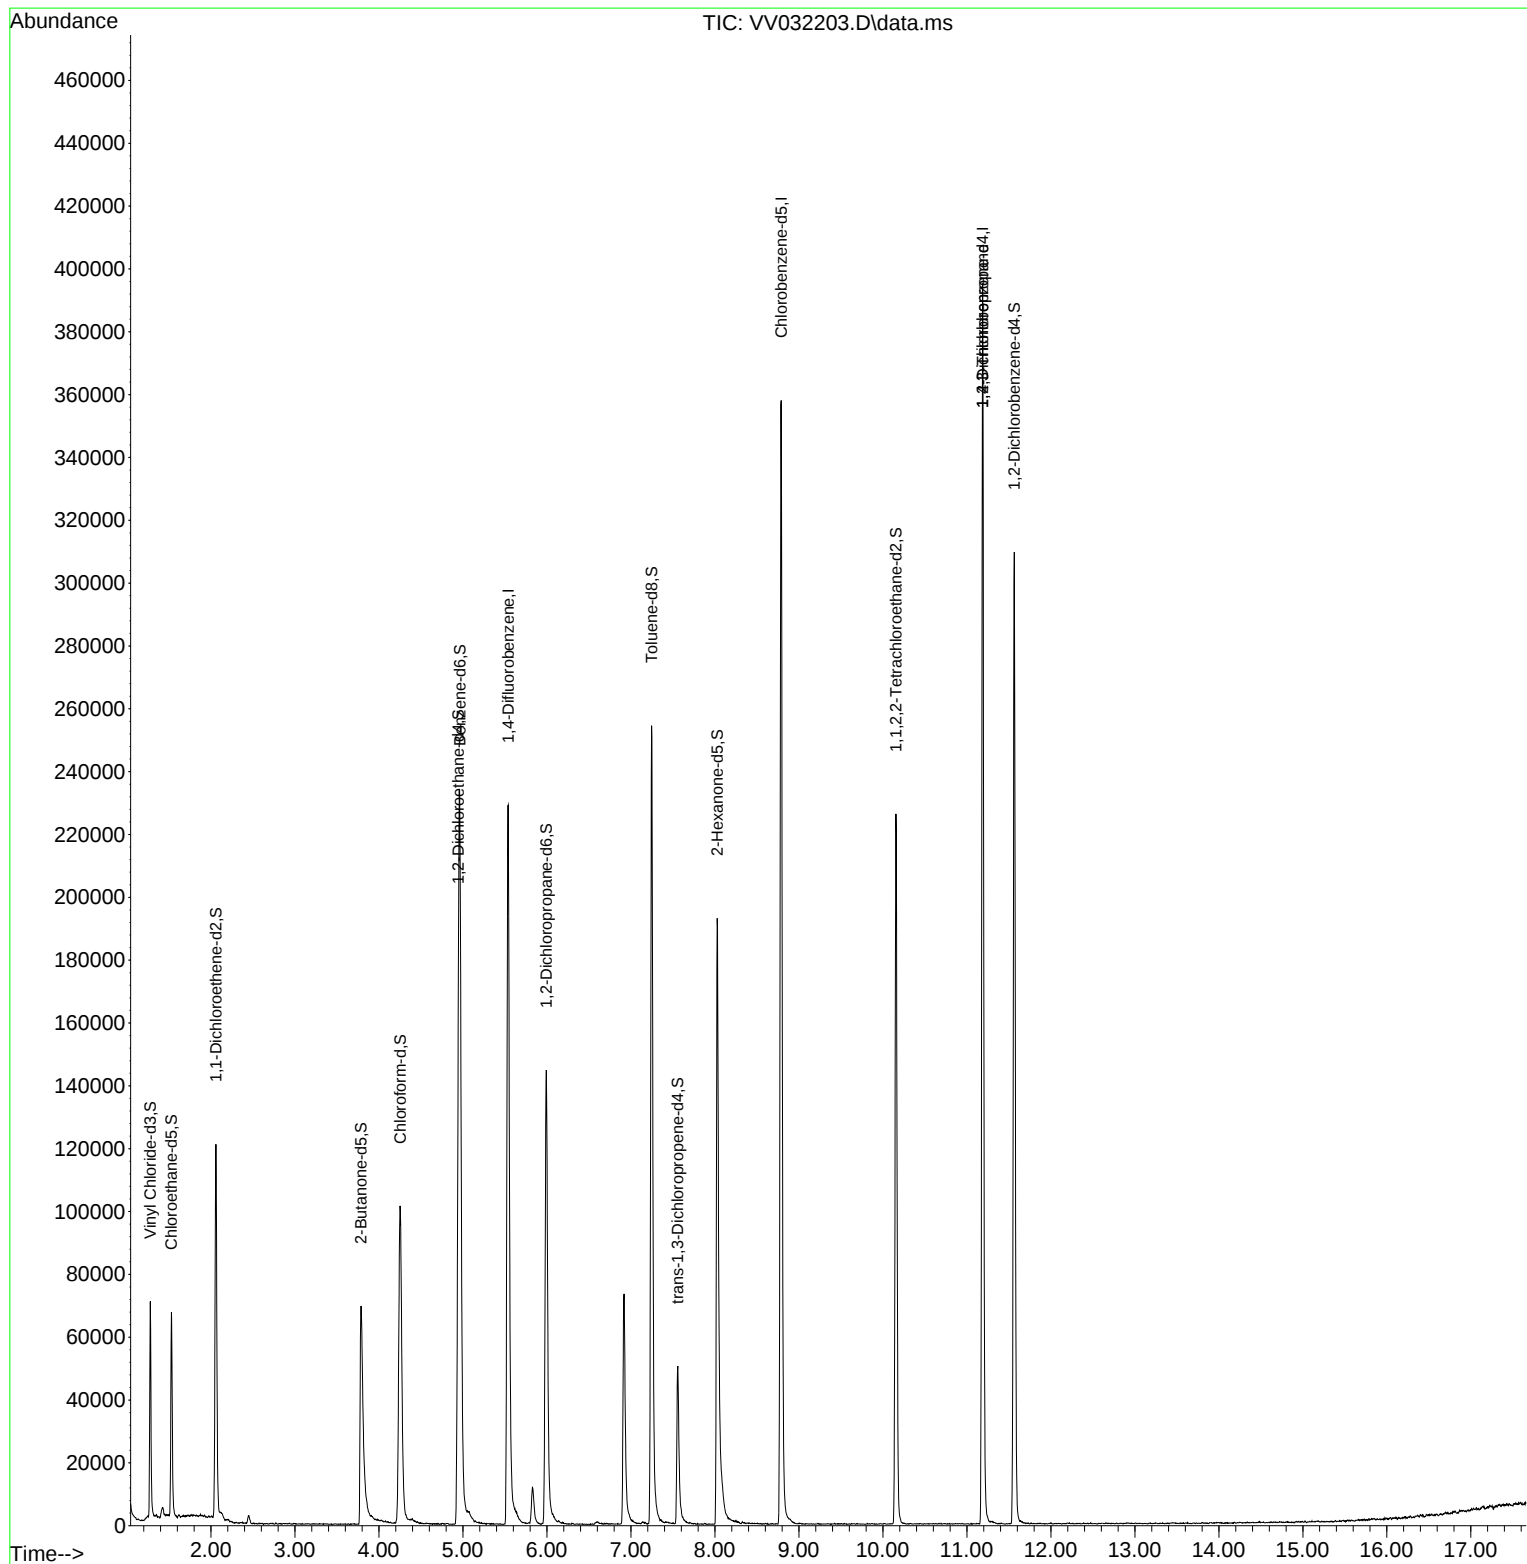

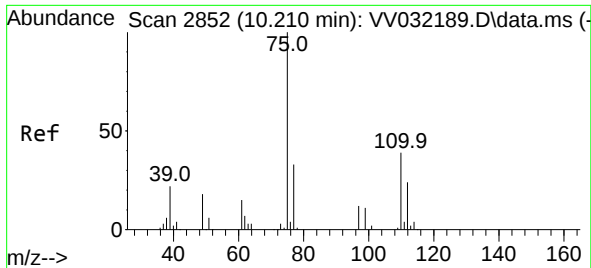

#61

1,2,3-Trichloropropane

Concen: 6.640 ug/L

RT: 11.188 min Scan# 31

Delta R.T. 0.977 min


Lab File: VV032203.D

Acq: 02 Oct 2023 16:59

Instrument :

MSVOA_V

ClientSampleId :

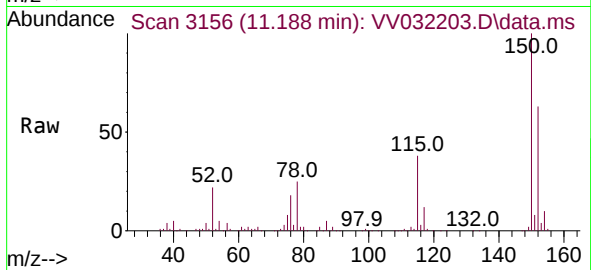

Tgt Ion: 75 Resp: 12870

Ion Ratio Lower Upper

75 100

77 31.6 26.1 39.1

110 2.4 30.5 45.7#

