

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100223\
 Data File : VW032200.D
 Acq On : 02 Oct 2023 14:22
 Operator : SY/MD
 Sample : 04592-05 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYY3

Quant Time: Oct 03 02:00:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 03 01:57:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	219889	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	215989	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	107944	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	51281	37.685	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.360%
7) Chloroethane-d5	1.532	69	48435	41.266	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.540%
11) 1,1-Dichloroethene-d2	2.060	65	22890	38.522	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.040%
21) 2-Butanone-d5	3.789	46	113337	92.628	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.630%
24) Chloroform-d	4.252	84	105161	36.930	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	73.860%
26) 1,2-Dichloroethane-d4	4.944	65	74923	43.729	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.460%
32) Benzene-d6	4.963	84	229896	40.489	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.980%
36) 1,2-Dichloropropane-d6	5.992	67	81482	43.004	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.000%
41) Toluene-d8	7.246	98	200861	38.777	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	77.560%#
43) trans-1,3-Dichloroprop...	7.558	79	34217	37.960	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.920%
47) 2-Hexanone-d5	8.027	63	65843	80.470	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	80.470%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	88210	32.732	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	65.460%
66) 1,2-Dichlorobenzene-d4	11.564	152	84087	42.956	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.920%
Target Compounds						
					Qvalue	
25) Chloroform	4.285	83	12815	4.170	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032200.D
Acq On : 02 Oct 2023 14:22
Operator : SY/MD
Sample : 04592-05 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY3

Quant Time: Oct 03 02:00:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 03 01:57:58 2023
Response via : Initial Calibration

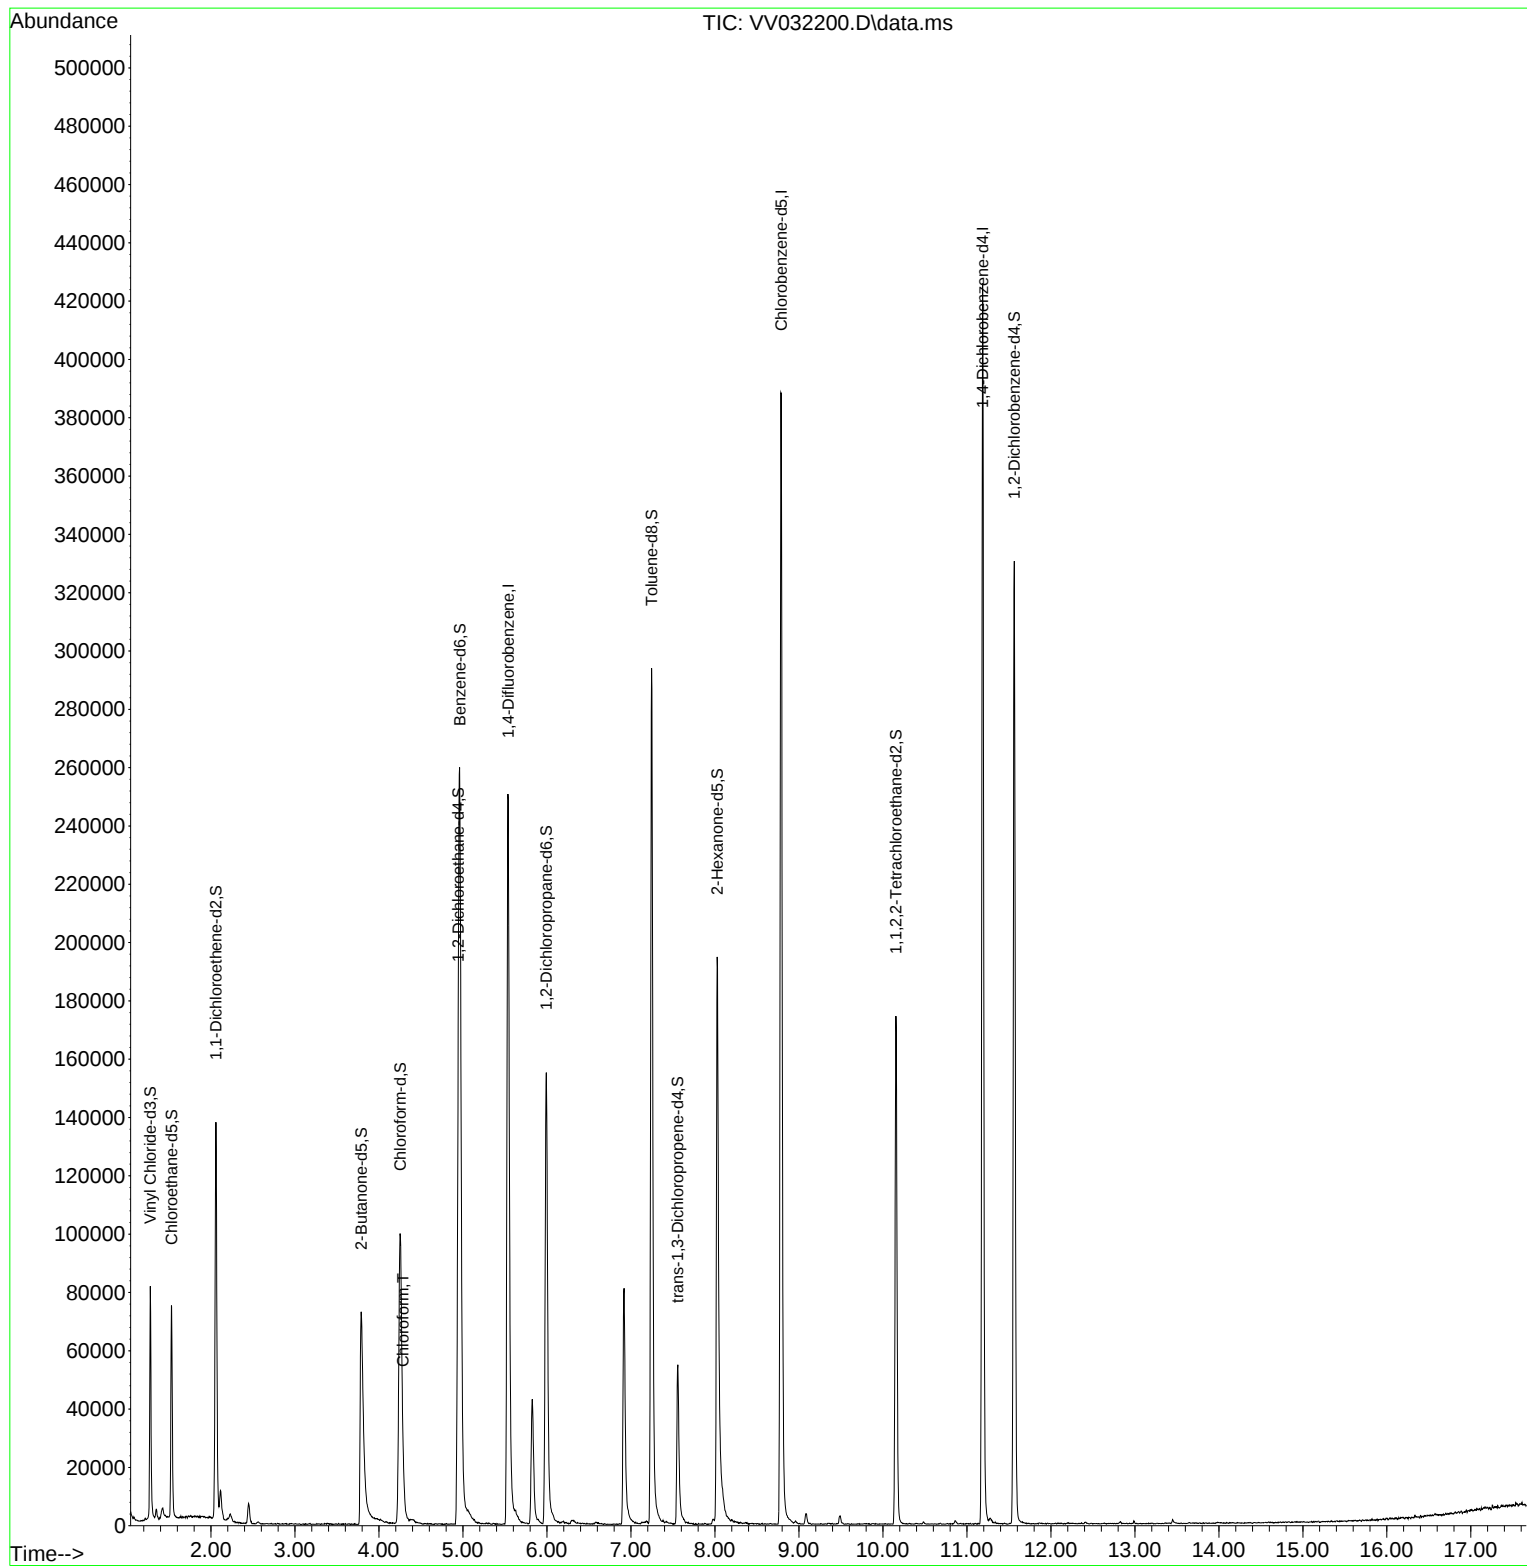

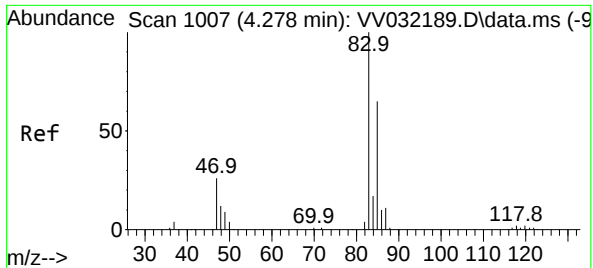

#25
 Chloroform
 Concen: 4.170 ug/L
 RT: 4.285 min Scan# 10
 Delta R.T. 0.006 min
 Lab File: VV032200.D
 Acq: 02 Oct 2023 14:22

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYY3

Tgt Ion: 83 Resp: 12815
 Ion Ratio Lower Upper
 83 100
 85 68.3 45.6 84.6

