

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032191.D
 Acq On : 02 Oct 2023 10:50
 Operator : SY/MD
 Sample : VV1002WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK203

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

Signal : TIC: VV032191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rBV	86117	90246	12.21%	1.508%
2	1.532	145	153	171	rVB	78846	96424	13.05%	1.611%
3	2.060	307	317	331	rBV	148964	214206	28.98%	3.579%
4	2.343	401	405	406	rBV2	265	158	0.02%	0.003%
5	2.375	412	415	417	rBV	275	205	0.03%	0.003%
6	2.388	417	419	425	rVV3	327	215	0.03%	0.004%
7	2.449	431	438	449	rVB5	1844	3065	0.41%	0.051%
8	2.523	458	461	462	rBV2	230	108	0.01%	0.002%
9	2.552	467	470	474	rBV2	167	157	0.02%	0.003%
10	2.587	479	481	484	rBV	220	134	0.02%	0.002%
11	2.690	510	513	514	rBV	309	111	0.02%	0.002%
12	2.745	528	530	535	rBV	240	166	0.02%	0.003%
13	3.288	696	699	702	rBV2	166	136	0.02%	0.002%
14	3.352	714	719	720	rBV	166	125	0.02%	0.002%
15	3.700	823	827	832	rBV	215	248	0.03%	0.004%
16	3.786	844	854	888	rBV	63752	174881	23.66%	2.922%
17	4.249	981	998	1028	rBV	115712	301237	40.76%	5.033%
18	4.484	1068	1071	1072	rBV	324	199	0.03%	0.003%
19	4.606	1107	1109	1112	rBV	227	108	0.01%	0.002%
20	4.654	1122	1124	1128	rVB3	321	160	0.02%	0.003%
21	4.674	1128	1130	1134	rBV2	318	198	0.03%	0.003%
22	4.725	1142	1146	1151	rVB2	192	160	0.02%	0.003%
23	4.854	1181	1186	1189	rVB2	291	221	0.03%	0.004%
24	4.957	1202	1218	1246	rBV2	277145	739135	100.00%	12.350%
25	5.214	1295	1298	1301	rVB2	348	189	0.03%	0.003%
26	5.281	1316	1319	1324	rVV3	215	190	0.03%	0.003%
27	5.333	1332	1335	1336	rVV	172	113	0.02%	0.002%
28	5.407	1355	1358	1363	rVB2	303	240	0.03%	0.004%
29	5.439	1363	1368	1372	rBV2	244	189	0.03%	0.003%
30	5.535	1386	1398	1427	rBV	246362	513921	69.53%	8.587%
31	5.773	1468	1472	1475	rBV2	200	154	0.02%	0.003%
32	5.828	1478	1489	1507	rVV2	12783	26232	3.55%	0.438%
33	5.918	1512	1517	1521	rVB3	251	247	0.03%	0.004%
34	5.941	1521	1524	1526	rBV2	211	130	0.02%	0.002%
35	5.992	1526	1540	1571	rBV	165516	358455	48.50%	5.989%
36	6.227	1610	1613	1616	rVB3	388	263	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032191.D
 Acq On : 02 Oct 2023 10:50
 Operator : SY/MD
 Sample : VV1002WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK203

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

37	6.246	1616	1619	1621	rBV2	158	120	0.02%	0.002%
38	6.297	1633	1635	1641	rBV2	282	187	0.03%	0.003%
39	6.587	1719	1725	1727	rBV3	743	748	0.10%	0.012%
40	6.645	1741	1743	1747	rVB2	437	183	0.02%	0.003%
41	6.680	1751	1754	1757	rVV	394	279	0.04%	0.005%
42	6.735	1767	1771	1776	rBV3	281	309	0.04%	0.005%
43	6.915	1816	1827	1846	rBV	89020	168412	22.79%	2.814%
44	7.124	1888	1892	1893	rBV	393	289	0.04%	0.005%
45	7.246	1917	1930	1954	rBV	321476	580292	78.51%	9.696%
46	7.555	2017	2026	2049	rBV	60775	112665	15.24%	1.883%
47	7.725	2077	2079	2081	rVB2	276	118	0.02%	0.002%
48	7.760	2087	2090	2091	rBV2	222	122	0.02%	0.002%
49	7.793	2096	2100	2102	rBV2	269	192	0.03%	0.003%
50	7.886	2127	2129	2132	rVB	251	121	0.02%	0.002%
51	8.027	2164	2173	2208	rBV	181226	362465	49.04%	6.056%
52	8.375	2279	2281	2286	rVB2	363	233	0.03%	0.004%
53	8.558	2336	2338	2340	rBV	212	118	0.02%	0.002%
54	8.629	2354	2360	2363	rBV3	357	296	0.04%	0.005%
55	8.696	2377	2381	2382	rBV2	194	110	0.01%	0.002%
56	8.715	2386	2387	2391	rVB2	254	126	0.02%	0.002%
57	8.786	2398	2409	2433	rBV	377253	631869	85.49%	10.558%
58	9.037	2483	2487	2490	rVB2	270	212	0.03%	0.004%
59	9.092	2501	2504	2507	rVB2	190	134	0.02%	0.002%
60	9.156	2519	2524	2525	rBV	198	153	0.02%	0.003%
61	9.320	2570	2575	2579	rBV	143	160	0.02%	0.003%
62	9.445	2611	2614	2619	rBV	139	148	0.02%	0.002%
63	9.487	2620	2627	2628	rBV2	198	213	0.03%	0.004%
64	9.558	2644	2649	2653	rBV2	310	272	0.04%	0.005%
65	9.802	2721	2725	2726	rBV2	151	110	0.01%	0.002%
66	9.873	2744	2747	2749	rBV2	154	117	0.02%	0.002%
67	9.989	2781	2783	2788	rVB	189	124	0.02%	0.002%
68	10.069	2804	2808	2810	rBV	149	115	0.02%	0.002%
69	10.156	2822	2835	2856	rBV	234034	372156	50.35%	6.218%
70	10.249	2862	2864	2867	rVB2	371	189	0.03%	0.003%
71	10.336	2885	2891	2894	rBV2	272	310	0.04%	0.005%
72	10.423	2915	2918	2921	rBV	309	166	0.02%	0.003%
73	10.619	2974	2979	2984	rBV	166	204	0.03%	0.003%
74	10.670	2992	2995	2999	rBV	157	155	0.02%	0.003%
75	10.866	3054	3056	3064	rVB3	305	258	0.03%	0.004%
76	11.130	3135	3138	3143	rVB3	387	302	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032191.D
 Acq On : 02 Oct 2023 10:50
 Operator : SY/MD
 Sample : VV1002WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK203

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

77	11.188	3144	3156	3180	rBV	418486	646656	87.49%	10.805%
78	11.561	3258	3272	3294	rBV	360364	570592	77.20%	9.534%
79	11.690	3310	3312	3316	rVB	688	402	0.05%	0.007%
80	11.712	3316	3319	3321	rBV2	234	179	0.02%	0.003%
81	11.738	3325	3327	3329	rBV	188	135	0.02%	0.002%
82	12.101	3437	3440	3444	rBV2	149	164	0.02%	0.003%
83	12.156	3454	3457	3461	rBV	188	162	0.02%	0.003%
84	12.194	3466	3469	3472	rVB2	247	164	0.02%	0.003%
85	12.593	3590	3593	3598	rBV2	321	258	0.03%	0.004%
86	13.034	3727	3730	3736	rBV2	286	279	0.04%	0.005%
87	13.207	3779	3784	3791	rVB3	567	729	0.10%	0.012%
88	13.452	3852	3860	3869	rBV2	3465	5334	0.72%	0.089%
89	13.503	3873	3876	3878	rBV2	230	161	0.02%	0.003%
90	13.580	3897	3900	3905	rVB3	362	341	0.05%	0.006%
91	13.625	3911	3914	3920	rVB	305	231	0.03%	0.004%
92	13.786	3962	3964	3967	rVB2	265	127	0.02%	0.002%
93	13.805	3967	3970	3972	rBV	310	167	0.02%	0.003%
94	13.943	4010	4013	4015	rVB	372	228	0.03%	0.004%
95	13.969	4015	4021	4023	rBV3	417	400	0.05%	0.007%
96	14.050	4042	4046	4047	rBV	290	156	0.02%	0.003%
97	14.291	4120	4121	4128	rBV2	204	183	0.02%	0.003%
98	14.497	4183	4185	4188	rBV2	282	161	0.02%	0.003%
99	15.201	4402	4404	4406	rBV2	406	246	0.03%	0.004%
100	15.448	4478	4481	4482	rBV2	563	320	0.04%	0.005%




Sum of corrected areas: 5984853

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032191.D
Acq On : 02 Oct 2023 10:50
Operator : SY/MD
Sample : VV1002WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK203

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

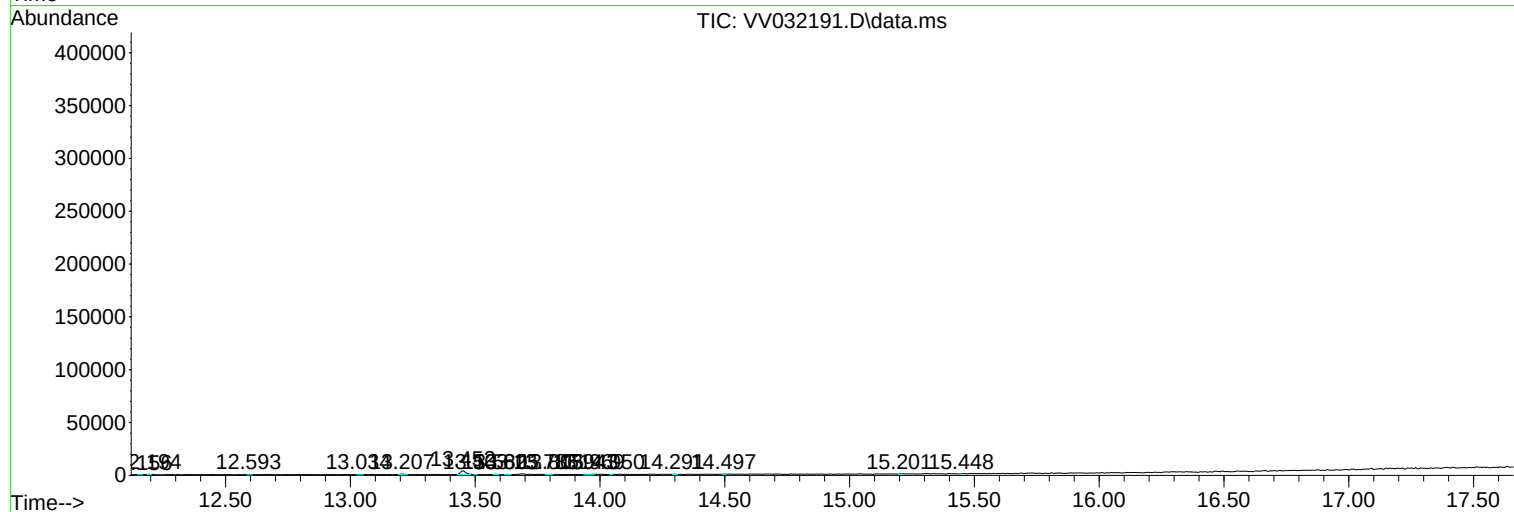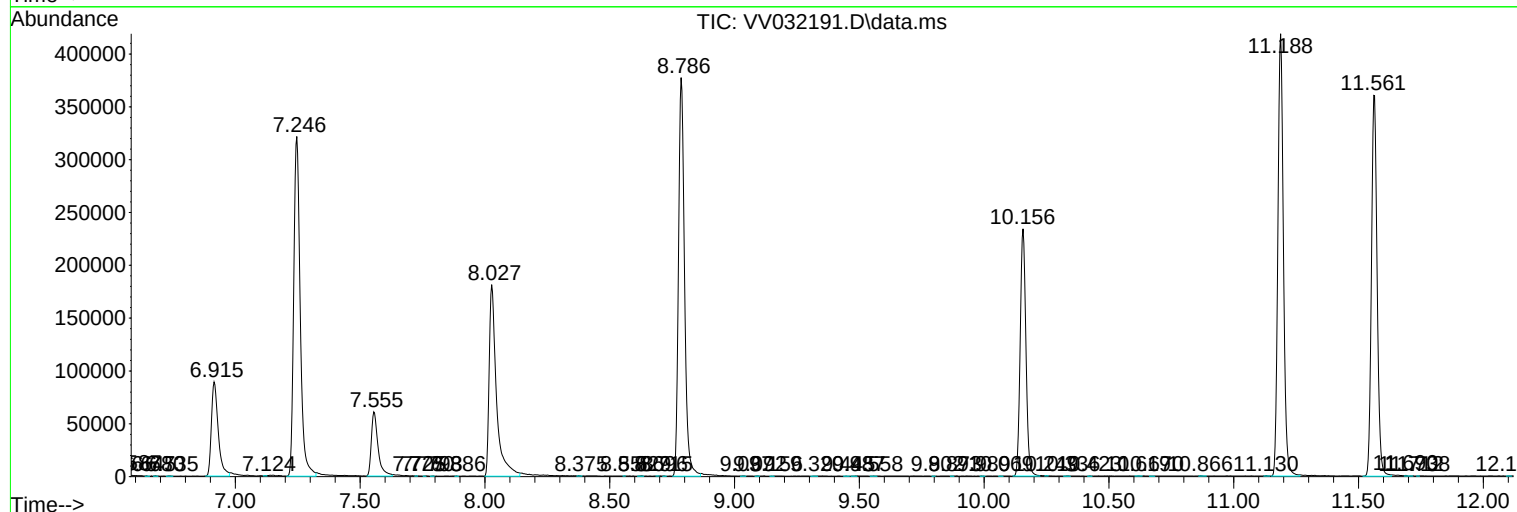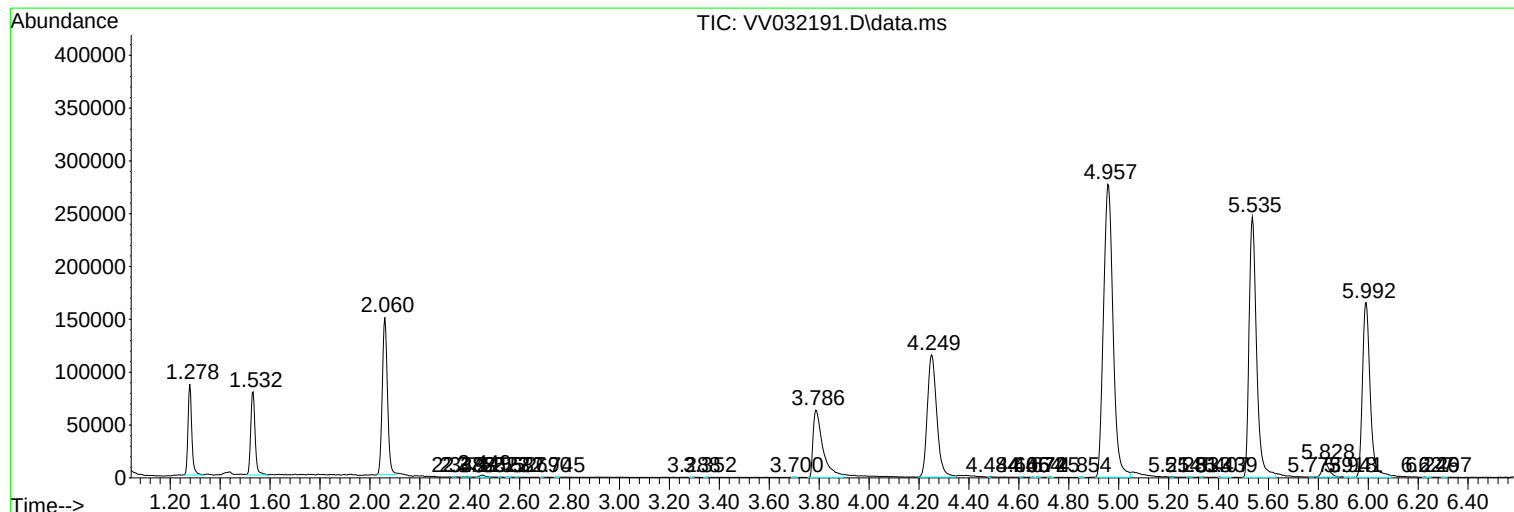

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032191.D
Acq On : 02 Oct 2023 10:50
Operator : SY/MD
Sample : VV1002WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK203

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032191.D
Acq On : 02 Oct 2023 10:50
Operator : SY/MD
Sample : VV1002WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK203

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------