

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032197.D
 Acq On : 02 Oct 2023 13:12
 Operator : SY/MD
 Sample : 04592-02 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

Signal : TIC: VV032197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	52	55	56	rBV	673	374	0.05%	0.006%
2	1.278	68	74	93	rVB	78104	83580	11.90%	1.404%
3	1.426	112	120	125	rBV4	3131	5123	0.73%	0.086%
4	1.532	146	153	171	rVB	74192	89605	12.75%	1.505%
5	2.063	307	318	328	rBV	137406	202329	28.80%	3.398%
6	2.285	383	387	390	rBV3	440	377	0.05%	0.006%
7	2.349	405	407	415	rVB3	322	290	0.04%	0.005%
8	2.400	419	423	424	rBV	237	161	0.02%	0.003%
9	2.452	430	439	451	rBV4	5905	10241	1.46%	0.172%
10	2.555	466	471	472	rBV2	509	332	0.05%	0.006%
11	2.616	488	490	495	rVB2	243	150	0.02%	0.003%
12	2.690	510	513	515	rBV	175	144	0.02%	0.002%
13	2.751	527	532	536	rVB2	238	195	0.03%	0.003%
14	2.793	542	545	552	rVB2	169	166	0.02%	0.003%
15	2.834	552	558	564	rVB2	255	223	0.03%	0.004%
16	2.989	602	606	609	rBB2	312	180	0.03%	0.003%
17	3.092	634	638	641	rBV2	205	228	0.03%	0.004%
18	3.182	664	666	673	rVB2	212	156	0.02%	0.003%
19	3.304	702	704	710	rVB	164	198	0.03%	0.003%
20	3.330	710	712	714	rBV	234	148	0.02%	0.002%
21	3.403	733	735	738	rBV	397	159	0.02%	0.003%
22	3.789	841	855	898	rBV	69834	203833	29.01%	3.424%
23	4.256	983	1000	1027	rBV2	107744	283299	40.32%	4.758%
24	4.548	1087	1091	1094	rVB3	237	150	0.02%	0.003%
25	4.619	1107	1113	1116	rBV2	301	285	0.04%	0.005%
26	4.825	1175	1177	1181	rVB	318	175	0.02%	0.003%
27	4.850	1181	1185	1187	rBV2	301	224	0.03%	0.004%
28	4.960	1203	1219	1249	rBV2	261153	702621	100.00%	11.801%
29	5.146	1275	1277	1281	rVB4	495	278	0.04%	0.005%
30	5.281	1316	1319	1321	rVB2	249	153	0.02%	0.003%
31	5.310	1325	1328	1332	rBV2	345	343	0.05%	0.006%
32	5.368	1340	1346	1350	rVB2	431	402	0.06%	0.007%
33	5.400	1350	1356	1360	rVB3	360	333	0.05%	0.006%
34	5.419	1360	1362	1367	rBV2	227	248	0.04%	0.004%
35	5.471	1375	1378	1384	rVB2	220	167	0.02%	0.003%
36	5.538	1384	1399	1423	rBV	257102	539022	76.72%	9.053%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032197.D
 Acq On : 02 Oct 2023 13:12
 Operator : SY/MD
 Sample : 04592-02 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

37	5.735	1457	1460	1465	rBV3	354	290	0.04%	0.005%
38	5.831	1480	1490	1515	rVB3	12196	28561	4.06%	0.480%
39	5.992	1528	1540	1559	rBV	157498	332103	47.27%	5.578%
40	6.304	1628	1637	1638	rBV2	1222	1466	0.21%	0.025%
41	6.468	1686	1688	1691	rBV2	254	144	0.02%	0.002%
42	6.490	1691	1695	1697	rVV2	255	202	0.03%	0.003%
43	6.509	1698	1701	1704	rVB2	281	147	0.02%	0.002%
44	6.574	1717	1721	1723	rBV2	427	319	0.05%	0.005%
45	6.583	1723	1724	1726	rVV2	369	180	0.03%	0.003%
46	6.596	1726	1728	1730	rVV	522	334	0.05%	0.006%
47	6.612	1730	1733	1735	rVB2	532	334	0.05%	0.006%
48	6.873	1807	1814	1817	rBV	113	151	0.02%	0.003%
49	6.918	1817	1828	1857	rBV	82173	161967	23.05%	2.720%
50	7.130	1890	1894	1899	rVB5	421	386	0.05%	0.006%
51	7.162	1900	1904	1908	rBV3	446	406	0.06%	0.007%
52	7.246	1919	1930	1954	rBV	296595	537435	76.49%	9.027%
53	7.503	2007	2010	2013	rVB2	219	144	0.02%	0.002%
54	7.558	2015	2027	2058	rBV	56282	106636	15.18%	1.791%
55	7.812	2101	2106	2109	rBV	259	200	0.03%	0.003%
56	7.870	2116	2124	2137	rBV5	2458	4743	0.68%	0.080%
57	7.982	2147	2159	2163	rBV5	1782	2858	0.41%	0.048%
58	8.027	2163	2173	2213	rVV	190919	375367	53.42%	6.305%
59	8.368	2270	2279	2286	rBV5	1215	1994	0.28%	0.033%
60	8.519	2321	2326	2329	rBV2	240	200	0.03%	0.003%
61	8.603	2346	2352	2356	rBV3	322	253	0.04%	0.004%
62	8.632	2356	2361	2367	rVB3	322	423	0.06%	0.007%
63	8.786	2398	2409	2439	rBV	404178	678581	96.58%	11.397%
64	8.956	2459	2462	2472	rVB2	692	875	0.12%	0.015%
65	9.001	2473	2476	2480	rVV2	201	172	0.02%	0.003%
66	9.030	2480	2485	2489	rVV3	284	296	0.04%	0.005%
67	9.062	2493	2495	2499	rBV	204	152	0.02%	0.003%
68	9.088	2499	2503	2513	rVV3	650	870	0.12%	0.015%
69	9.355	2581	2586	2587	rBV3	227	182	0.03%	0.003%
70	9.455	2614	2617	2621	rBV2	266	180	0.03%	0.003%
71	9.484	2624	2626	2631	rBV3	279	216	0.03%	0.004%
72	9.808	2724	2727	2731	rVB2	198	158	0.02%	0.003%
73	9.889	2747	2752	2757	rVB2	215	254	0.04%	0.004%
74	9.918	2757	2761	2767	rBV	159	146	0.02%	0.002%
75	10.040	2796	2799	2805	rVB2	176	145	0.02%	0.002%
76	10.156	2824	2835	2857	rVV	227822	363718	51.77%	6.109%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032197.D
 Acq On : 02 Oct 2023 13:12
 Operator : SY/MD
 Sample : 04592-02 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

77	10.271	2867	2871	2874	rBV	235	175	0.02%	0.003%
78	10.326	2884	2888	2891	rBV	491	452	0.06%	0.008%
79	10.381	2902	2905	2908	rBV2	275	215	0.03%	0.004%
80	10.429	2917	2920	2924	rBV2	214	162	0.02%	0.003%
81	10.496	2937	2941	2944	rBV2	226	159	0.02%	0.003%
82	10.792	3027	3033	3036	rBV2	167	214	0.03%	0.004%
83	10.866	3051	3056	3057	rBV	221	154	0.02%	0.003%
84	11.011	3097	3101	3105	rBV2	231	218	0.03%	0.004%
85	11.188	3144	3156	3180	rBV	442159	683303	97.25%	11.477%
86	11.329	3197	3200	3202	rVV	408	231	0.03%	0.004%
87	11.348	3204	3206	3211	rVB	507	241	0.03%	0.004%
88	11.564	3259	3273	3294	rBV	339136	535042	76.15%	8.986%
89	11.638	3294	3296	3301	rVB5	658	383	0.05%	0.006%
90	12.194	3463	3469	3471	rBV2	390	370	0.05%	0.006%
91	12.297	3496	3501	3503	rBV3	195	169	0.02%	0.003%
92	12.461	3546	3552	3554	rBV2	294	301	0.04%	0.005%
93	13.056	3734	3737	3742	rBV2	252	186	0.03%	0.003%
94	13.455	3852	3861	3868	rBV3	671	1219	0.17%	0.020%
95	13.811	3969	3972	3976	rVB	297	206	0.03%	0.003%
96	13.837	3977	3980	3983	rBV3	371	222	0.03%	0.004%
97	13.905	3997	4001	4004	rBV	498	459	0.07%	0.008%
98	14.377	4145	4148	4152	rBV2	335	235	0.03%	0.004%
99	14.596	4214	4216	4220	rBV3	264	166	0.02%	0.003%
100	15.316	4437	4440	4442	rBV2	444	293	0.04%	0.005%




Sum of corrected areas: 5953855

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032197.D
Acq On : 02 Oct 2023 13:12
Operator : SY/MD
Sample : 04592-02 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

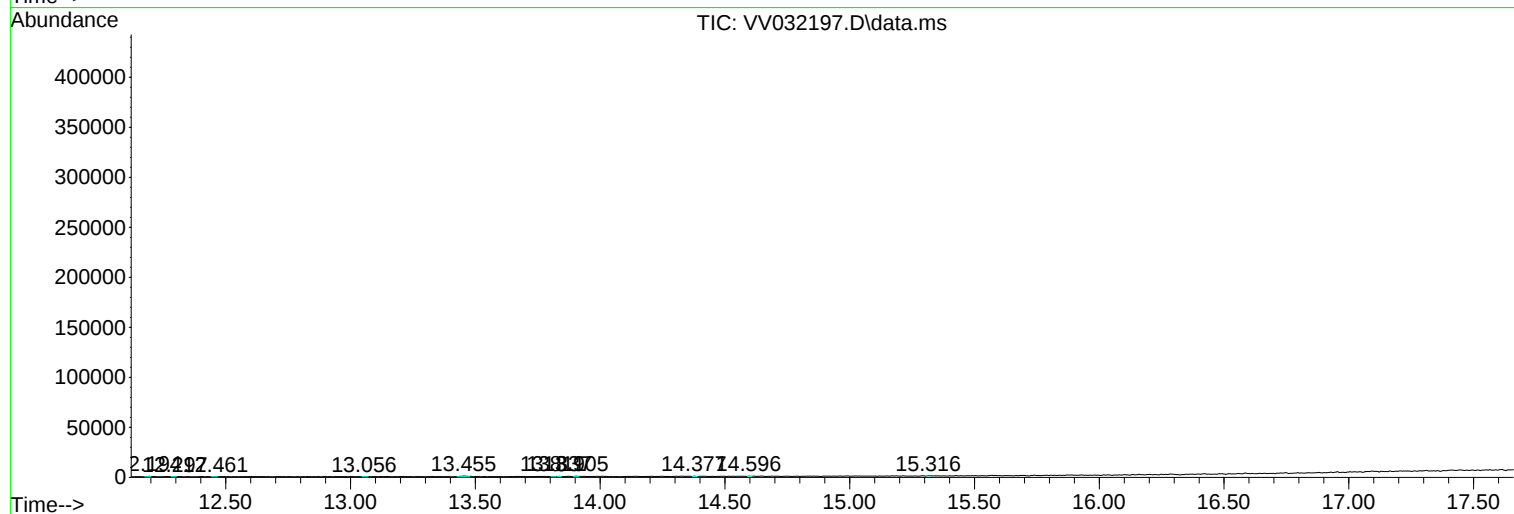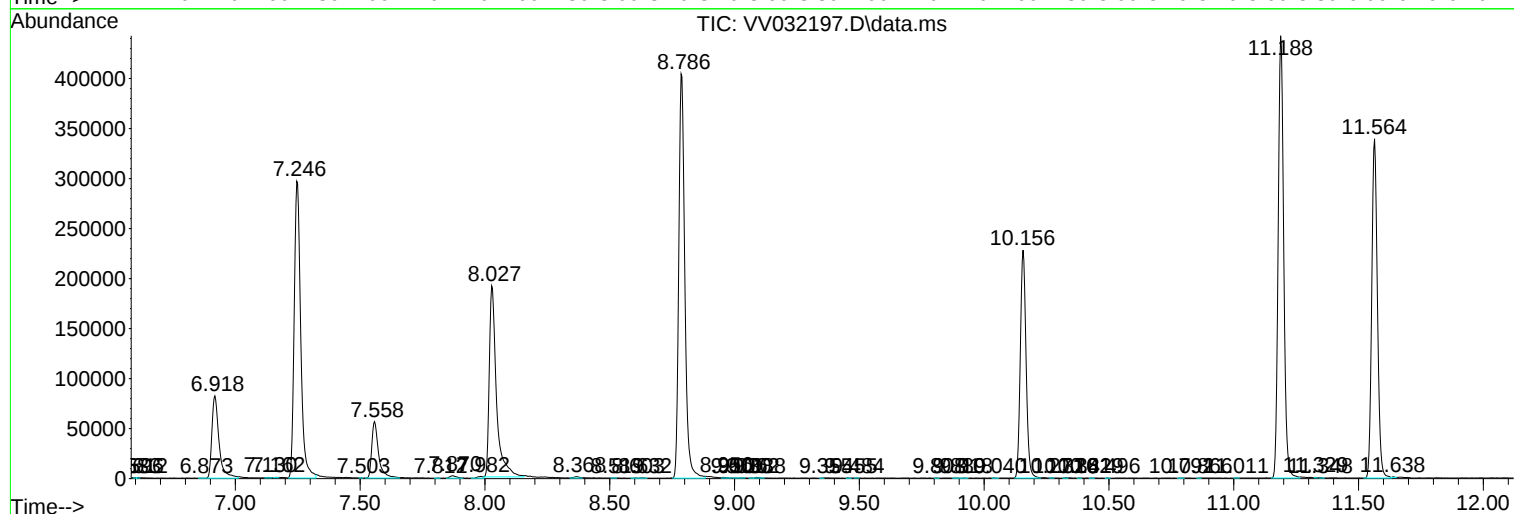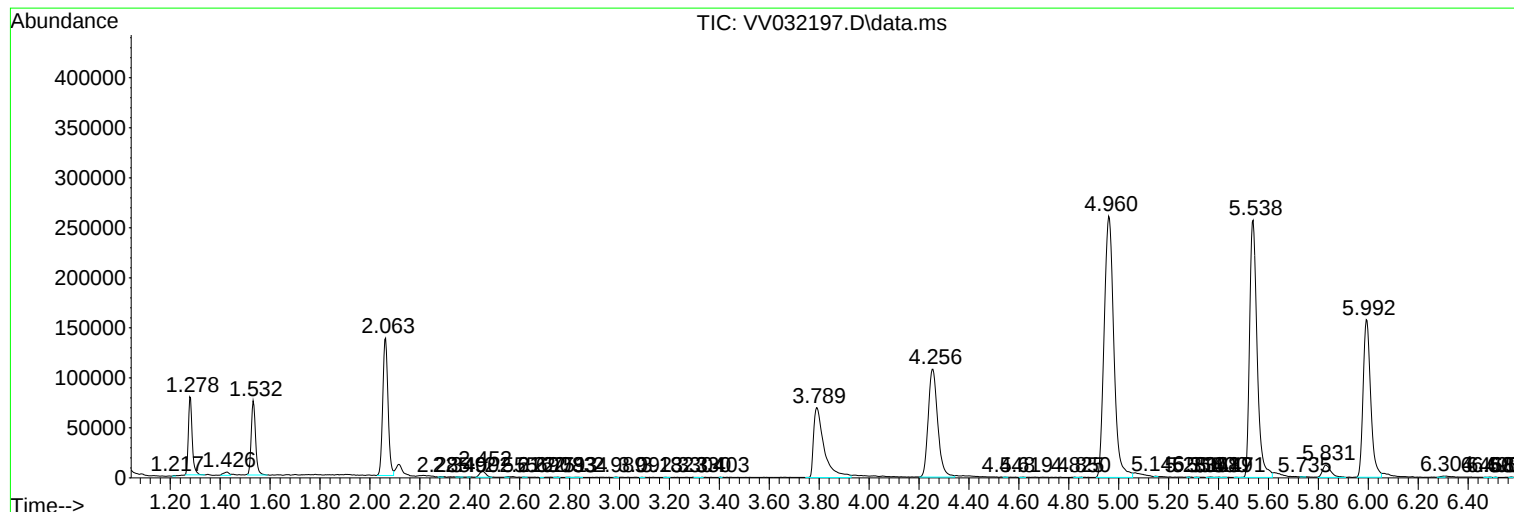

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032197.D
Acq On : 02 Oct 2023 13:12
Operator : SY/MD
Sample : 04592-02 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032197.D
Acq On : 02 Oct 2023 13:12
Operator : SY/MD
Sample : 04592-02 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------