

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032198.D
 Acq On : 02 Oct 2023 13:35
 Operator : SY/MD
 Sample : 04592-03 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

Signal : TIC: VV032198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	76807	84587	12.22%	1.452%
2	1.532	146	153	169	rVB	74575	89866	12.98%	1.543%
3	2.063	308	318	329	rBV	133406	196870	28.44%	3.379%
4	2.449	430	438	452	rVB2	6145	10809	1.56%	0.186%
5	2.693	508	514	519	rVB3	300	359	0.05%	0.006%
6	2.879	570	572	576	rVB2	172	74	0.01%	0.001%
7	2.902	576	579	581	rBV	139	98	0.01%	0.002%
8	2.976	600	602	603	rBV	215	73	0.01%	0.001%
9	3.037	618	621	628	rVB	209	170	0.02%	0.003%
10	3.130	647	650	653	rBV2	159	90	0.01%	0.002%
11	3.220	676	678	679	rBV2	141	62	0.01%	0.001%
12	3.346	714	717	719	rBV	145	90	0.01%	0.002%
13	3.368	719	724	726	rVV2	180	144	0.02%	0.002%
14	3.603	795	797	800	rBV	182	88	0.01%	0.002%
15	3.632	805	806	807	rVB	111	21	0.00%	0.000%
16	3.664	812	816	819	rBV2	210	195	0.03%	0.003%
17	3.741	836	840	842	rBV2	63	53	0.01%	0.001%
18	3.754	842	844	845	rBV	272	119	0.02%	0.002%
19	3.789	846	855	892	rBV	70463	199179	28.78%	3.419%
20	4.252	983	999	1028	rBV	107683	280509	40.53%	4.815%
21	4.494	1069	1074	1076	rBV3	404	355	0.05%	0.006%
22	4.548	1088	1091	1092	rBV2	315	186	0.03%	0.003%
23	4.635	1116	1118	1122	rBV3	221	138	0.02%	0.002%
24	4.712	1140	1142	1146	rVB	160	107	0.02%	0.002%
25	4.748	1149	1153	1158	rBV2	253	209	0.03%	0.004%
26	4.770	1158	1160	1162	rVV	273	130	0.02%	0.002%
27	4.960	1203	1219	1247	rBV2	257979	692144	100.00%	11.881%
28	5.336	1334	1336	1338	rBV2	129	37	0.01%	0.001%
29	5.378	1346	1349	1352	rBV2	222	121	0.02%	0.002%
30	5.477	1379	1380	1381	rBV2	111	30	0.00%	0.001%
31	5.538	1387	1399	1423	rBV	252053	520909	75.26%	8.941%
32	5.831	1478	1490	1510	rBV2	12136	26519	3.83%	0.455%
33	5.992	1525	1540	1578	rBV	157804	339263	49.02%	5.823%
34	6.249	1617	1620	1624	rBV2	471	422	0.06%	0.007%
35	6.461	1682	1686	1689	rVB3	336	243	0.04%	0.004%
36	6.545	1709	1712	1716	rBV3	329	260	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032198.D
 Acq On : 02 Oct 2023 13:35
 Operator : SY/MD
 Sample : 04592-03 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

37	6.767	1778	1781	1783	rBV2	184	108	0.02%	0.002%
38	6.876	1813	1815	1816	rBV	148	56	0.01%	0.001%
39	6.918	1817	1828	1853	rBV	82434	158330	22.88%	2.718%
40	7.246	1919	1930	1955	rBV	296697	532643	76.96%	9.143%
41	7.558	2017	2027	2050	rBV	55996	103209	14.91%	1.772%
42	7.722	2076	2078	2081	rBV2	305	161	0.02%	0.003%
43	7.770	2091	2093	2094	rBV2	177	62	0.01%	0.001%
44	7.783	2095	2097	2101	rVB3	486	301	0.04%	0.005%
45	7.808	2101	2105	2106	rBV2	272	134	0.02%	0.002%
46	7.818	2106	2108	2110	rVB	167	48	0.01%	0.001%
47	7.870	2117	2124	2134	rBV7	2550	3867	0.56%	0.066%
48	7.972	2152	2156	2157	rBV	1175	766	0.11%	0.013%
49	8.027	2164	2173	2205	rBV	191029	369532	53.39%	6.343%
50	8.442	2298	2302	2305	rBV3	320	249	0.04%	0.004%
51	8.545	2331	2334	2335	rBV2	162	69	0.01%	0.001%
52	8.590	2346	2348	2349	rBV2	154	83	0.01%	0.001%
53	8.619	2355	2357	2358	rBV	153	45	0.01%	0.001%
54	8.680	2374	2376	2380	rVB2	383	205	0.03%	0.004%
55	8.699	2380	2382	2383	rBV2	123	58	0.01%	0.001%
56	8.735	2391	2393	2395	rVB	159	65	0.01%	0.001%
57	8.789	2398	2410	2439	rBV	390152	654594	94.57%	11.236%
58	9.024	2479	2483	2487	rVB2	387	269	0.04%	0.005%
59	9.046	2488	2490	2492	rBV	125	78	0.01%	0.001%
60	9.082	2498	2501	2505	rBV2	516	360	0.05%	0.006%
61	9.101	2505	2507	2512	rVB2	380	259	0.04%	0.004%
62	9.214	2540	2542	2543	rBV	136	38	0.01%	0.001%
63	9.487	2624	2627	2629	rBV3	155	116	0.02%	0.002%
64	9.693	2690	2691	2692	rBV	143	37	0.01%	0.001%
65	9.741	2700	2706	2711	rBV2	194	256	0.04%	0.004%
66	9.789	2719	2721	2725	rBV2	173	99	0.01%	0.002%
67	9.828	2730	2733	2734	rBV	135	91	0.01%	0.002%
68	9.905	2755	2757	2762	rVB3	317	206	0.03%	0.004%
69	9.931	2762	2765	2769	rBV2	122	110	0.02%	0.002%
70	9.988	2780	2783	2787	rBV	170	138	0.02%	0.002%
71	10.156	2823	2835	2857	rBV	230668	363514	52.52%	6.240%
72	10.320	2884	2886	2887	rBV	229	95	0.01%	0.002%
73	10.651	2985	2989	2990	rBV2	216	152	0.02%	0.003%
74	10.824	3039	3043	3051	rBV2	299	555	0.08%	0.010%
75	10.988	3092	3094	3095	rBV	165	54	0.01%	0.001%
76	11.188	3145	3156	3181	rBV	433757	661716	95.60%	11.358%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032198.D
Acq On : 02 Oct 2023 13:35
Operator : SY/MD
Sample : 04592-03 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Title : VOC Analysis

77	11.451	3235	3238	3243	rBV	327	206	0.03%	0.004%
78	11.564	3261	3273	3295	rBV	331712	528335	76.33%	9.069%
79	11.921	3382	3384	3387	rBV	247	61	0.01%	0.001%




Sum of corrected areas: 5825859

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032198.D
Acq On : 02 Oct 2023 13:35
Operator : SY/MD
Sample : 04592-03 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZZY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

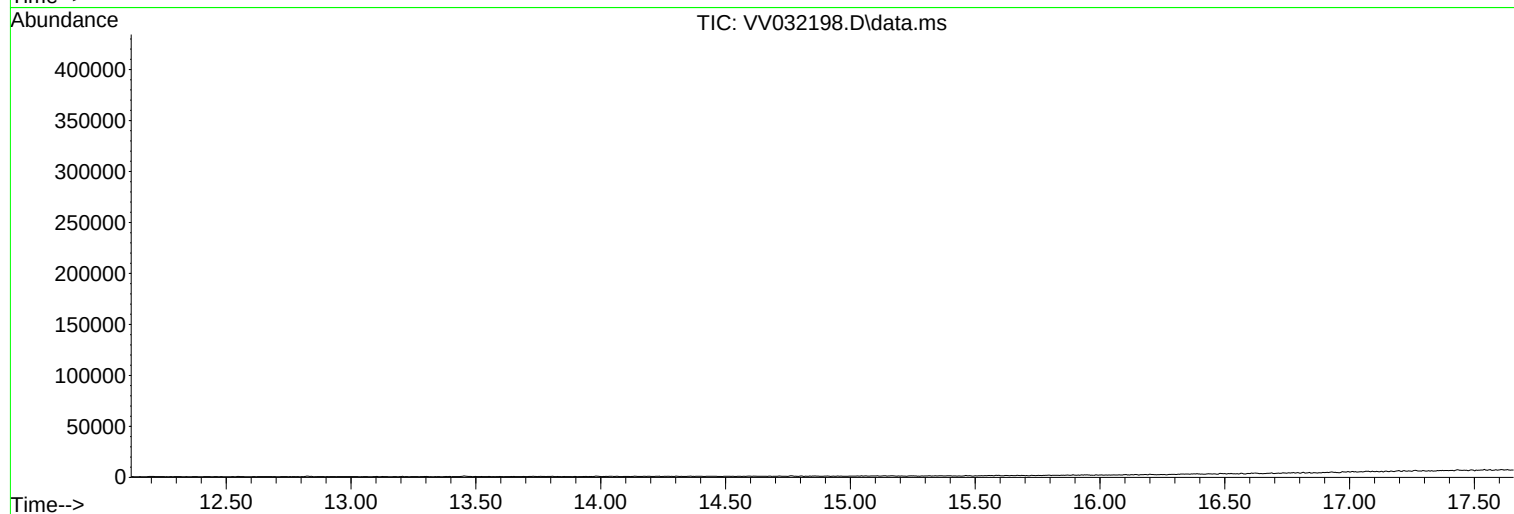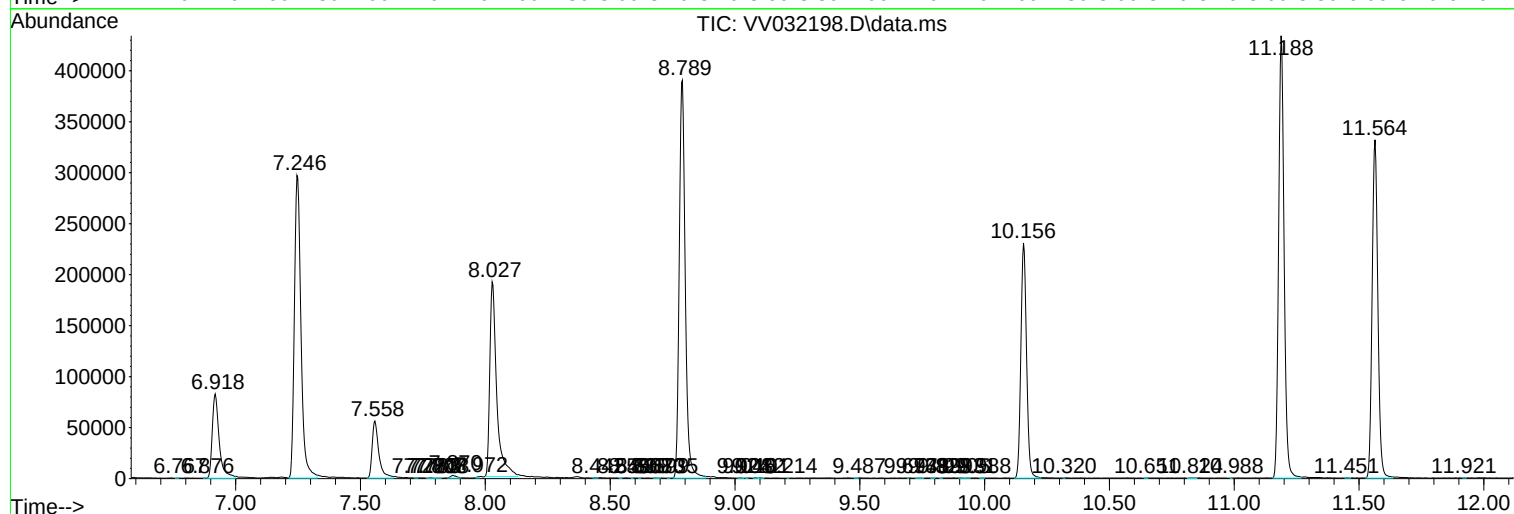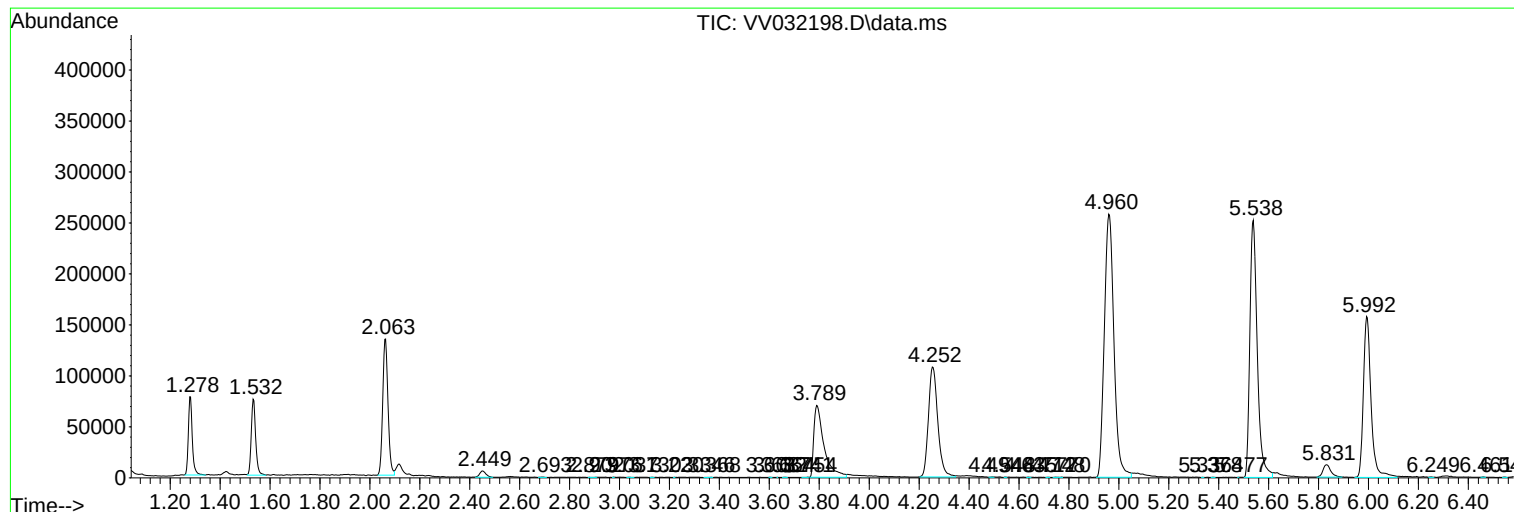

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032198.D
Acq On : 02 Oct 2023 13:35
Operator : SY/MD
Sample : 04592-03 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032198.D
Acq On : 02 Oct 2023 13:35
Operator : SY/MD
Sample : 04592-03 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------