

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032199.D
 Acq On : 02 Oct 2023 13:59
 Operator : SY/MD
 Sample : 04592-04 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M

Title : VOC Analysis

Signal : TIC: VV032199.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	51	54	56	rBV3	913	616	0.09%	0.011%
2	1.278	67	74	88	rBV	76464	81294	12.03%	1.398%
3	1.532	145	153	166	rVB	70416	83814	12.40%	1.441%
4	2.060	307	317	329	rBV	132878	193160	28.59%	3.322%
5	2.201	359	361	362	rBV	791	379	0.06%	0.007%
6	2.281	383	386	392	rVB3	430	388	0.06%	0.007%
7	2.378	412	416	419	rBV2	438	339	0.05%	0.006%
8	2.449	429	438	452	rVB2	6425	10472	1.55%	0.180%
9	2.561	466	473	477	rBV3	876	1164	0.17%	0.020%
10	2.722	520	523	526	rVV2	269	189	0.03%	0.003%
11	2.982	602	604	610	rVB3	314	250	0.04%	0.004%
12	3.220	675	678	683	rBV2	168	166	0.02%	0.003%
13	3.285	696	698	703	rVB2	188	150	0.02%	0.003%
14	3.317	703	708	711	rBV2	162	181	0.03%	0.003%
15	3.687	820	823	826	rBV2	200	160	0.02%	0.003%
16	3.789	844	855	894	rBV	68367	195207	28.89%	3.357%
17	4.146	964	966	970	rVB2	319	168	0.02%	0.003%
18	4.179	972	976	978	rBV3	263	196	0.03%	0.003%
19	4.252	984	999	1027	rBV2	106750	273396	40.46%	4.702%
20	4.400	1044	1045	1047	rBV2	537	154	0.02%	0.003%
21	4.503	1075	1077	1079	rVB3	381	157	0.02%	0.003%
22	4.590	1101	1104	1111	rVB4	254	220	0.03%	0.004%
23	4.629	1113	1116	1119	rVB3	562	347	0.05%	0.006%
24	4.658	1119	1125	1129	rVB3	379	414	0.06%	0.007%
25	4.757	1153	1156	1158	rBV2	242	200	0.03%	0.003%
26	4.960	1203	1219	1248	rBV2	254406	675712	100.00%	11.621%
27	5.127	1270	1271	1274	rVB2	529	238	0.04%	0.004%
28	5.220	1293	1300	1316	rVB6	2423	5751	0.85%	0.099%
29	5.349	1337	1340	1346	rVB4	618	452	0.07%	0.008%
30	5.416	1357	1361	1364	rVB3	259	218	0.03%	0.004%
31	5.477	1376	1380	1381	rBV	278	166	0.02%	0.003%
32	5.535	1385	1398	1427	rBV	251812	527521	78.07%	9.072%
33	5.831	1478	1490	1507	rBV2	11477	25643	3.79%	0.441%
34	5.992	1526	1540	1578	rBV	153910	330279	48.88%	5.680%
35	6.201	1602	1605	1607	rBV2	344	186	0.03%	0.003%
36	6.246	1616	1619	1623	rVB3	372	207	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032199.D
 Acq On : 02 Oct 2023 13:59
 Operator : SY/MD
 Sample : 04592-04 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

37	6.297	1628	1635	1637	rBV3	1273	1344	0.20%	0.023%
38	6.407	1666	1669	1670	rBV	324	167	0.02%	0.003%
39	6.426	1670	1675	1676	rBV3	1663	1355	0.20%	0.023%
40	6.522	1702	1705	1707	rVB	512	277	0.04%	0.005%
41	6.574	1717	1721	1723	rBV3	362	320	0.05%	0.006%
42	6.661	1745	1748	1752	rVB3	346	270	0.04%	0.005%
43	6.683	1752	1755	1759	rVB2	259	179	0.03%	0.003%
44	6.918	1818	1828	1853	rBV	80775	155264	22.98%	2.670%
45	7.127	1884	1893	1904	rBV2	7144	12937	1.91%	0.222%
46	7.246	1919	1930	1961	rBV	285746	519010	76.81%	8.926%
47	7.481	2001	2003	2010	rVB3	473	427	0.06%	0.007%
48	7.558	2017	2027	2058	rVV	54122	104049	15.40%	1.789%
49	7.866	2113	2123	2144	rVV	13495	24152	3.57%	0.415%
50	7.944	2144	2147	2150	rBV2	257	183	0.03%	0.003%
51	7.982	2150	2159	2162	rBV6	1269	2100	0.31%	0.036%
52	8.027	2163	2173	2208	rBV	188616	363998	53.87%	6.260%
53	8.268	2246	2248	2252	rVB2	440	176	0.03%	0.003%
54	8.362	2271	2277	2286	rVB4	1466	2293	0.34%	0.039%
55	8.452	2303	2305	2307	rBV	227	158	0.02%	0.003%
56	8.571	2339	2342	2345	rVB	272	184	0.03%	0.003%
57	8.625	2350	2359	2375	rBV3	12236	21707	3.21%	0.373%
58	8.786	2398	2409	2436	rVV	389152	656389	97.14%	11.289%
59	8.966	2461	2465	2468	rVB3	530	435	0.06%	0.007%
60	9.114	2508	2511	2516	rVB	339	223	0.03%	0.004%
61	9.249	2547	2553	2554	rBV	229	181	0.03%	0.003%
62	9.509	2632	2634	2640	rVB2	267	225	0.03%	0.004%
63	9.690	2683	2690	2692	rBV	191	204	0.03%	0.004%
64	9.735	2698	2704	2706	rBV2	185	183	0.03%	0.003%
65	9.892	2750	2753	2759	rVB	238	241	0.04%	0.004%
66	10.030	2793	2796	2800	rVB2	343	221	0.03%	0.004%
67	10.085	2807	2813	2817	rBV2	189	210	0.03%	0.004%
68	10.156	2822	2835	2857	rBV	224183	353717	52.35%	6.083%
69	10.313	2879	2884	2886	rBV	257	180	0.03%	0.003%
70	10.336	2886	2891	2893	rBV2	188	193	0.03%	0.003%
71	10.397	2905	2910	2913	rVB2	269	237	0.04%	0.004%
72	10.435	2917	2922	2925	rVV2	214	165	0.02%	0.003%
73	10.452	2925	2927	2931	rVV2	218	155	0.02%	0.003%
74	10.796	3030	3034	3037	rBV	208	179	0.03%	0.003%
75	10.863	3050	3055	3058	rBV3	457	482	0.07%	0.008%
76	10.963	3081	3086	3090	rVB	247	224	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032199.D
 Acq On : 02 Oct 2023 13:59
 Operator : SY/MD
 Sample : 04592-04 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M

Title : VOC Analysis

77	10.989	3090	3094	3095	rBV	210	156	0.02%	0.003%
78	11.188	3145	3156	3180	rVV	426536	659898	97.66%	11.349%
79	11.281	3183	3185	3189	rVB3	404	245	0.04%	0.004%
80	11.304	3190	3192	3195	rBV3	641	290	0.04%	0.005%
81	11.435	3230	3233	3234	rBV	262	168	0.02%	0.003%
82	11.564	3257	3273	3296	rBV	324852	513419	75.98%	8.830%
83	11.767	3331	3336	3339	rVB3	371	318	0.05%	0.005%
84	11.866	3363	3367	3372	rBV4	364	290	0.04%	0.005%
85	11.963	3394	3397	3398	rBV2	245	154	0.02%	0.003%
86	12.069	3426	3430	3433	rVB2	259	215	0.03%	0.004%
87	12.365	3517	3522	3526	rBV3	332	278	0.04%	0.005%
88	12.455	3547	3550	3554	rBV2	219	175	0.03%	0.003%
89	12.988	3709	3716	3722	rVB4	1669	2118	0.31%	0.036%
90	13.069	3738	3741	3745	rBV2	218	178	0.03%	0.003%
91	13.445	3855	3858	3859	rBV2	459	229	0.03%	0.004%
92	13.525	3880	3883	3885	rBV2	239	182	0.03%	0.003%
93	13.693	3932	3935	3938	rVB2	394	233	0.03%	0.004%
94	13.712	3938	3941	3946	rVB2	235	180	0.03%	0.003%
95	13.908	3999	4002	4005	rVB	271	155	0.02%	0.003%
96	13.931	4005	4009	4011	rBV	215	185	0.03%	0.003%
97	14.091	4054	4059	4062	rVB2	310	289	0.04%	0.005%
98	14.159	4077	4080	4083	rBV2	248	193	0.03%	0.003%
99	14.181	4083	4087	4096	rVV3	337	616	0.09%	0.011%
100	14.329	4131	4133	4137	rBV2	338	217	0.03%	0.004%




Sum of corrected areas: 5814529

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032199.D
Acq On : 02 Oct 2023 13:59
Operator : SY/MD
Sample : 04592-04 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

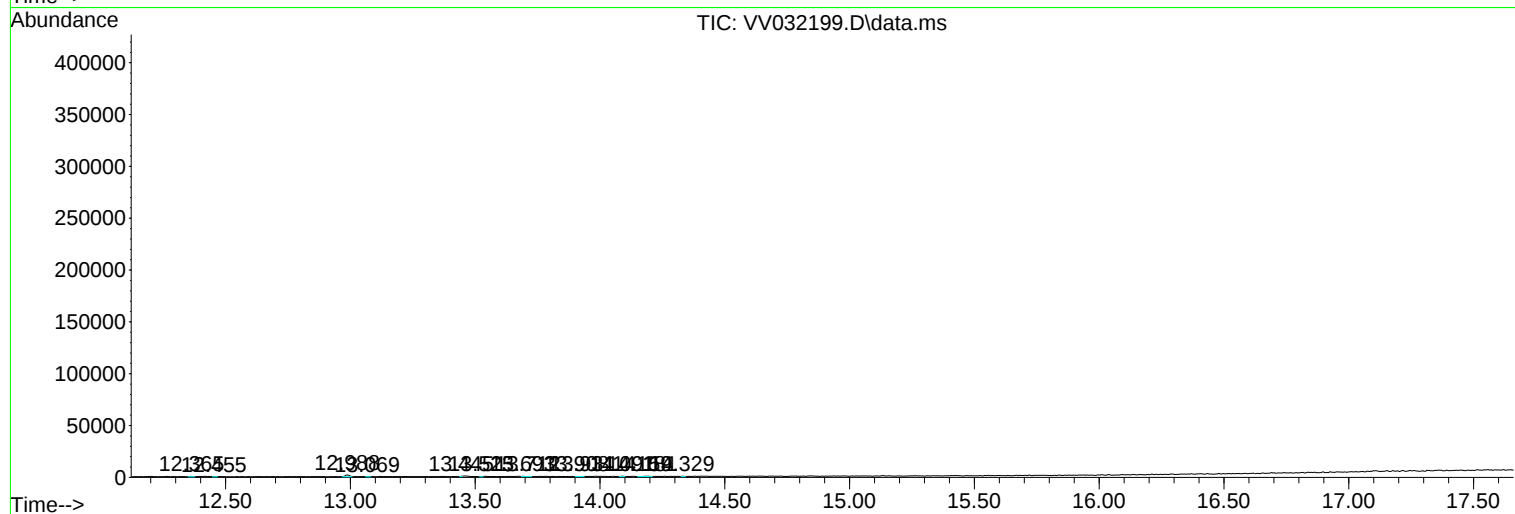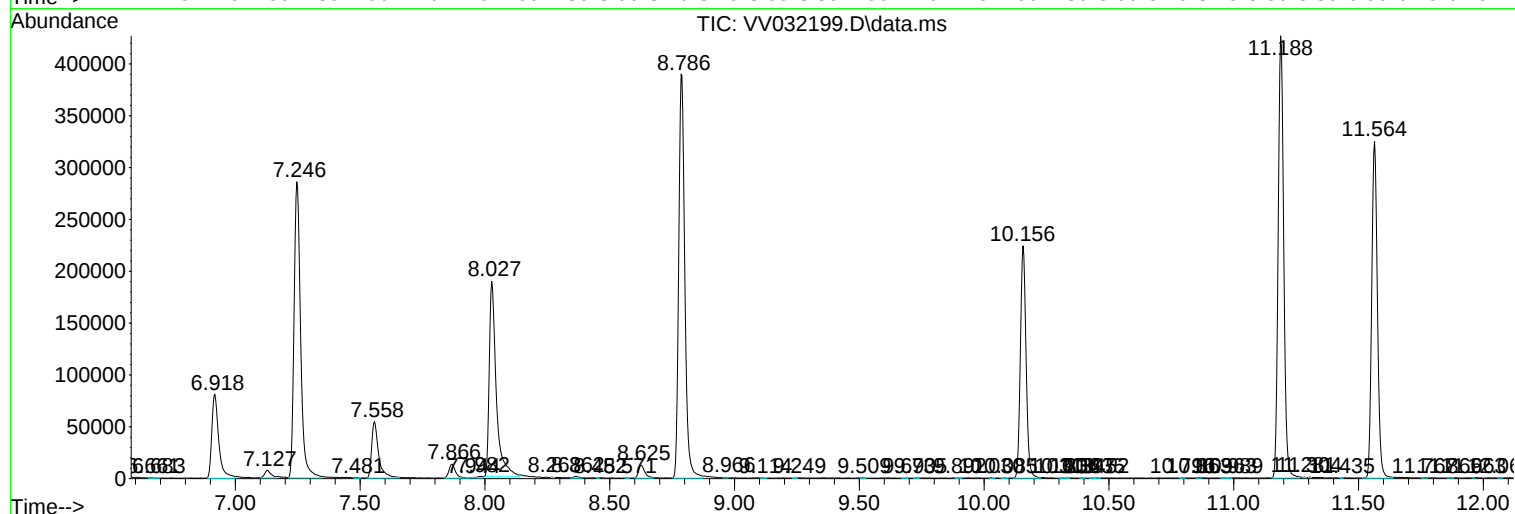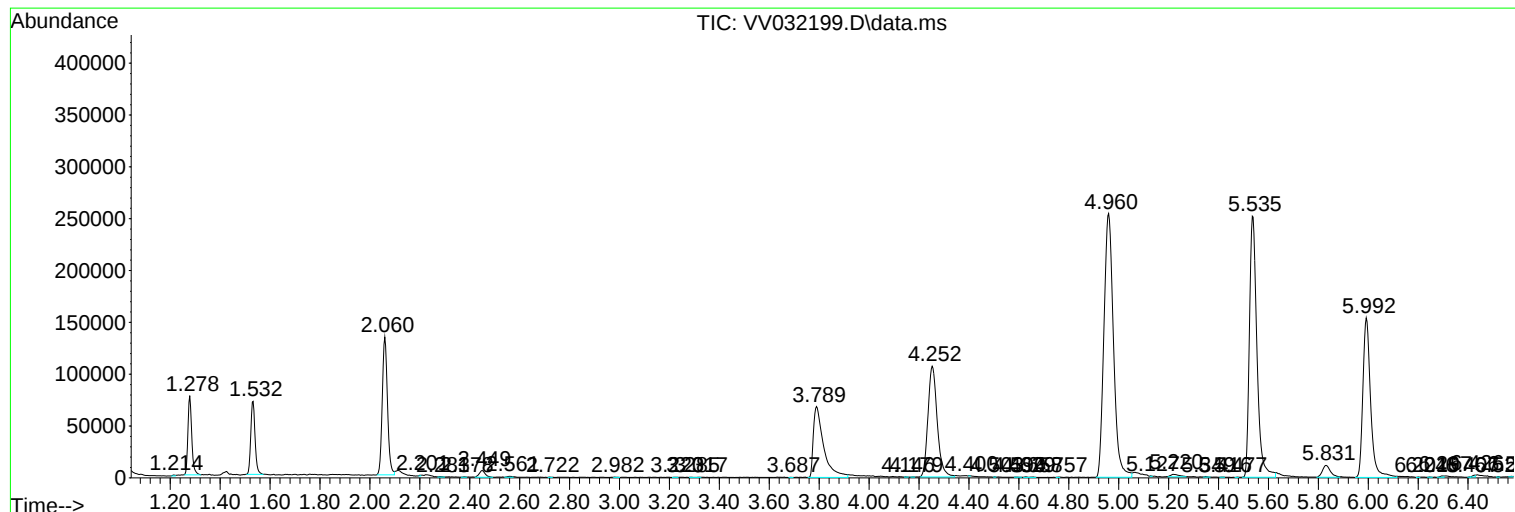

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032199.D
Acq On : 02 Oct 2023 13:59
Operator : SY/MD
Sample : 04592-04 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032199.D
Acq On : 02 Oct 2023 13:59
Operator : SY/MD
Sample : 04592-04 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc