

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032200.D
 Acq On : 02 Oct 2023 14:22
 Operator : SY/MD
 Sample : 04592-05 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

Signal : TIC: VV032200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVV	79386	84026	12.23%	1.443%
2	1.349	92	96	104	rVB	3326	3898	0.57%	0.067%
3	1.426	111	120	127	rBV9	3378	6071	0.88%	0.104%
4	1.529	145	152	167	rVB	72402	86308	12.57%	1.482%
5	2.060	307	317	328	rBV	135300	196638	28.63%	3.377%
6	2.449	428	438	451	rVB2	6978	11790	1.72%	0.202%
7	2.561	465	473	485	rVB	768	1546	0.23%	0.027%
8	2.793	540	545	547	rBV	332	239	0.03%	0.004%
9	3.008	606	612	613	rBV	201	157	0.02%	0.003%
10	3.053	622	626	630	rVB3	211	199	0.03%	0.003%
11	3.127	647	649	655	rVB3	238	168	0.02%	0.003%
12	3.182	663	666	671	rVB	342	203	0.03%	0.003%
13	3.285	695	698	703	rVB2	213	188	0.03%	0.003%
14	3.391	730	731	736	rVB2	347	204	0.03%	0.004%
15	3.519	767	771	776	rBV2	301	221	0.03%	0.004%
16	3.571	784	787	791	rBV2	212	160	0.02%	0.003%
17	3.600	791	796	801	rVB2	257	194	0.03%	0.003%
18	3.632	801	806	809	rBV2	180	166	0.02%	0.003%
19	3.712	829	831	835	rVB	331	171	0.02%	0.003%
20	3.789	845	855	894	rBV2	72857	208685	30.38%	3.583%
21	4.252	983	999	1026	rBV	99166	277155	40.35%	4.759%
22	4.577	1097	1100	1103	rBV2	294	147	0.02%	0.003%
23	4.603	1104	1108	1109	rVV3	209	143	0.02%	0.002%
24	4.680	1126	1132	1137	rVB3	220	252	0.04%	0.004%
25	4.805	1169	1171	1174	rVB2	253	143	0.02%	0.002%
26	4.960	1203	1219	1248	rBV2	259509	686839	100.00%	11.794%
27	5.182	1286	1288	1291	rBV3	423	220	0.03%	0.004%
28	5.275	1315	1317	1318	rBV	255	141	0.02%	0.002%
29	5.310	1325	1328	1333	rVB3	392	340	0.05%	0.006%
30	5.362	1340	1344	1350	rBV4	328	378	0.06%	0.006%
31	5.439	1365	1368	1373	rVB2	188	176	0.03%	0.003%
32	5.471	1373	1378	1380	rBV2	146	140	0.02%	0.002%
33	5.535	1387	1398	1425	rBV	250449	518575	75.50%	8.905%
34	5.825	1476	1488	1506	rBV2	42581	88933	12.95%	1.527%
35	5.992	1527	1540	1575	rBV	154755	333065	48.49%	5.719%
36	6.156	1589	1591	1594	rVB3	316	152	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032200.D
 Acq On : 02 Oct 2023 14:22
 Operator : SY/MD
 Sample : 04592-05 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

37	6.297	1628	1635	1636	rBV2	1202	1243	0.18%	0.021%
38	6.365	1654	1656	1660	rBV	248	171	0.02%	0.003%
39	6.477	1688	1691	1693	rBV2	343	168	0.02%	0.003%
40	6.561	1714	1717	1719	rBV3	357	203	0.03%	0.003%
41	6.584	1719	1724	1727	rBV3	594	636	0.09%	0.011%
42	6.651	1743	1745	1749	rVB2	224	134	0.02%	0.002%
43	6.686	1753	1756	1762	rBV3	304	265	0.04%	0.005%
44	6.918	1817	1828	1861	rBV	80952	157892	22.99%	2.711%
45	7.056	1869	1871	1876	rVV2	478	334	0.05%	0.006%
46	7.127	1889	1893	1895	rBV3	461	350	0.05%	0.006%
47	7.246	1918	1930	1970	rBV	293334	534197	77.78%	9.173%
48	7.558	2017	2027	2056	rVV	54621	102899	14.98%	1.767%
49	7.741	2082	2084	2087	rVB2	388	169	0.02%	0.003%
50	7.770	2089	2093	2095	rBV2	320	195	0.03%	0.003%
51	7.805	2100	2104	2108	rBV2	339	224	0.03%	0.004%
52	7.876	2124	2126	2129	rBV	320	215	0.03%	0.004%
53	7.937	2142	2145	2150	rBV2	141	142	0.02%	0.002%
54	7.982	2150	2159	2162	rBV3	1669	2595	0.38%	0.045%
55	8.027	2163	2173	2214	rVV	193531	380993	55.47%	6.542%
56	8.304	2257	2259	2262	rVV3	306	163	0.02%	0.003%
57	8.368	2275	2279	2282	rVV3	430	317	0.05%	0.005%
58	8.384	2282	2284	2288	rVB2	519	275	0.04%	0.005%
59	8.419	2292	2295	2297	rBV	261	200	0.03%	0.003%
60	8.513	2319	2324	2327	rVB3	283	259	0.04%	0.004%
61	8.555	2334	2337	2339	rBV	255	142	0.02%	0.002%
62	8.593	2347	2349	2353	rBV3	217	153	0.02%	0.003%
63	8.661	2364	2370	2378	rBV2	250	341	0.05%	0.006%
64	8.786	2398	2409	2455	rBV	388086	650438	94.70%	11.169%
65	8.960	2459	2463	2468	rVB4	626	571	0.08%	0.010%
66	9.008	2476	2478	2482	rVB2	304	220	0.03%	0.004%
67	9.085	2490	2502	2513	rBV3	3668	6286	0.92%	0.108%
68	9.130	2513	2516	2522	rVB3	402	405	0.06%	0.007%
69	9.165	2522	2527	2529	rBV2	184	180	0.03%	0.003%
70	9.313	2569	2573	2580	rBV2	130	148	0.02%	0.003%
71	9.342	2580	2582	2583	rBV	302	165	0.02%	0.003%
72	9.397	2597	2599	2603	rVB	296	178	0.03%	0.003%
73	9.490	2620	2628	2636	rBV5	2704	4108	0.60%	0.071%
74	9.628	2667	2671	2675	rVB2	203	142	0.02%	0.002%
75	9.706	2691	2695	2699	rVB	217	151	0.02%	0.003%
76	9.876	2741	2748	2752	rBV3	290	434	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032200.D
 Acq On : 02 Oct 2023 14:22
 Operator : SY/MD
 Sample : 04592-05 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M

Title : VOC Analysis

77	10.156	2823	2835	2855	rBV	174265	279402	40.68%	4.798%
78	10.313	2878	2884	2886	rBV	292	225	0.03%	0.004%
79	10.484	2931	2937	2944	rVV2	729	819	0.12%	0.014%
80	10.683	2994	2999	3004	rVB2	349	367	0.05%	0.006%
81	10.860	3046	3054	3060	rBV3	1117	1633	0.24%	0.028%
82	11.098	3123	3128	3129	rBV	341	259	0.04%	0.004%
83	11.133	3136	3139	3142	rBV2	357	248	0.04%	0.004%
84	11.188	3144	3156	3177	rBV	425479	653558	95.15%	11.223%
85	11.336	3200	3202	3207	rVB3	490	280	0.04%	0.005%
86	11.362	3207	3210	3213	rVB3	225	143	0.02%	0.002%
87	11.445	3235	3236	3242	rVB2	227	170	0.02%	0.003%
88	11.564	3261	3273	3298	rVV	330044	525066	76.45%	9.016%
89	11.857	3362	3364	3365	rBV	369	188	0.03%	0.003%
90	11.892	3373	3375	3379	rVB	261	157	0.02%	0.003%
91	11.963	3392	3397	3400	rBV2	295	322	0.05%	0.006%
92	12.159	3456	3458	3462	rBV2	252	166	0.02%	0.003%
93	12.204	3469	3472	3475	rVB2	332	242	0.04%	0.004%
94	12.365	3519	3522	3527	rVB2	344	236	0.03%	0.004%
95	12.400	3531	3533	3534	rBV2	374	166	0.02%	0.003%
96	12.988	3713	3716	3722	rVB	973	771	0.11%	0.013%
97	13.355	3827	3830	3833	rBV	205	189	0.03%	0.003%
98	13.448	3853	3859	3871	rBV4	1383	2101	0.31%	0.036%
99	13.554	3887	3892	3895	rBV3	261	226	0.03%	0.004%
100	15.130	4379	4382	4385	rBV2	411	260	0.04%	0.004%




Sum of corrected areas: 5823526

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032200.D
Acq On : 02 Oct 2023 14:22
Operator : SY/MD
Sample : 04592-05 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

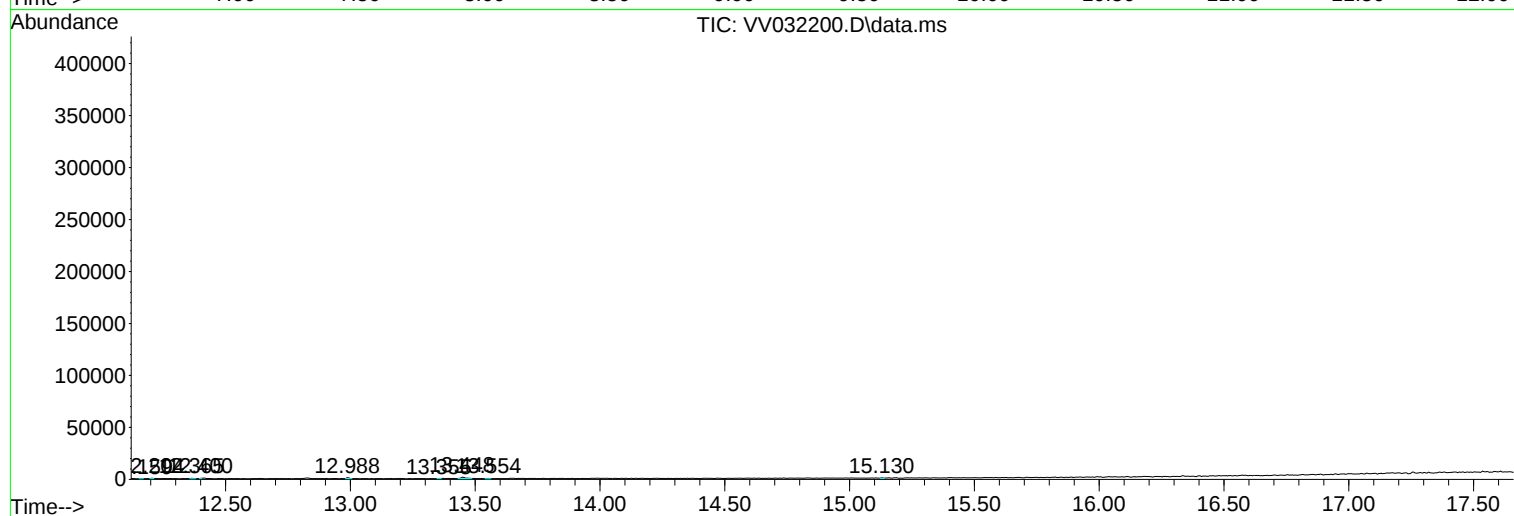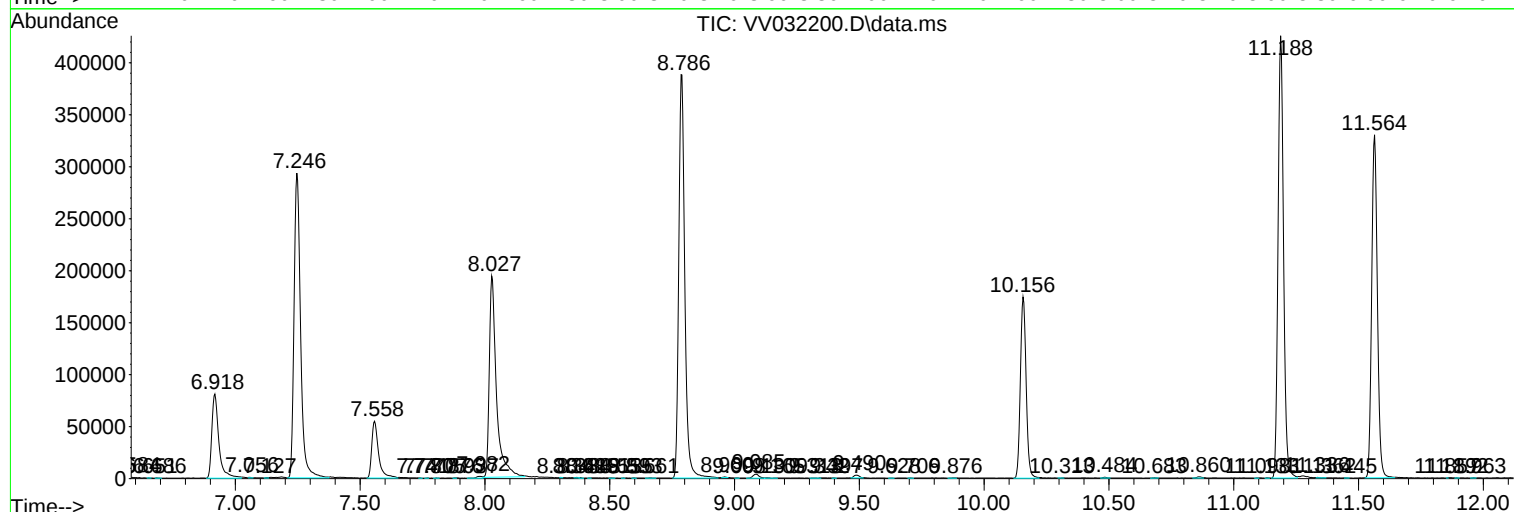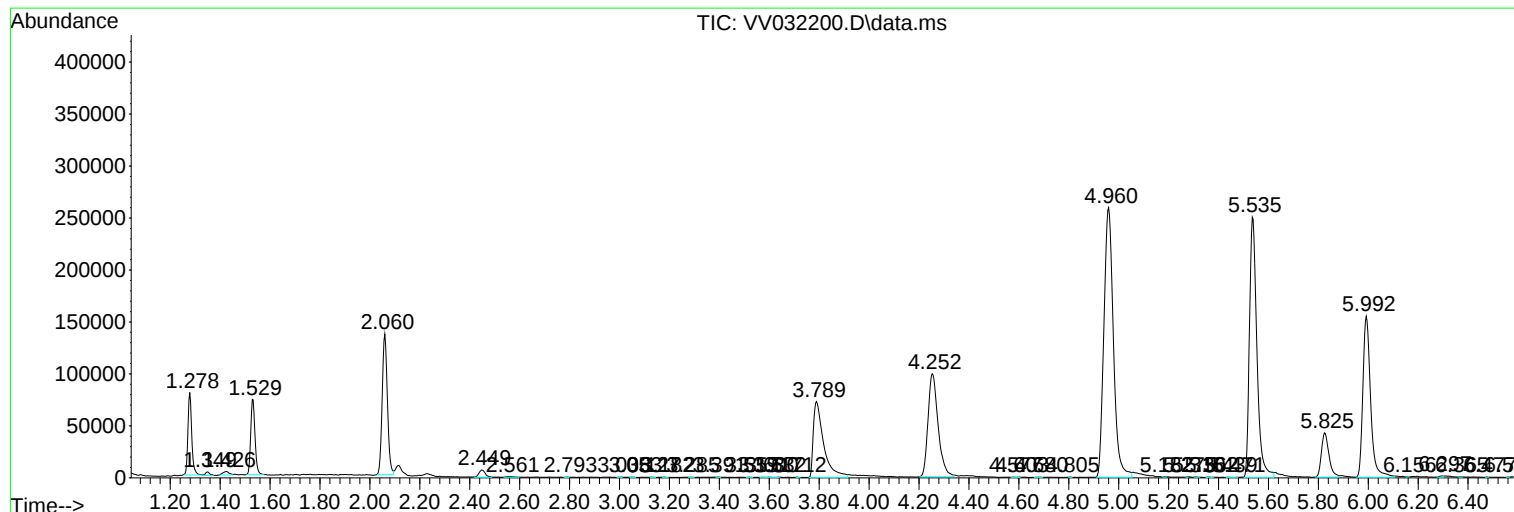

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032200.D
Acq On : 02 Oct 2023 14:22
Operator : SY/MD
Sample : 04592-05 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032200.D
Acq On : 02 Oct 2023 14:22
Operator : SY/MD
Sample : 04592-05 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------