

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032202.D
 Acq On : 02 Oct 2023 16:36
 Operator : SY/MD
 Sample : VIBLK233
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

Signal : TIC: VV032202.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	36	40	46	rBV	608	523	0.09%	0.010%
2	1.278	67	74	88	rVB	59842	63806	10.54%	1.279%
3	1.529	145	152	167	rVB	60186	73321	12.11%	1.469%
4	2.056	307	316	328	rBV	101342	149810	24.74%	3.002%
5	2.227	362	369	385	rVB	4318	8283	1.37%	0.166%
6	2.352	405	408	411	rVB2	255	201	0.03%	0.004%
7	2.378	411	416	419	rVB2	522	419	0.07%	0.008%
8	2.397	419	422	428	rBV3	687	568	0.09%	0.011%
9	2.445	429	437	448	rVB2	5636	9500	1.57%	0.190%
10	2.571	471	476	478	rVB3	253	213	0.04%	0.004%
11	2.690	511	513	517	rVB2	248	172	0.03%	0.003%
12	2.709	517	519	520	rBV2	288	149	0.02%	0.003%
13	2.854	562	564	566	rVV2	247	148	0.02%	0.003%
14	2.905	568	580	584	rVV4	680	1302	0.22%	0.026%
15	2.925	584	586	589	rVV2	501	359	0.06%	0.007%
16	2.947	591	593	595	rVV2	386	180	0.03%	0.004%
17	2.966	595	599	600	rVV2	328	239	0.04%	0.005%
18	3.060	625	628	632	rBV	238	178	0.03%	0.004%
19	3.195	665	670	671	rBV	200	181	0.03%	0.004%
20	3.362	716	722	723	rBV	140	135	0.02%	0.003%
21	3.397	730	733	735	rBV2	143	130	0.02%	0.003%
22	3.503	760	766	769	rBV2	226	293	0.05%	0.006%
23	3.519	769	771	775	rVV2	183	163	0.03%	0.003%
24	3.661	810	815	818	rBV2	261	196	0.03%	0.004%
25	3.786	842	854	888	rBV	61398	167845	27.72%	3.364%
26	4.249	979	998	1021	rBV	96523	247523	40.88%	4.961%
27	4.542	1086	1089	1097	rVB2	343	371	0.06%	0.007%
28	4.577	1097	1100	1103	rBV	266	214	0.04%	0.004%
29	4.632	1114	1117	1122	rVB3	236	186	0.03%	0.004%
30	4.677	1129	1131	1137	rVB2	271	183	0.03%	0.004%
31	4.744	1148	1152	1156	rVB2	261	234	0.04%	0.005%
32	4.770	1157	1160	1161	rBV	285	136	0.02%	0.003%
33	4.799	1167	1169	1171	rBV	333	184	0.03%	0.004%
34	4.957	1201	1218	1244	rBV2	227722	605486	100.00%	12.135%
35	5.195	1290	1292	1294	rVB2	348	167	0.03%	0.003%
36	5.313	1324	1329	1330	rBV	298	236	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032202.D
 Acq On : 02 Oct 2023 16:36
 Operator : SY/MD
 Sample : VIBLK233
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

37	5.355	1339	1342	1345	rVB	189	132	0.02%	0.003%
38	5.381	1345	1350	1354	rBV3	201	238	0.04%	0.005%
39	5.535	1386	1398	1420	rBV	209651	437082	72.19%	8.760%
40	5.825	1477	1488	1516	rVB3	12352	28459	4.70%	0.570%
41	5.989	1525	1539	1579	rBV	139249	302899	50.03%	6.070%
42	6.275	1625	1628	1632	rVB2	267	154	0.03%	0.003%
43	6.320	1640	1642	1647	rVB3	406	251	0.04%	0.005%
44	6.468	1686	1688	1694	rVB2	359	240	0.04%	0.005%
45	6.493	1694	1696	1702	rBV2	224	207	0.03%	0.004%
46	6.574	1716	1721	1723	rBV2	742	584	0.10%	0.012%
47	6.667	1746	1750	1755	rVB4	340	355	0.06%	0.007%
48	6.715	1762	1765	1770	rBV2	231	156	0.03%	0.003%
49	6.915	1815	1827	1855	rBV	71699	140553	23.21%	2.817%
50	7.063	1871	1873	1880	rVB4	459	423	0.07%	0.008%
51	7.133	1889	1895	1899	rBV4	543	724	0.12%	0.015%
52	7.172	1902	1907	1908	rBV3	1800	1413	0.23%	0.028%
53	7.246	1918	1930	1962	rBV	238629	437923	72.33%	8.776%
54	7.442	1988	1991	1998	rVB3	458	401	0.07%	0.008%
55	7.555	2015	2026	2058	rBV	49342	93573	15.45%	1.875%
56	7.664	2058	2060	2067	rVB5	381	340	0.06%	0.007%
57	7.731	2078	2081	2083	rVB	411	210	0.03%	0.004%
58	7.754	2083	2088	2091	rBV3	301	235	0.04%	0.005%
59	7.799	2099	2102	2103	rBV2	296	144	0.02%	0.003%
60	7.870	2122	2124	2128	rVV	308	270	0.04%	0.005%
61	7.982	2155	2159	2164	rBV2	880	891	0.15%	0.018%
62	8.027	2164	2173	2206	rBV	165032	333733	55.12%	6.688%
63	8.310	2259	2261	2265	rVB	361	132	0.02%	0.003%
64	8.346	2270	2272	2276	rVB3	464	281	0.05%	0.006%
65	8.387	2282	2285	2289	rVB3	250	170	0.03%	0.003%
66	8.436	2296	2300	2304	rVB2	451	393	0.06%	0.008%
67	8.458	2304	2307	2309	rBV2	196	156	0.03%	0.003%
68	8.490	2315	2317	2318	rVV2	382	164	0.03%	0.003%
69	8.500	2318	2320	2325	rVV2	342	243	0.04%	0.005%
70	8.526	2326	2328	2331	rVB	322	146	0.02%	0.003%
71	8.786	2398	2409	2431	rBV	332042	549151	90.70%	11.006%
72	9.011	2475	2479	2480	rBV2	335	276	0.05%	0.006%
73	9.021	2480	2482	2483	rVB	404	141	0.02%	0.003%
74	9.233	2544	2548	2553	rBV2	303	259	0.04%	0.005%
75	9.384	2592	2595	2602	rVB	206	137	0.02%	0.003%
76	9.577	2652	2655	2659	rVB	217	164	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
 Data File : VV032202.D
 Acq On : 02 Oct 2023 16:36
 Operator : SY/MD
 Sample : VIBLK233
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

77	9.944	2766	2769	2774	rVB2	166	135	0.02%	0.003%
78	10.043	2793	2800	2802	rBV2	203	232	0.04%	0.005%
79	10.156	2822	2835	2855	rBV	206476	327058	54.02%	6.555%
80	10.259	2865	2867	2873	rVB3	271	159	0.03%	0.003%
81	10.683	2996	2999	3003	rBV3	207	171	0.03%	0.003%
82	10.870	3053	3057	3060	rBV2	171	136	0.02%	0.003%
83	11.133	3135	3139	3141	rBV	268	186	0.03%	0.004%
84	11.188	3145	3156	3178	rBV	349664	548142	90.53%	10.985%
85	11.310	3192	3194	3196	rVV	423	171	0.03%	0.003%
86	11.323	3196	3198	3201	rVB2	339	179	0.03%	0.004%
87	11.519	3252	3259	3261	rBV3	603	759	0.13%	0.015%
88	11.564	3261	3273	3294	rVV	279412	443187	73.20%	8.882%
89	11.873	3365	3369	3374	rVV2	211	187	0.03%	0.004%
90	11.898	3374	3377	3380	rVB2	314	178	0.03%	0.004%
91	12.300	3499	3502	3510	rBV4	424	416	0.07%	0.008%
92	12.358	3516	3520	3527	rBV3	300	337	0.06%	0.007%
93	12.390	3527	3530	3532	rBV	242	162	0.03%	0.003%
94	12.802	3656	3658	3663	rVB	281	189	0.03%	0.004%
95	13.783	3960	3963	3965	rBV	268	167	0.03%	0.003%
96	13.850	3982	3984	3987	rVB	285	142	0.02%	0.003%
97	14.049	4044	4046	4051	rVB	246	142	0.02%	0.003%
98	14.111	4062	4065	4067	rBV	243	163	0.03%	0.003%
99	14.439	4161	4167	4170	rBV2	281	355	0.06%	0.007%
100	15.220	4408	4410	4412	rBV3	306	149	0.02%	0.003%




Sum of corrected areas: 4989739

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032202.D
Acq On : 02 Oct 2023 16:36
Operator : SY/MD
Sample : VIBLK233
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

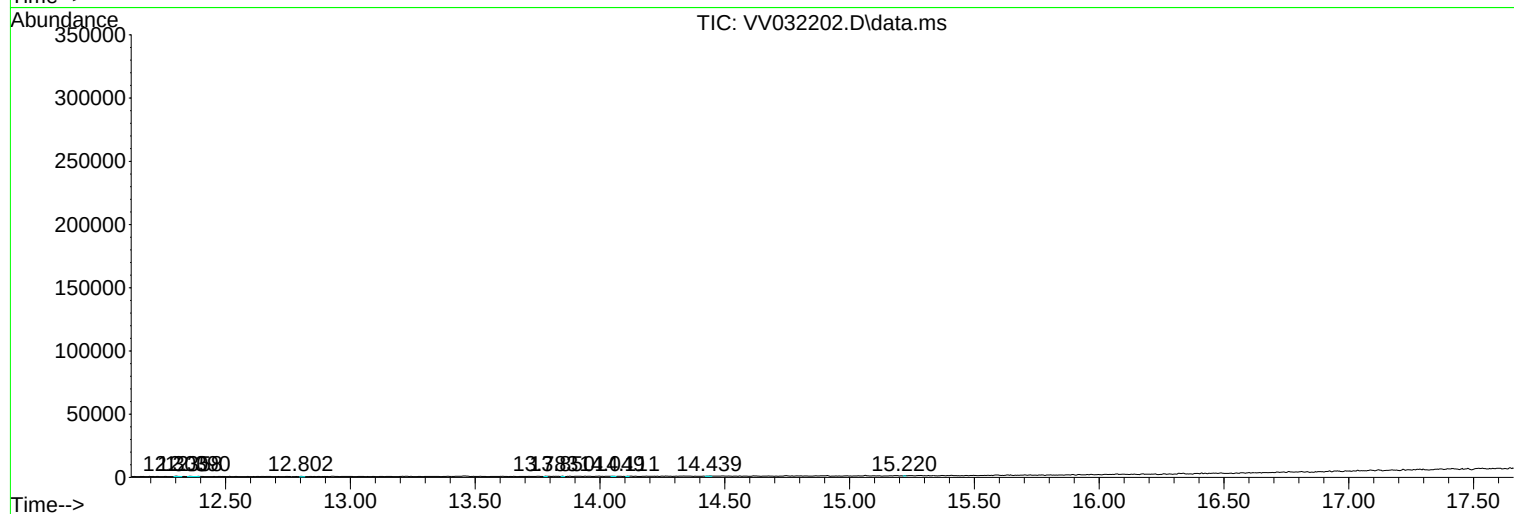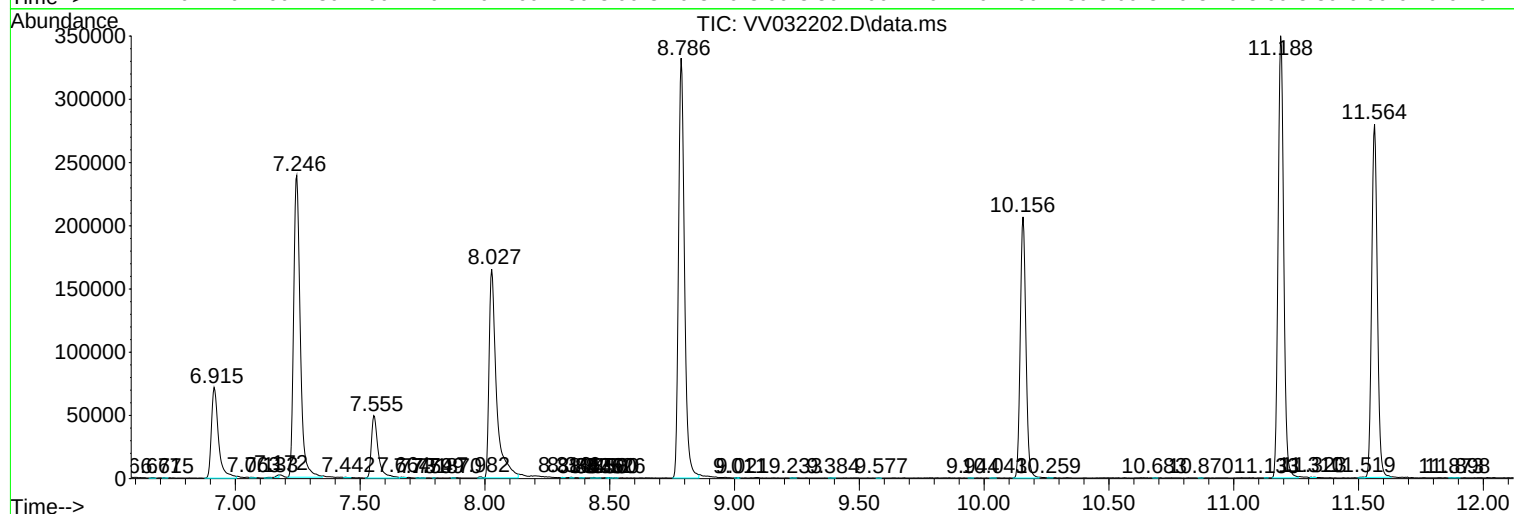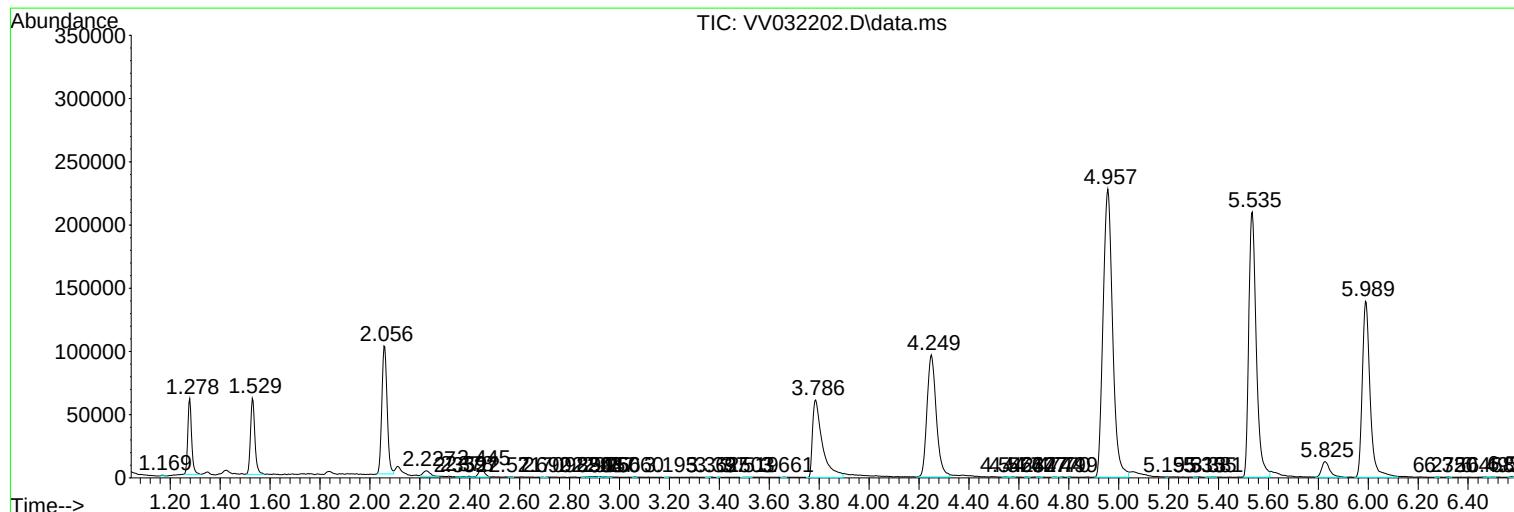

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032202.D
Acq On : 02 Oct 2023 16:36
Operator : SY/MD
Sample : VIBLK233
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032202.D
Acq On : 02 Oct 2023 16:36
Operator : SY/MD
Sample : VIBLK233
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------