


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100223\
Data File : VV032188.D
Acq On : 02 Oct 2023 08:56
Operator : SY/MD
Sample : BFB218
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB218

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Title : VOC Analysis
Last Update : Tue Oct 03 01:57:58 2023

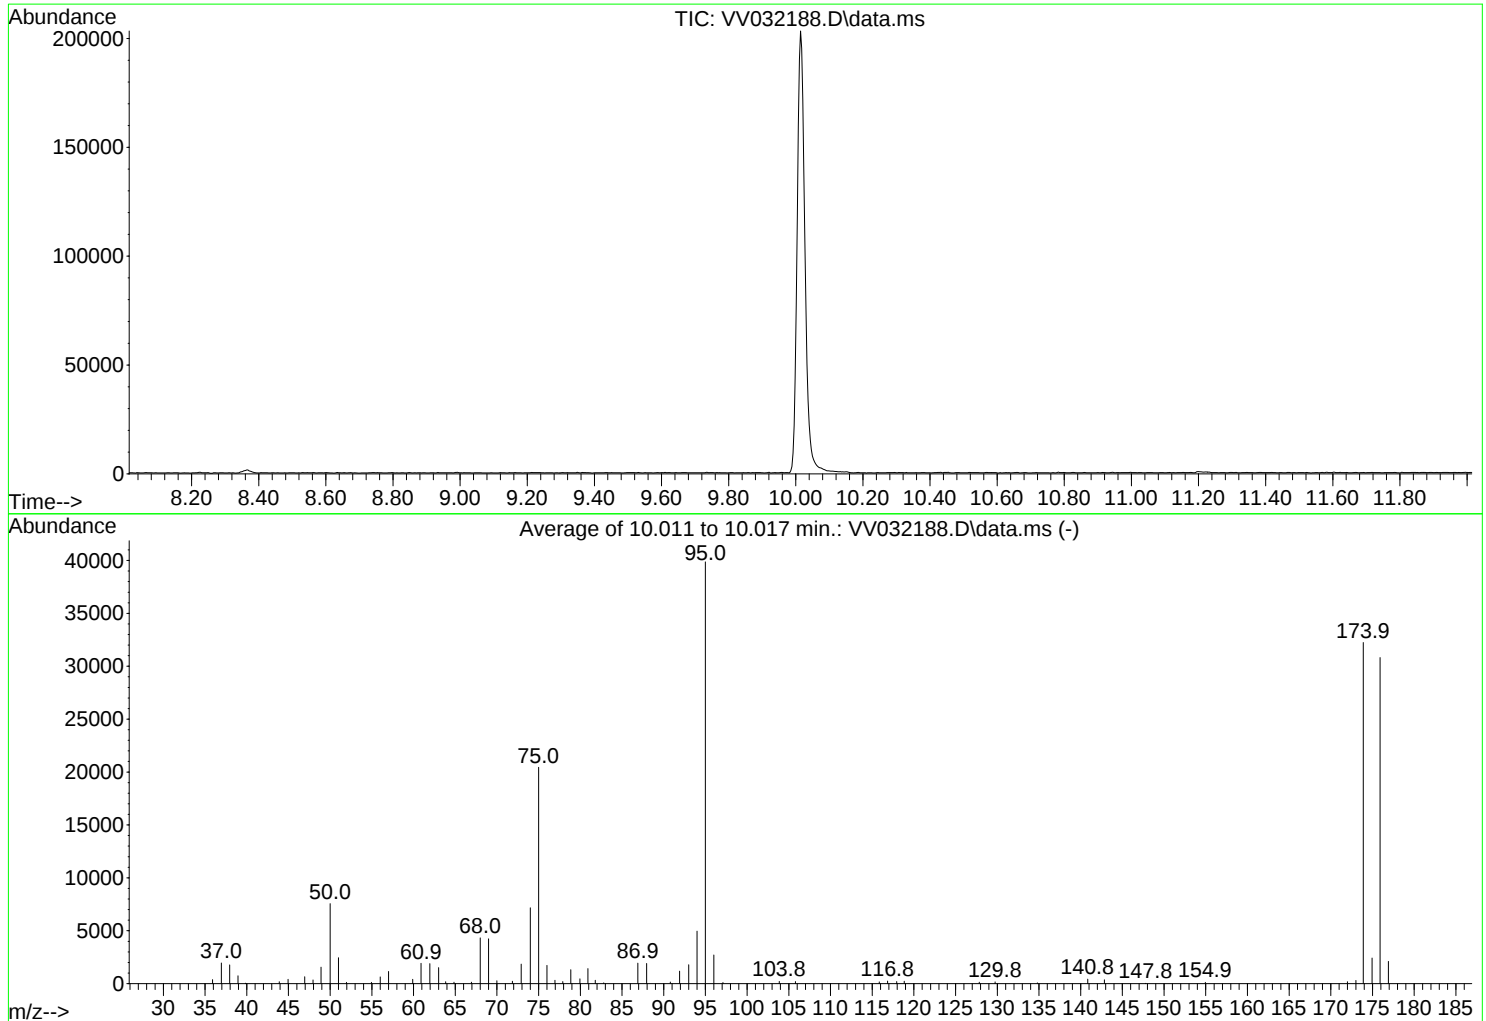

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	7564	PASS
75	95	30	80	51.3	20445	PASS
95	95	100	100	100.0	39869	PASS
96	95	5	9	6.8	2715	PASS
173	174	0.00	2	0.9	301	PASS
174	95	50	120	80.9	32251	PASS
175	174	5	9	7.5	2421	PASS
176	174	95	105	95.6	30827	PASS
177	176	5	10	6.8	2100	PASS

m/z	Abundance
40.00	133.0
43.90	405.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
35.90	360.0
37.00	1943.0
38.00	1755.0
39.00	734.0
39.80	176.0
43.90	613.0
45.00	387.0
47.00	648.0
47.90	342.0
48.90	1579.0
50.00	7685.0
51.00	2378.0
51.90	115.0
55.00	118.0
56.00	625.0
57.00	1068.0
59.90	404.0
60.90	1919.0
61.90	1825.0
63.00	1474.0
63.90	197.0
64.80	142.0
66.90	145.0
68.00	4170.0
69.00	4357.0
70.00	263.0
71.90	218.0
72.90	1733.0
74.00	7066.0
75.00	19832.0
76.00	1650.0
76.90	330.0
77.90	241.0
78.80	1284.0
80.00	440.0
80.90	1392.0
81.80	289.0
82.80	121.0
86.90	2013.0
88.00	1909.0
90.80	163.0
91.90	1176.0
93.00	1748.0
94.00	4857.0
95.00	39016.0
96.00	2737.0
97.10	112.0
103.90	182.0
105.80	188.0
115.90	185.0
116.80	240.0
118.00	178.0
118.90	255.0
127.80	128.0
129.70	155.0
140.80	380.0
142.90	411.0
154.90	115.0
172.00	158.0
173.90	30648.0
174.90	2247.0
175.90	29176.0
176.90	2010.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
35.90	380.0
36.90	2029.0
37.90	1770.0
39.00	767.0
39.80	178.0
43.90	575.0
44.90	427.0
46.90	670.0
48.00	359.0
48.90	1598.0
50.00	7824.0
51.00	2517.0
51.90	118.0
54.90	121.0
56.00	662.0
57.00	1213.0
59.90	419.0
60.90	1995.0
61.90	1935.0
63.00	1570.0
63.80	198.0
64.90	138.0
67.00	149.0
68.00	4496.0
69.00	4420.0
70.00	262.0
71.80	235.0
72.90	1888.0
74.00	7405.0
75.00	21160.0
76.00	1779.0
76.90	321.0
77.90	204.0
78.90	1360.0
79.90	486.0
80.90	1482.0
81.80	323.0
82.80	121.0
86.90	2019.0
88.00	1988.0
90.80	155.0
91.90	1224.0
93.00	1862.0
94.00	5137.0
95.00	41256.0
96.00	2806.0
97.10	113.0
103.90	230.0
105.80	203.0
115.90	167.0
116.90	253.0
118.00	196.0
118.90	237.0
127.80	135.0
129.80	174.0
134.80	103.0
140.90	430.0
142.80	356.0
155.00	129.0
171.90	183.0
173.00	433.0
173.90	33448.0
174.90	2510.0
175.90	31912.0
176.90	2198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
35.90	378.0
36.90	1870.0
37.90	1769.0
38.90	732.0
39.80	167.0
43.90	579.0
44.90	431.0
46.90	644.0
47.90	339.0
48.90	1507.0
50.00	7183.0
51.00	2440.0
52.00	109.0
54.90	138.0
56.00	641.0
57.00	1186.0
59.90	407.0
60.90	1845.0
62.00	1897.0
63.00	1502.0
63.80	169.0
64.90	137.0
67.00	129.0
68.00	4295.0
69.00	3951.0
70.00	279.0
71.90	220.0
72.90	1905.0
74.00	7035.0
75.00	20344.0
76.00	1770.0
77.00	296.0
77.90	165.0
78.80	1321.0
79.90	447.0
80.90	1409.0
81.80	345.0
86.90	1765.0
87.90	1832.0
90.80	149.0
91.90	1128.0
93.00	1758.0
94.00	4867.0
95.00	39336.0
96.00	2603.0
97.10	105.0
103.80	231.0
105.80	210.0
115.80	146.0
116.90	244.0
117.90	196.0
118.80	212.0
127.90	147.0
129.80	175.0
134.80	113.0
140.90	451.0
142.80	312.0
147.80	109.0
155.00	125.0
172.10	193.0
173.00	471.0
173.90	32656.0
175.00	2506.0
175.90	31392.0
176.90	2092.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218