

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100318\
 Data File : VV008047.D
 Acq On : 03 Oct 2018 12:57
 Operator : SY/MD
 Sample : J5182-21
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JLC90

Quant Time: Oct 04 08:13:10 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Oct 04 07:54:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	87326	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	84221	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	40322	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	21812	4.66	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.20%
7) Chloroethane-d5	1.59	69	20278	5.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.20%
11) 1,1-Dichloroethene-d2	2.14	63	35268	3.34	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.80%
20) 2-Butanone-d5	3.97	46	68729	48.81	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.62%
24) Chloroform-d	4.41	84	52091	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
26) 1,2-Dichloroethane-d4	5.09	65	28066	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
32) Benzene-d6	5.10	84	101191	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
36) 1,2-Dichloropropane-d6	6.12	67	32248	5.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.20%
41) Toluene-d8	7.36	98	93159	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
43) trans-1,3-Dichloropropene-	7.67	79	10998	4.48	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.60%
46) 2-Hexanone-d5	8.14	63	46823	43.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.44%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21927	4.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	39422	5.05	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.00%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	6307	0.983 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100318\
Data File : VV008047.D
Acq On : 03 Oct 2018 12:57
Operator : SY/MD
Sample : J5182-21
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JLC90

Quant Time: Oct 04 08:13:10 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 04 07:54:45 2018
Response via : Initial Calibration

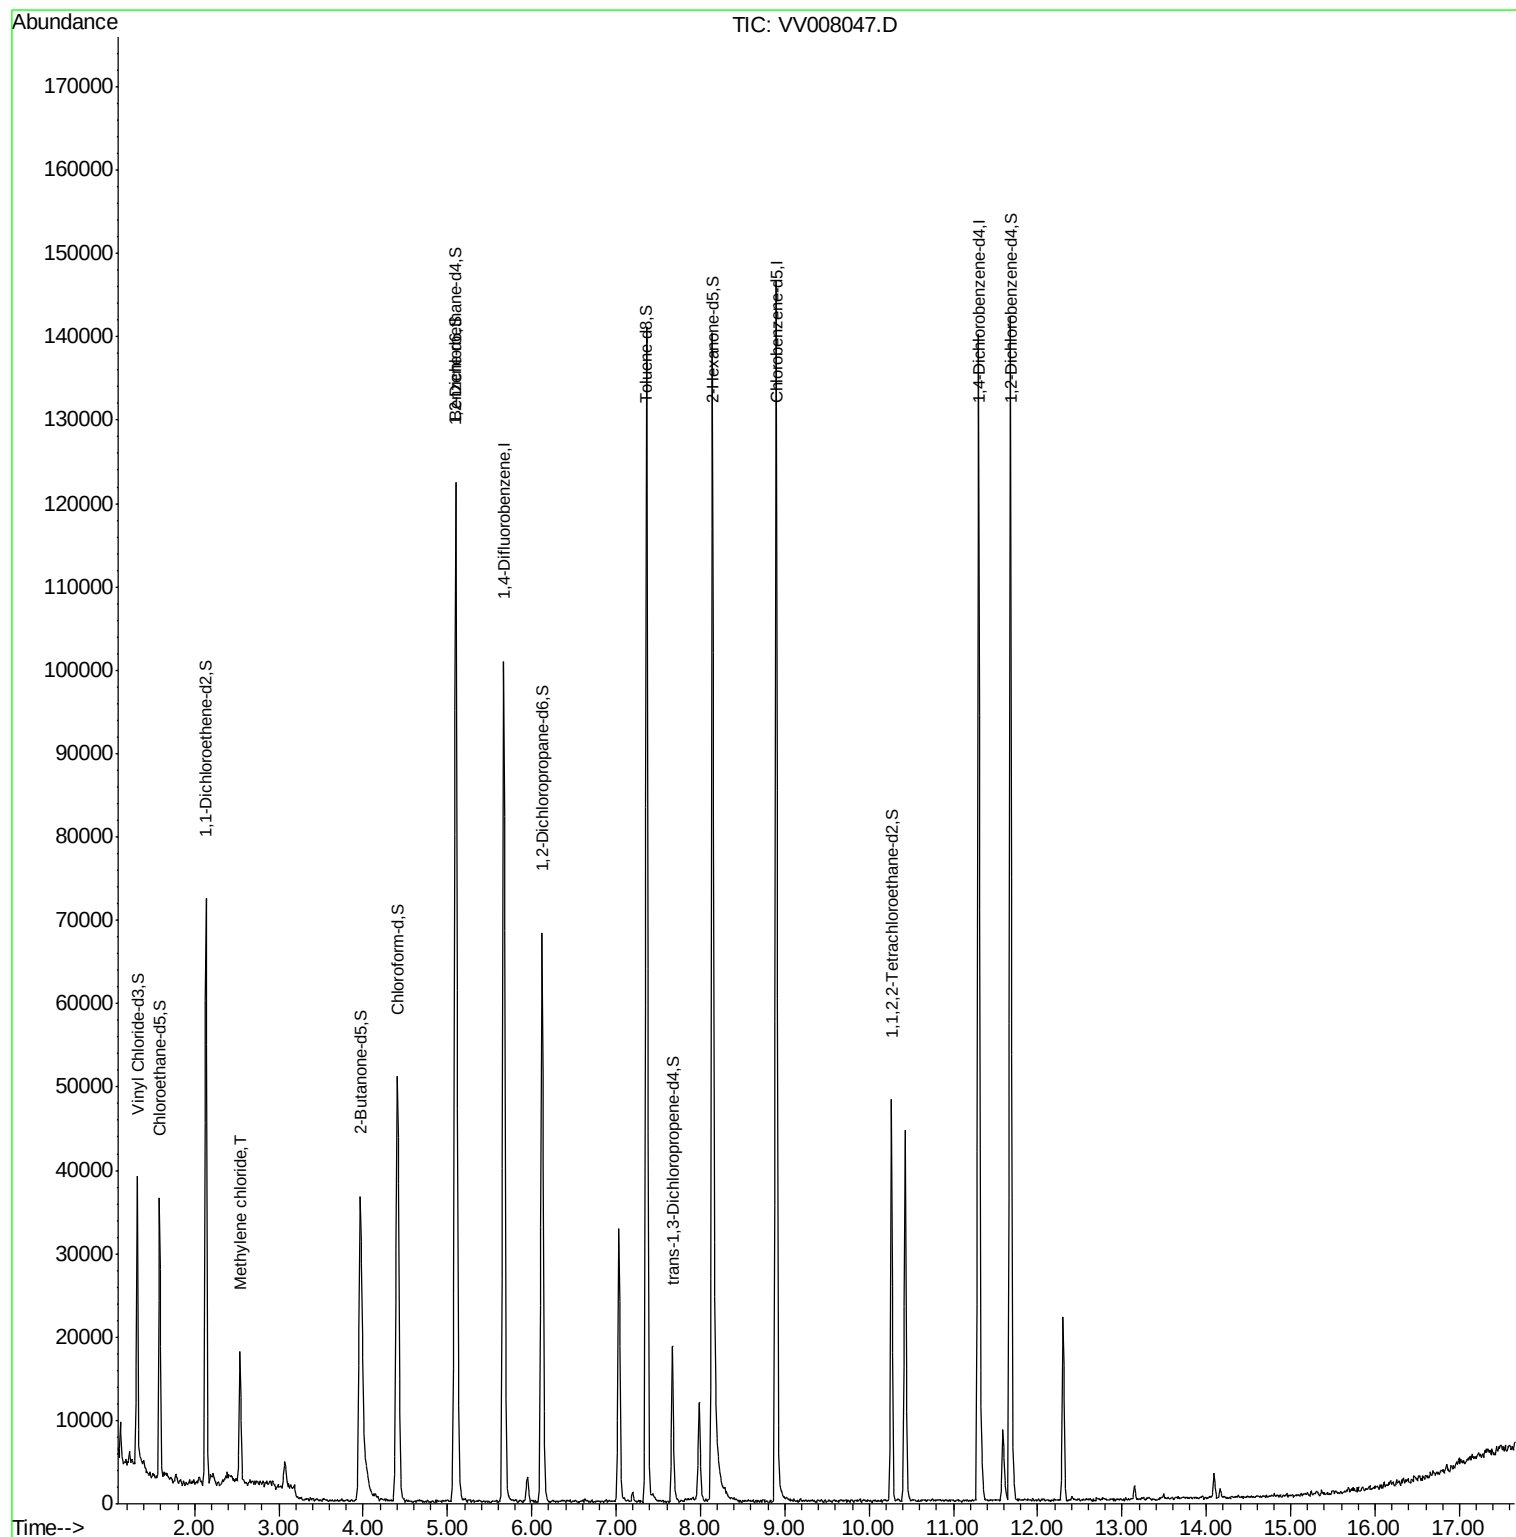

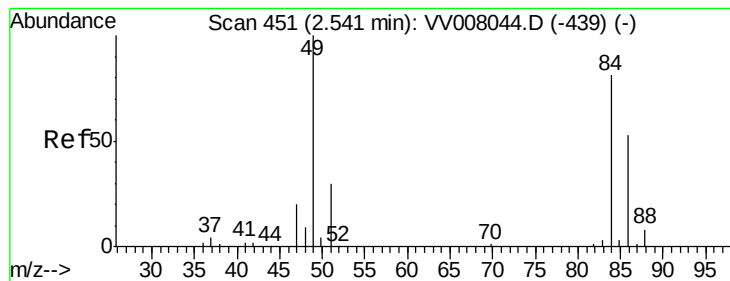

#16
 Methvlene chloride
 Concen: 0.983 ug/L
 RT: 2.54 min Scan# 451
 Delta R.T. 0.00 min
 Lab File: VV008047.D
 Acq: 03 Oct 2018 12:57

Instrument :
 MSVOA_V
 ClientSampleId :
 JLC90

Tot Ion: 84 Resp: 6307
 Ion Ratio Lower Upper
 84 100
 86 69.2 47.3 87.8
 49 130.6 90.0 167.2

