

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100318\
 Data File : VV008049.D
 Acq On : 03 Oct 2018 14:50
 Operator : SY/MD
 Sample : J5160-10DL 40X
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GACB3DL

Quant Time: Oct 04 08:21:53 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Oct 04 07:54:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	84169	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	81271	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	39441	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	21237	4.71	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.20%
7) Chloroethane-d5	1.59	69	19367	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.40%
11) 1,1-Dichloroethene-d2	2.14	63	35743	3.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.20%
20) 2-Butanone-d5	3.96	46	73852	54.42	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.84%
24) Chloroform-d	4.41	84	53808	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.80%
26) 1,2-Dichloroethane-d4	5.09	65	28342	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.20%
32) Benzene-d6	5.10	84	103087	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.20%
36) 1,2-Dichloropropane-d6	6.13	67	33180	5.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.80%
41) Toluene-d8	7.36	98	94442	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.60%
43) trans-1,3-Dichloropropene-	7.67	79	11326	4.78	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.60%
46) 2-Hexanone-d5	8.14	63	50003	47.83	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.66%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	23857	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	39654	5.19	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.80%


Target Compounds					Ovalue
47) Tetrachloroethene	8.02	164	39263	6.359 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100318\
Data File : VV008049.D
Acq On : 03 Oct 2018 14:50
Operator : SY/MD
Sample : J5160-10DL 40X
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GACB3DL

Quant Time: Oct 04 08:21:53 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 04 07:54:45 2018
Response via : Initial Calibration

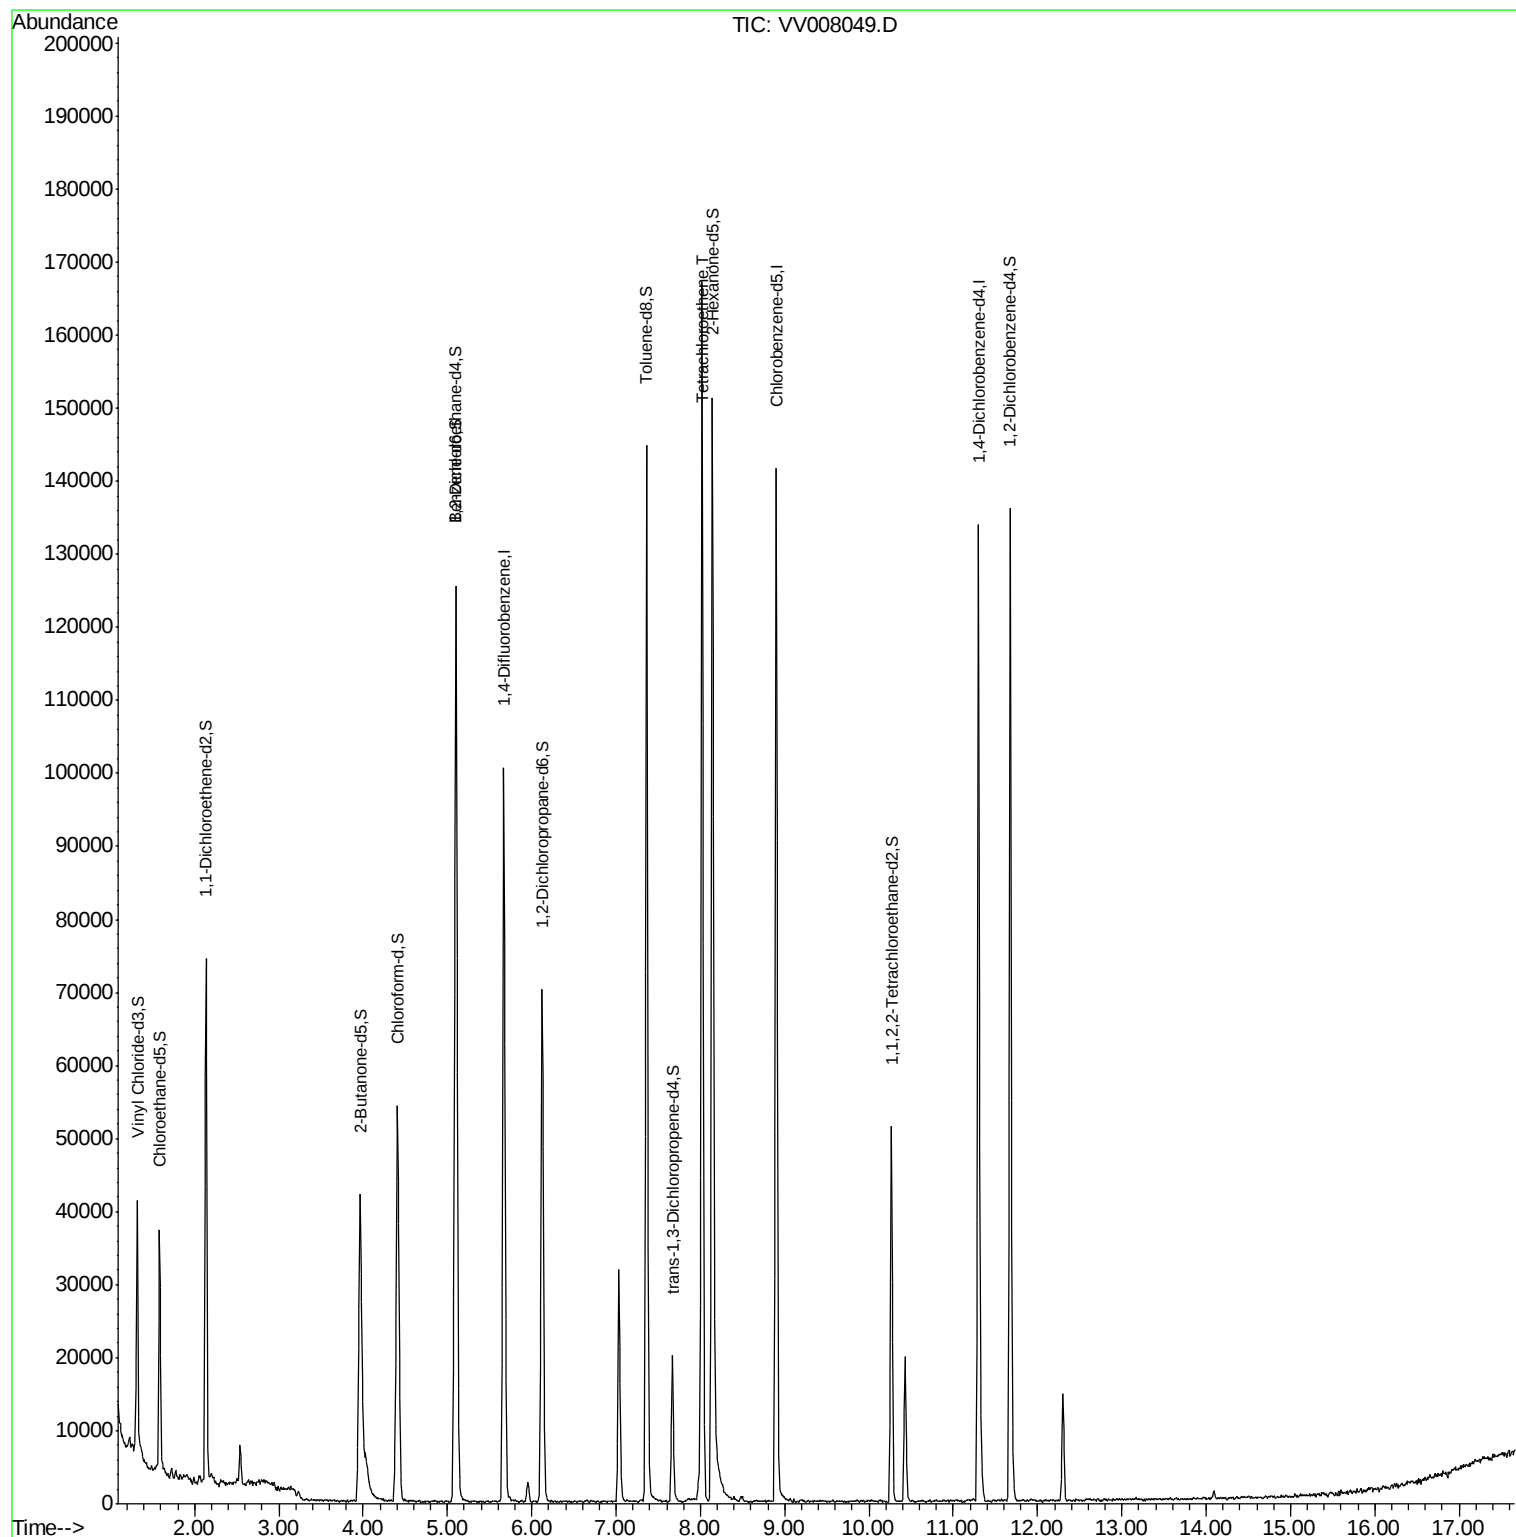

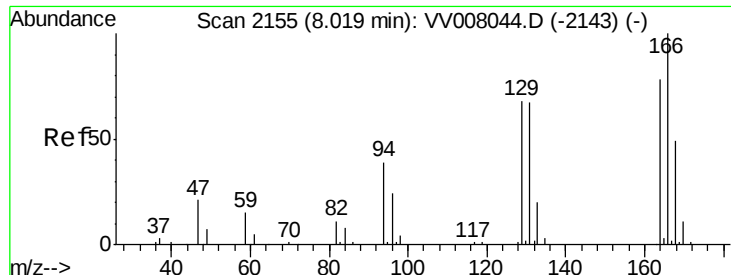

#47

Tetrachloroethene

Concen: 6.359 ug/L

RT: 8.02 min Scan# 2156

Delta R.T. 0.00 min

Lab File: VV008049.D


Acq: 03 Oct 2018 14:50

Instrument :

MSVOA_V

ClientSampleId :

GACB3DL

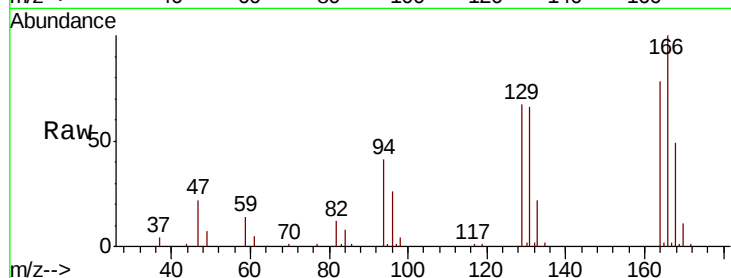

Tot Ion:164 Resp: 39263


Ion Ratio Lower Upper

164 100

129 85.9 59.2 110.0

131 84.1 57.1 106.1

166 128.1 88.6 164.6

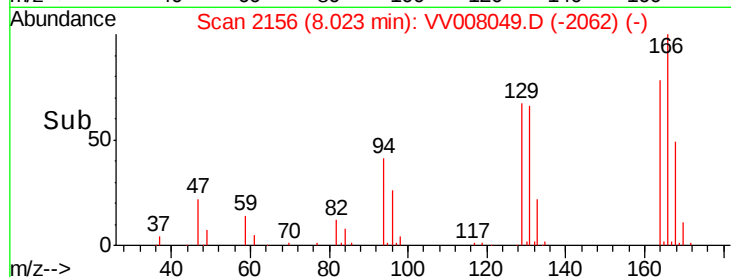

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

