


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100318\
Data File : VV008043.D
Acq On : 03 Oct 2018 09:17
Operator : SY/MD
Sample : BFB01
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB01

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Oct 08 02:28:16 2018

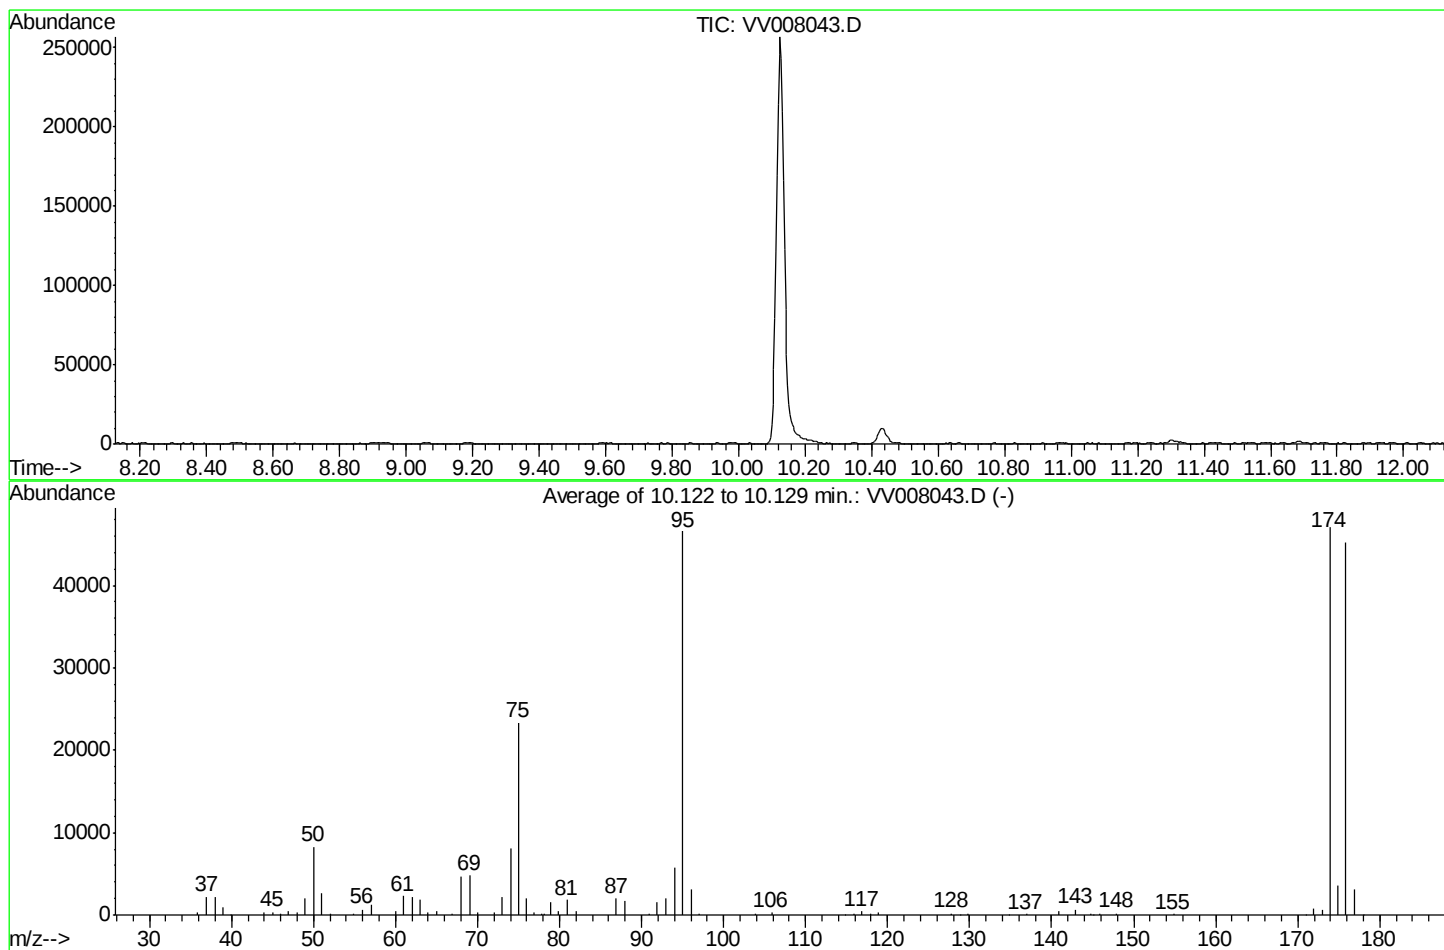

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	8266	PASS
75	95	30	80	50.1	23325	PASS
95	95	100	100	100.0	46592	PASS
96	95	5	9	6.6	3089	PASS
173	174	0.00	2	1.4	644	PASS
174	95	50	120	101.0	47053	PASS
175	174	5	9	7.6	3561	PASS
176	174	95	101	96.1	45229	PASS
177	176	5	9	6.7	3045	PASS

m/z	Abundance
43.90	272.0

Instrument :
MSVOA_V
ClientSampleId :
BFB01

m/z	Abundance
35.90	391.0
37.00	2275.0
38.00	2302.0
39.00	983.0
44.00	554.0
45.00	386.0
46.00	103.0
46.80	517.0
48.00	380.0
48.90	1998.0
50.00	8314.0
51.00	2651.0
52.00	169.0
54.90	142.0
55.90	673.0
57.00	1192.0
59.90	490.0
61.00	2347.0
62.00	2186.0
63.00	1983.0
63.90	297.0
65.00	477.0
66.90	178.0
68.00	4658.0
69.00	4764.0
70.00	363.0
72.00	344.0
73.00	2108.0
74.00	8091.0
75.00	23264.0
76.00	1987.0
76.80	325.0
77.80	176.0
78.90	1595.0
79.90	482.0
80.90	1797.0
81.90	422.0
86.90	2027.0
87.90	1773.0
91.00	241.0
91.90	1557.0
92.90	2217.0
94.00	5659.0
95.00	46120.0
96.00	3039.0
96.90	163.0
103.80	185.0
105.80	306.0
115.90	209.0
116.90	452.0
117.80	187.0
118.80	281.0
127.80	208.0
128.90	103.0
129.90	146.0
134.80	121.0
136.90	120.0
140.90	491.0
142.90	685.0
144.80	192.0
145.80	104.0
147.90	160.0
154.90	129.0
171.90	768.0
173.00	647.0
173.90	45872.0
174.90	3670.0
175.90	43656.0
176.90	2995.0

Instrument :
MSVOA_V
ClientSampleId :
BFB01

m/z	Abundance
35.90	387.0
37.00	2286.0
38.00	2249.0
39.00	1020.0
44.00	570.0
45.00	406.0
46.00	138.0
46.90	530.0
48.00	347.0
48.90	2052.0
50.00	8541.0
51.00	2729.0
52.00	170.0
54.90	177.0
55.90	664.0
57.00	1306.0
60.00	516.0
61.00	2384.0
62.00	2241.0
63.00	1992.0
63.90	286.0
65.00	509.0
66.90	165.0
68.00	4789.0
69.00	4937.0
70.00	355.0
72.00	363.0
73.00	2182.0
74.00	8305.0
75.00	24008.0
76.00	2177.0
76.80	322.0
77.70	145.0
78.10	164.0
78.90	1620.0
79.90	488.0
80.90	1873.0
82.00	431.0
86.90	2065.0
87.90	1747.0
91.00	241.0
91.90	1708.0
92.90	2120.0
94.00	5863.0
95.00	47968.0
96.00	3220.0
97.00	149.0
103.80	196.0
105.90	315.0
114.80	111.0
115.80	203.0
116.90	449.0
117.90	186.0
118.80	312.0
127.80	203.0
128.90	115.0
129.80	154.0
134.90	112.0
136.90	137.0
140.90	530.0
142.90	699.0
144.80	154.0
145.90	105.0
148.00	175.0
154.90	148.0
171.00	108.0
171.90	780.0
172.90	664.0
173.90	48624.0
174.90	3668.0
175.90	46592.0
176.90	3175.0

Instrument :
MSVOA_V
ClientSampleId :
BFB01

m/z	Abundance
35.90	344.0
37.00	2092.0
38.00	2010.0
39.00	919.0
39.90	138.0
43.90	554.0
45.00	380.0
46.10	141.0
46.90	538.0
47.90	289.0
48.90	1865.0
50.00	7945.0
51.00	2518.0
52.00	138.0
54.90	181.0
56.00	607.0
57.00	1225.0
60.00	461.0
60.90	2175.0
62.00	2067.0
63.00	1821.0
63.90	252.0
65.00	507.0
66.90	135.0
68.00	4466.0
69.00	4593.0
69.90	354.0
72.00	348.0
73.00	2097.0
74.00	7722.0
75.00	22704.0
76.00	2130.0
76.80	264.0
78.10	168.0
78.90	1530.0
79.90	429.0
80.90	1733.0
82.00	384.0
86.90	1833.0
87.90	1679.0
91.00	203.0
91.90	1586.0
93.00	1904.0
94.00	5524.0
95.00	45688.0
96.00	3010.0
97.00	115.0
103.80	195.0
105.90	282.0
114.80	108.0
115.80	179.0
116.90	392.0
117.90	174.0
118.80	288.0
127.80	167.0
129.80	157.0
136.90	142.0
140.90	516.0
142.90	642.0
145.00	138.0
145.90	101.0
147.90	174.0
154.80	130.0
171.00	105.0
171.90	710.0
172.90	622.0
173.90	46664.0
174.90	3346.0
175.90	45440.0
176.90	2965.0
178.00	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB01