

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100320\
 Data File : VV018653.D
 Acq On : 03 Oct 2020 14:25
 Operator : SY/MD
 Sample : VV1003WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	80	rVB	155705	154562	14.73%	1.839%
2	1.576	144	151	163	rBV	140738	157902	15.05%	1.878%
3	2.119	310	320	347	rVB	287549	436450	41.60%	5.192%
4	2.521	439	445	448	rBV4	1971	2206	0.21%	0.026%
5	2.640	480	482	484	rVV2	246	118	0.01%	0.001%
6	2.659	484	488	496	rVB3	436	455	0.04%	0.005%
7	2.721	505	507	511	rVB	477	223	0.02%	0.003%
8	2.891	558	560	561	rBV	209	72	0.01%	0.001%
9	2.942	573	576	578	rBV	220	139	0.01%	0.002%
10	3.003	594	595	597	rBV	150	50	0.00%	0.001%
11	3.036	604	605	607	rVB	221	82	0.01%	0.001%
12	3.065	608	614	621	rVB3	775	742	0.07%	0.009%
13	3.209	657	659	663	rVB2	365	217	0.02%	0.003%
14	3.264	673	676	679	rBV2	213	150	0.01%	0.002%
15	3.441	728	731	736	rBV	276	240	0.02%	0.003%
16	3.540	759	762	764	rVB	308	173	0.02%	0.002%
17	3.573	769	772	774	rBV	168	117	0.01%	0.001%
18	3.788	835	839	840	rBV2	226	183	0.02%	0.002%
19	3.907	866	876	906	rBV	66492	204916	19.53%	2.438%
20	4.370	1003	1020	1048	rBV	173613	428554	40.85%	5.098%
21	4.669	1111	1113	1116	rBV2	142	79	0.01%	0.001%
22	4.733	1131	1133	1134	rBV2	173	78	0.01%	0.001%
23	4.762	1139	1142	1146	rVV2	239	223	0.02%	0.003%
24	4.782	1146	1148	1151	rVB	320	145	0.01%	0.002%
25	4.888	1179	1181	1184	rBV2	197	88	0.01%	0.001%
26	4.962	1201	1204	1208	rBV	150	149	0.01%	0.002%
27	5.068	1219	1237	1274	rBV2	404575	1049051	100.00%	12.480%
28	5.431	1349	1350	1355	rVB2	283	140	0.01%	0.002%
29	5.508	1370	1374	1379	rBV	633	534	0.05%	0.006%
30	5.637	1400	1414	1438	rBV	366177	728846	69.48%	8.671%
31	5.923	1492	1503	1526	rBV2	36625	72585	6.92%	0.863%
32	6.045	1537	1541	1542	rBV2	373	262	0.02%	0.003%
33	6.090	1542	1555	1586	rVV	234464	474209	45.20%	5.641%
34	6.309	1619	1623	1625	rBV	344	204	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100320\
 Data File : VV018653.D
 Acq On : 03 Oct 2020 14:25
 Operator : SY/MD
 Sample : VV1003WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	6.322	1625	1627	1630	rVB2	258	122	0.01%	0.001%
36	6.383	1642	1646	1649	rBV2	235	222	0.02%	0.003%
37	6.425	1657	1659	1660	rBV	204	73	0.01%	0.001%
38	6.518	1686	1688	1690	rBV	251	105	0.01%	0.001%
39	6.601	1711	1714	1719	rBV2	208	167	0.02%	0.002%
40	6.720	1748	1751	1754	rBV	263	185	0.02%	0.002%
41	6.775	1762	1768	1769	rBV2	193	175	0.02%	0.002%
42	6.843	1787	1789	1793	rBV2	290	201	0.02%	0.002%
43	7.003	1829	1839	1860	rBV	127174	233696	22.28%	2.780%
44	7.219	1903	1906	1911	rBV3	592	646	0.06%	0.008%
45	7.334	1930	1942	1966	rBV	484018	828985	79.02%	9.862%
46	7.588	2017	2021	2027	rBV3	366	385	0.04%	0.005%
47	7.640	2027	2037	2060	rBV	94779	164906	15.72%	1.962%
48	7.807	2087	2089	2093	rVB2	660	402	0.04%	0.005%
49	7.891	2110	2115	2118	rBV2	582	428	0.04%	0.005%
50	7.939	2127	2130	2131	rBV	272	148	0.01%	0.002%
51	7.994	2145	2147	2155	rVB5	697	592	0.06%	0.007%
52	8.058	2165	2167	2172	rVB2	345	160	0.02%	0.002%
53	8.106	2172	2182	2216	rBV2	192499	399448	38.08%	4.752%
54	8.453	2288	2290	2296	rVB4	374	227	0.02%	0.003%
55	8.479	2296	2298	2301	rBV2	339	169	0.02%	0.002%
56	8.637	2345	2347	2350	rVB	274	146	0.01%	0.002%
57	8.678	2358	2360	2363	rVB	205	76	0.01%	0.001%
58	8.772	2388	2389	2392	rBV	152	62	0.01%	0.001%
59	8.871	2407	2420	2444	rBV	571369	925271	88.20%	11.007%
60	9.074	2482	2483	2484	rBV	161	43	0.00%	0.001%
61	9.093	2488	2489	2490	rVB	240	46	0.00%	0.001%
62	9.148	2504	2506	2507	rBV	250	123	0.01%	0.001%
63	9.215	2525	2527	2529	rBV	154	85	0.01%	0.001%
64	9.312	2555	2557	2562	rVB2	325	184	0.02%	0.002%
65	9.428	2590	2593	2596	rBV3	270	190	0.02%	0.002%
66	9.492	2611	2613	2617	rBV2	221	113	0.01%	0.001%
67	9.553	2629	2632	2634	rBV	270	148	0.01%	0.002%
68	9.569	2634	2637	2641	rVB3	520	419	0.04%	0.005%
69	9.624	2650	2654	2659	rBV3	308	356	0.03%	0.004%
70	9.659	2663	2665	2674	rVB	307	321	0.03%	0.004%
71	10.077	2793	2795	2797	rBV	111	60	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100320\
 Data File : VV018653.D
 Acq On : 03 Oct 2020 14:25
 Operator : SY/MD
 Sample : VV1003WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	10.145	2814	2816	2819	rBV	310	98	0.01%	0.001%
73	10.235	2833	2844	2867	rBV	259494	406353	38.74%	4.834%
74	10.334	2872	2875	2878	rBV	362	212	0.02%	0.003%
75	10.707	2989	2991	2997	rBV2	303	258	0.02%	0.003%
76	11.270	3154	3166	3189	rBV	580090	899274	85.72%	10.698%
77	11.646	3270	3283	3307	rBV	524875	820640	78.23%	9.763%
78	11.829	3337	3340	3342	rBV2	445	273	0.03%	0.003%
79	11.913	3364	3366	3367	rBV	278	92	0.01%	0.001%
80	12.129	3431	3433	3436	rBV2	295	108	0.01%	0.001%
81	12.473	3536	3540	3542	rBV2	375	332	0.03%	0.004%
82	12.553	3561	3565	3569	rBV2	318	305	0.03%	0.004%
83	12.672	3595	3602	3611	rBV5	1680	2527	0.24%	0.030%
84	13.225	3771	3774	3776	rVB2	303	170	0.02%	0.002%
85	13.772	3941	3944	3951	rVB4	1415	1575	0.15%	0.019%
86	14.122	4050	4053	4055	rBV3	335	251	0.02%	0.003%
87	14.643	4212	4215	4217	rBV2	597	335	0.03%	0.004%


Sum of corrected areas: 8406032

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100320\
Data File : VV018653.D
Acq On : 03 Oct 2020 14:25
Operator : SY/MD
Sample : VV1003WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

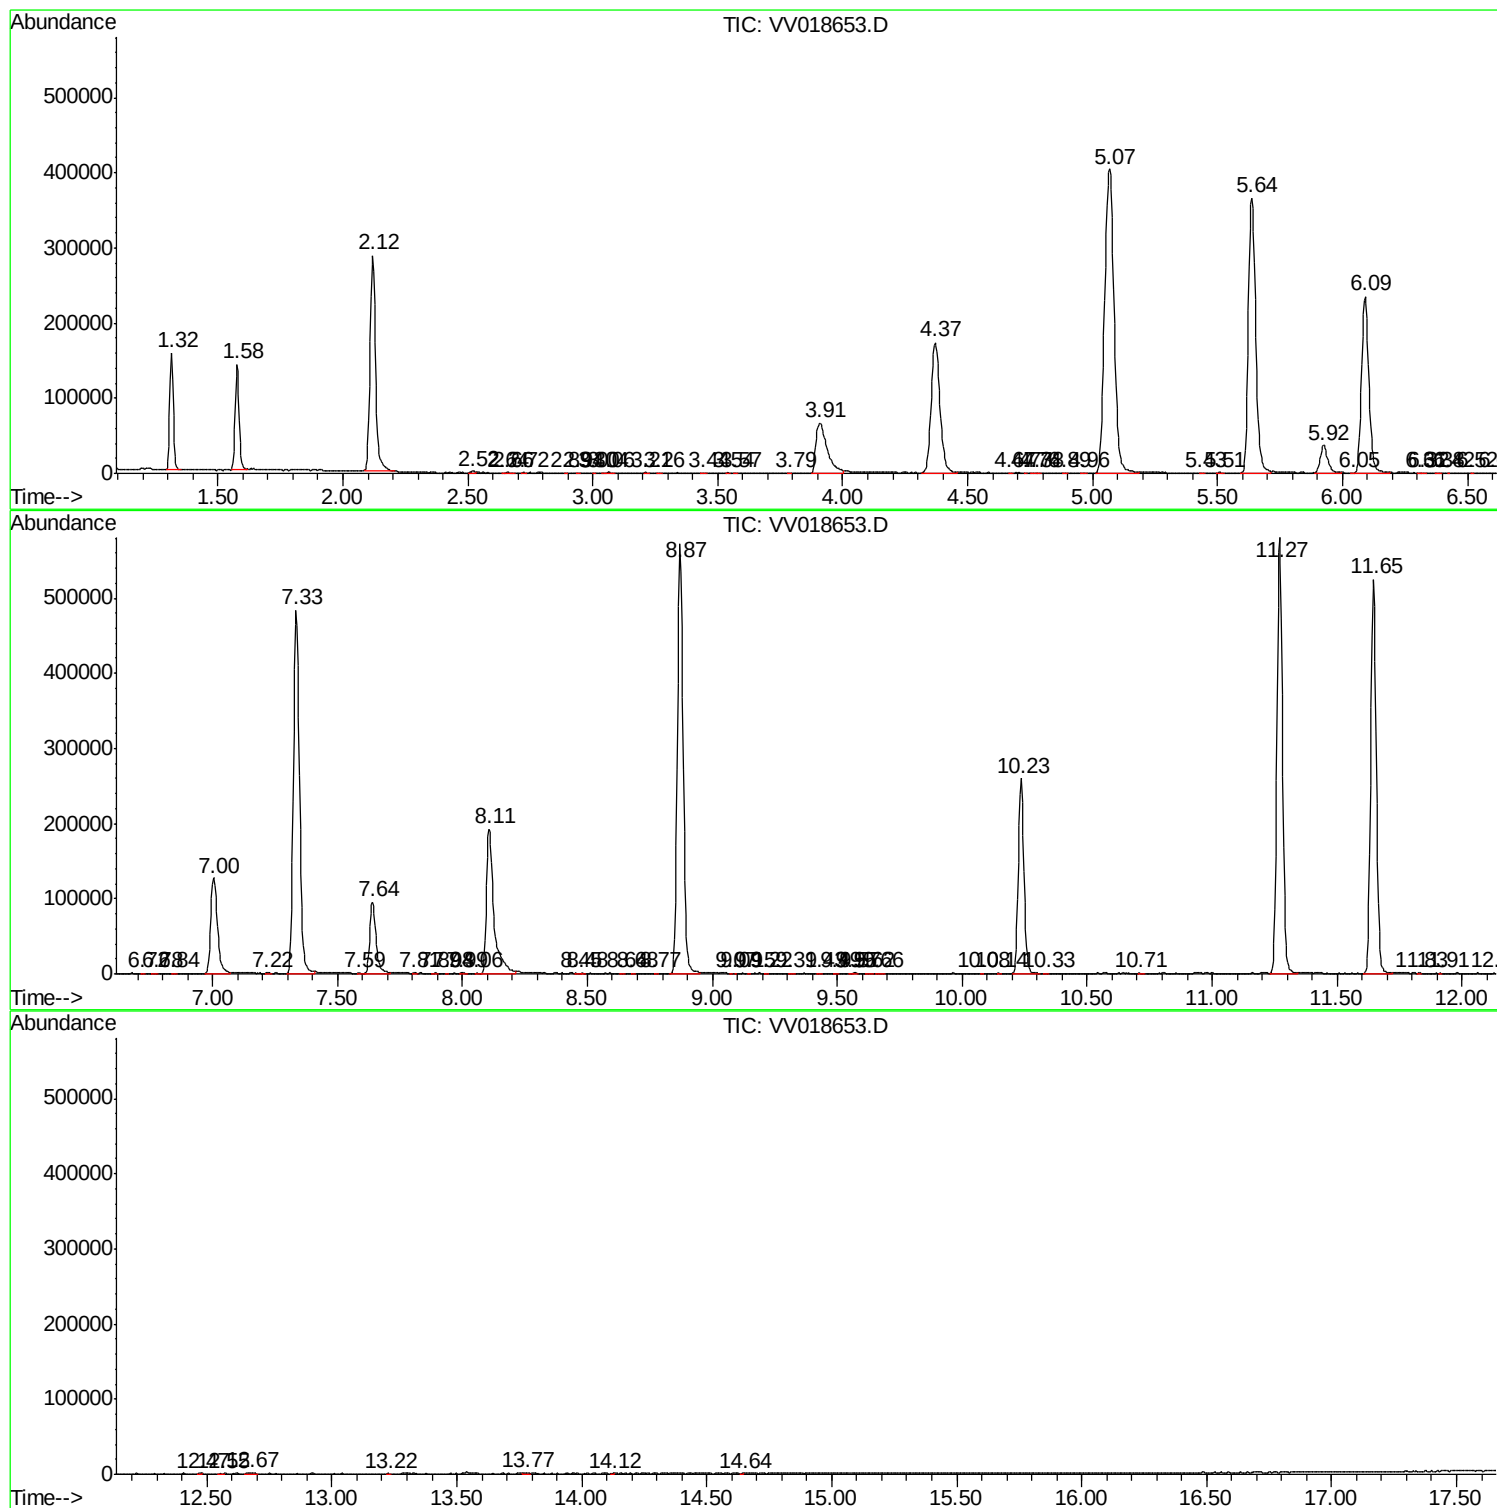

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100320\
Data File : VV018653.D
Acq On : 03 Oct 2020 14:25
Operator : SY/MD
Sample : VV1003WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1










Instrument :
MSVOA_V
ClientSampleId :
VBLK63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propanoic acid, 2,2,3-trich... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.		
5.92	4.98 ug/L	72585	1,4-Difluorobenzene	5.64		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Propanoic acid, 2,2,3-trichloro-...	190	C4H5Cl3O2	004749-35-3	50
2		Ethylene, 1,2-dichloro-, (Z)-	96	C2H2Cl2	000156-59-2	35
3		m-Methoxybenzonitrile	133	C8H7NO	001527-89-5	9
4		Difluoro(methylamino)phosphine s...	131	CH4F2NPS	1000306-16-8	9
5		Dihydro-4,5-dichloro-2(3H)furanone	154	C4H4Cl2O2	114434-99-0	9

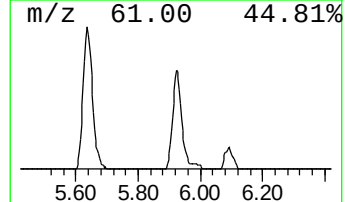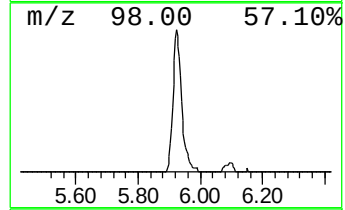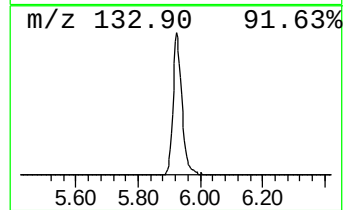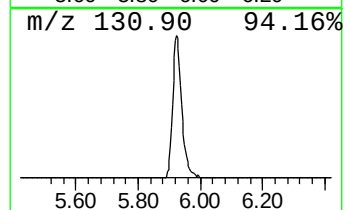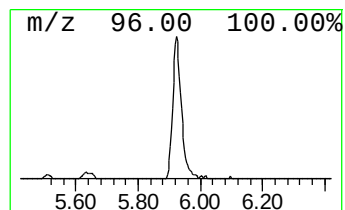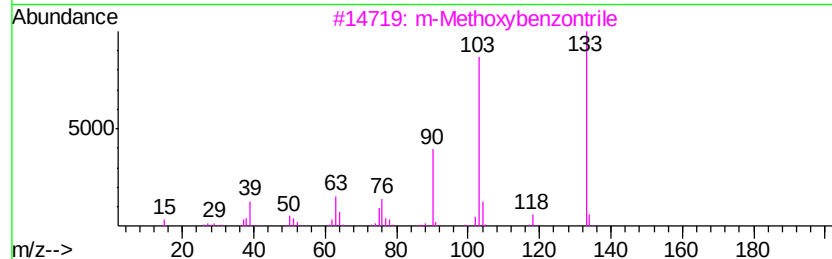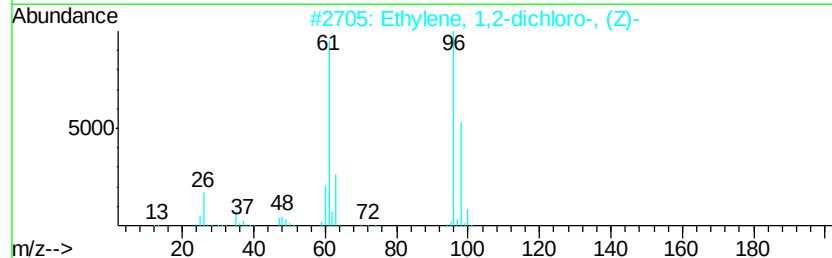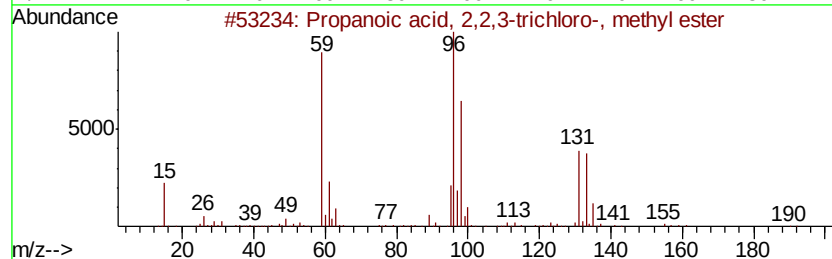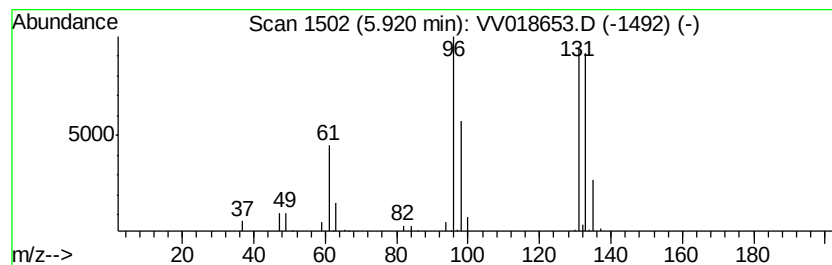

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100320\
Data File : VV018653.D
Acq On : 03 Oct 2020 14:25
Operator : SY/MD
Sample : VV1003WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propanoic acid, 2...	5.92	5.0	ug/L	72585	1	5.64	728846	50.0