

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100320\
 Data File : VV018654.D
 Acq On : 03 Oct 2020 14:59
 Operator : SY/MD
 Sample : L4237-12DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	86	rVB	147199	144961	14.88%	1.682%
2	1.579	144	152	164	rBV	123445	143425	14.72%	1.664%
3	2.119	311	320	354	rVB	262005	408498	41.93%	4.741%
4	2.521	438	445	458	rVB6	2015	3635	0.37%	0.042%
5	2.624	474	477	484	rBV3	571	619	0.06%	0.007%
6	2.952	574	579	582	rBV	361	373	0.04%	0.004%
7	3.003	593	595	600	rVB	348	197	0.02%	0.002%
8	3.052	607	610	611	rBV	251	133	0.01%	0.002%
9	3.251	669	672	675	rBV	184	160	0.02%	0.002%
10	3.373	707	710	713	rBV2	193	137	0.01%	0.002%
11	3.482	741	744	746	rBV2	362	191	0.02%	0.002%
12	3.518	751	755	759	rVV3	291	237	0.02%	0.003%
13	3.566	768	770	773	rVB	321	150	0.02%	0.002%
14	3.672	800	803	805	rBV	105	82	0.01%	0.001%
15	3.913	867	878	914	rBV	59536	198165	20.34%	2.300%
16	4.370	1004	1020	1051	rBV	159942	401331	41.20%	4.657%
17	4.563	1079	1080	1083	rBV	227	125	0.01%	0.001%
18	4.601	1089	1092	1093	rBV	473	202	0.02%	0.002%
19	4.666	1109	1112	1113	rBV	173	77	0.01%	0.001%
20	4.704	1121	1124	1126	rBV	312	146	0.01%	0.002%
21	4.945	1195	1199	1203	rBV	331	325	0.03%	0.004%
22	5.068	1220	1237	1271	rBV2	374698	974200	100.00%	11.305%
23	5.328	1315	1318	1321	rBV2	395	321	0.03%	0.004%
24	5.428	1346	1349	1355	rVB3	445	342	0.04%	0.004%
25	5.453	1355	1357	1360	rBV	177	102	0.01%	0.001%
26	5.473	1361	1363	1368	rVB2	208	141	0.01%	0.002%
27	5.492	1368	1369	1370	rBV	150	40	0.00%	0.000%
28	5.502	1370	1372	1374	rBV2	245	140	0.01%	0.002%
29	5.531	1380	1381	1382	rBV	213	49	0.01%	0.001%
30	5.572	1392	1394	1396	rBV	210	105	0.01%	0.001%
31	5.637	1401	1414	1447	rBV	365690	730440	74.98%	8.477%
32	5.933	1492	1506	1531	rBV3	335858	683613	70.17%	7.933%
33	6.090	1542	1555	1582	rVB2	216427	436085	44.76%	5.061%
34	6.318	1624	1626	1628	rBV2	311	138	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100320\
 Data File : VV018654.D
 Acq On : 03 Oct 2020 14:59
 Operator : SY/MD
 Sample : L4237-12DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	6.463	1668	1671	1673	rBV	262	202	0.02%	0.002%
36	6.588	1705	1710	1712	rBV2	265	265	0.03%	0.003%
37	6.621	1718	1720	1723	rVB2	250	137	0.01%	0.002%
38	6.637	1723	1725	1732	rVB3	345	313	0.03%	0.004%
39	6.678	1732	1738	1739	rBV2	493	475	0.05%	0.006%
40	6.807	1774	1778	1786	rBV2	316	412	0.04%	0.005%
41	6.913	1808	1811	1814	rBV2	202	144	0.01%	0.002%
42	7.003	1828	1839	1859	rBV	118360	213822	21.95%	2.481%
43	7.222	1905	1907	1909	rBV2	261	128	0.01%	0.001%
44	7.283	1921	1926	1928	rBV	321	306	0.03%	0.004%
45	7.334	1930	1942	1964	rBV	443760	766111	78.64%	8.891%
46	7.640	2027	2037	2061	rBV	91429	155511	15.96%	1.805%
47	7.833	2095	2097	2099	rBV	307	181	0.02%	0.002%
48	8.058	2165	2167	2172	rVB2	499	310	0.03%	0.004%
49	8.106	2172	2182	2225	rBV2	181893	381865	39.20%	4.431%
50	8.453	2288	2290	2292	rBV2	294	179	0.02%	0.002%
51	8.492	2297	2302	2303	rBV	359	265	0.03%	0.003%
52	8.572	2325	2327	2331	rVB2	443	279	0.03%	0.003%
53	8.595	2331	2334	2338	rBV2	395	300	0.03%	0.003%
54	8.678	2358	2360	2363	rBV	122	67	0.01%	0.001%
55	8.739	2375	2379	2380	rBV	300	170	0.02%	0.002%
56	8.765	2385	2387	2389	rBV2	191	58	0.01%	0.001%
57	8.871	2408	2420	2446	rBV	571795	925187	94.97%	10.737%
58	9.116	2494	2496	2499	rBV	250	145	0.01%	0.002%
59	9.199	2520	2522	2524	rBV	65	32	0.00%	0.000%
60	9.244	2535	2536	2539	rVB	312	69	0.01%	0.001%
61	9.315	2555	2558	2563	rVB	329	261	0.03%	0.003%
62	9.418	2587	2590	2592	rBV	243	155	0.02%	0.002%
63	9.617	2650	2652	2654	rBV2	125	65	0.01%	0.001%
64	9.672	2667	2669	2670	rBV	168	52	0.01%	0.001%
65	10.045	2781	2785	2787	rBV2	316	253	0.03%	0.003%
66	10.106	2803	2804	2805	rBV	123	32	0.00%	0.000%
67	10.135	2810	2813	2814	rBV2	238	124	0.01%	0.001%
68	10.235	2832	2844	2867	rBV	242136	381107	39.12%	4.423%
69	10.485	2920	2922	2926	rBV2	193	154	0.02%	0.002%
70	10.550	2939	2942	2943	rBV	205	118	0.01%	0.001%
71	11.193	3140	3142	3144	rBV	332	127	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100320\
Data File : VV018654.D
Acq On : 03 Oct 2020 14:59
Operator : SY/MD
Sample : L4237-12DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC7DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Title : VOC Analysis

72	11.270	3155	3166	3189	rBV	576622	893836	91.75%	10.373%
73	11.646	3271	3283	3302	rBV	502336	763439	78.37%	8.860%
74	11.813	3333	3335	3337	rBV	313	143	0.01%	0.002%
75	11.855	3347	3348	3350	rBV2	301	111	0.01%	0.001%
76	12.064	3411	3413	3420	rVB2	420	354	0.04%	0.004%
77	12.579	3570	3573	3575	rBV	272	152	0.02%	0.002%
78	12.614	3582	3584	3587	rBV	280	154	0.02%	0.002%
79	14.759	4248	4251	4253	rBV	492	394	0.04%	0.005%
80	14.906	4295	4297	4299	rBV	401	228	0.02%	0.003%


Sum of corrected areas: 8617077

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100320\
Data File : VV018654.D
Acq On : 03 Oct 2020 14:59
Operator : SY/MD
Sample : L4237-12DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
E0AC7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

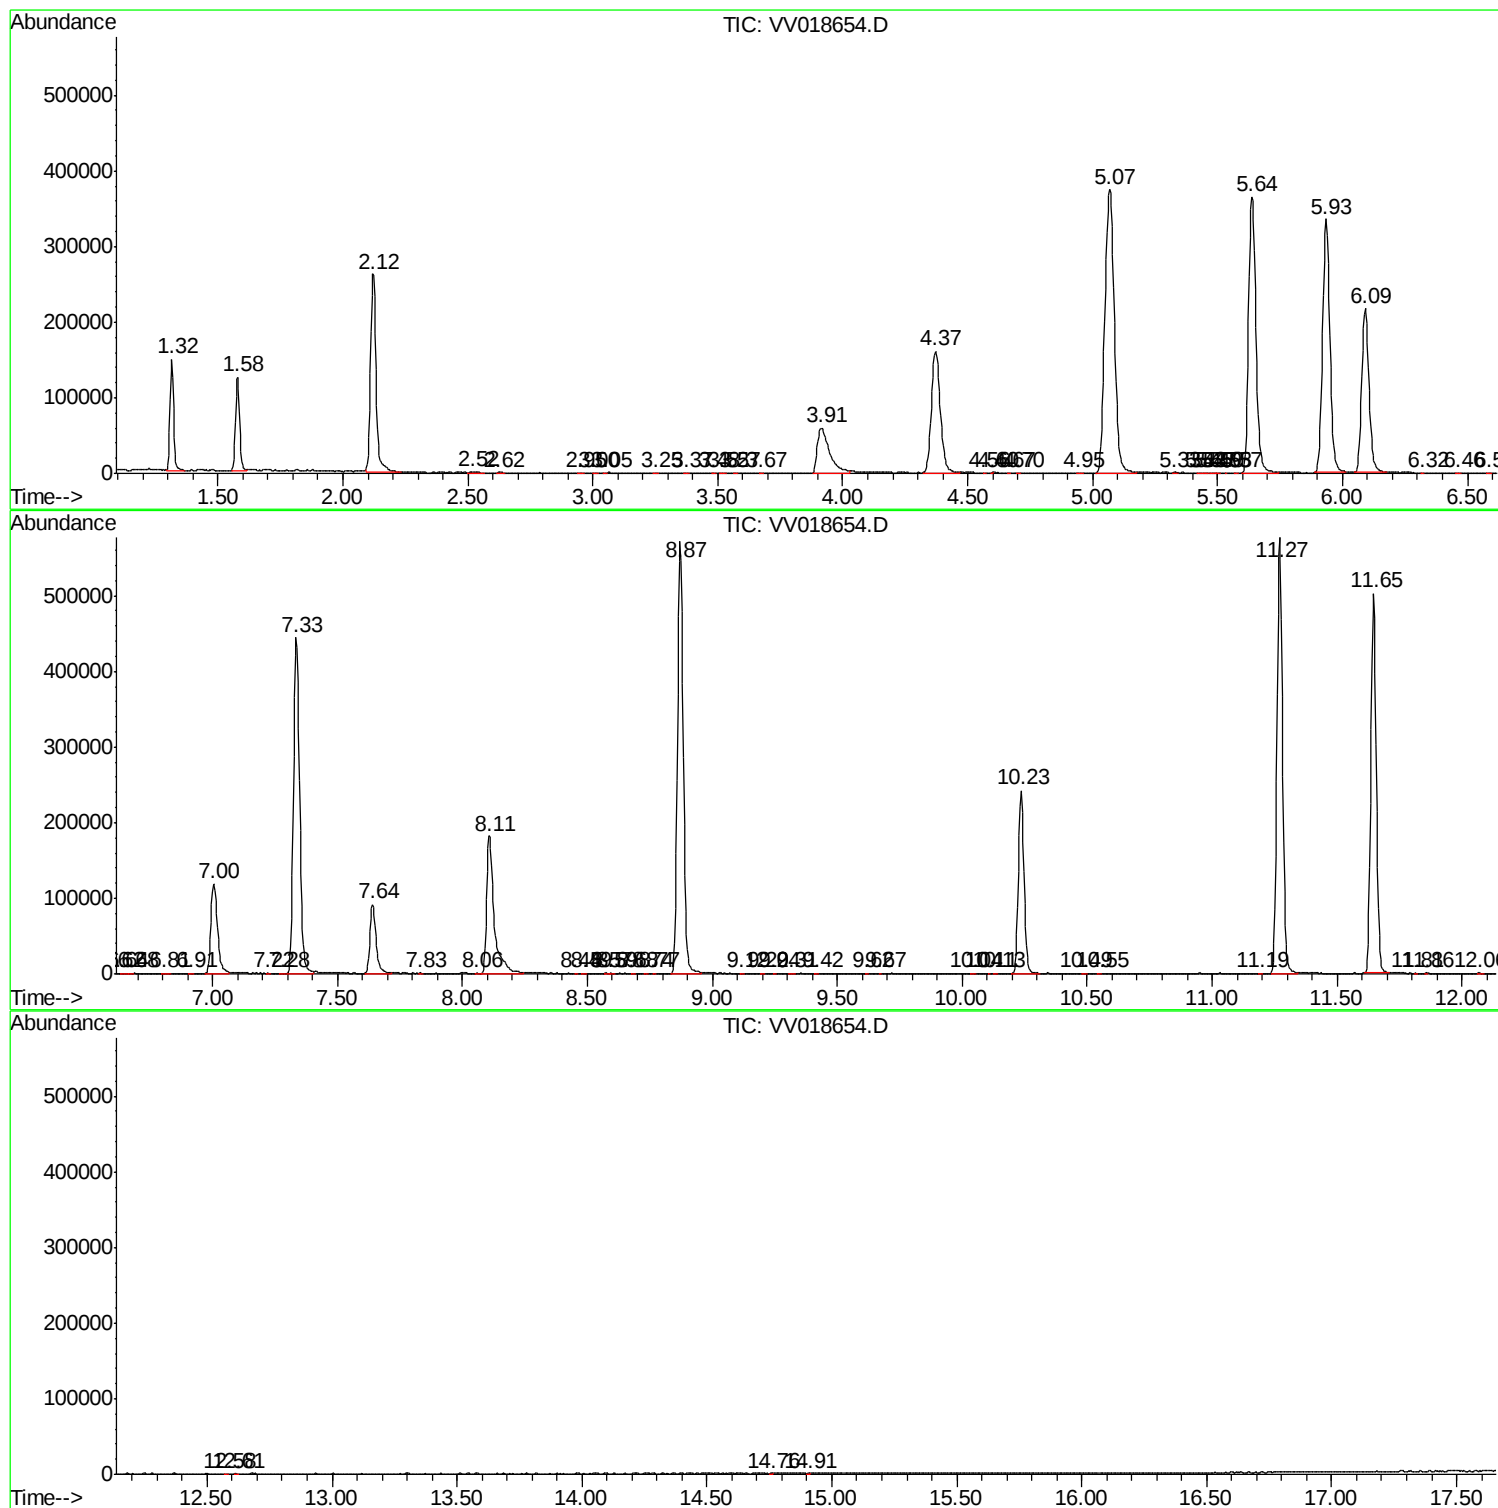

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100320\
Data File : VV018654.D
Acq On : 03 Oct 2020 14:59
Operator : SY/MD
Sample : L4237-12DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV100320\
Data File : VV018654.D
Acq On : 03 Oct 2020 14:59
Operator : SY/MD
Sample : L4237-12DL 5X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
E0AC7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc