

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100320\
 Data File : VV018656.D
 Acq On : 03 Oct 2020 15:46
 Operator : SY/MD
 Sample : L4237-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	157121	152876	12.89%	1.659%
2	1.579	144	152	167	rBV	129983	149044	12.57%	1.617%
3	2.122	312	321	351	rVB	275913	425935	35.92%	4.622%
4	2.621	473	476	479	rBV3	345	168	0.01%	0.002%
5	2.679	491	494	497	rBV2	217	149	0.01%	0.002%
6	2.717	504	506	510	rBV	285	171	0.01%	0.002%
7	2.772	520	523	525	rBV	559	355	0.03%	0.004%
8	2.878	548	556	557	rBV2	319	436	0.04%	0.005%
9	2.913	564	567	572	rVB	282	215	0.02%	0.002%
10	2.936	572	574	575	rBV	153	57	0.00%	0.001%
11	2.994	587	592	593	rBV2	279	209	0.02%	0.002%
12	3.065	608	614	620	rBV5	926	1414	0.12%	0.015%
13	3.090	620	622	628	rVB	304	179	0.02%	0.002%
14	3.119	629	631	632	rVB	139	35	0.00%	0.000%
15	3.138	635	637	641	rBV	172	86	0.01%	0.001%
16	3.235	665	667	669	rBV	284	109	0.01%	0.001%
17	3.409	718	721	726	rBV2	249	244	0.02%	0.003%
18	3.470	738	740	745	rBV	196	156	0.01%	0.002%
19	3.495	745	748	750	rBV	155	93	0.01%	0.001%
20	3.518	750	755	758	rBV2	195	203	0.02%	0.002%
21	3.672	800	803	807	rBV2	177	160	0.01%	0.002%
22	3.695	807	810	812	rBV	151	88	0.01%	0.001%
23	3.843	854	856	859	rBV	236	95	0.01%	0.001%
24	3.859	859	861	865	rVB2	283	151	0.01%	0.002%
25	3.913	867	878	916	rBV	62240	198290	16.72%	2.152%
26	4.373	1005	1021	1047	rBV	163911	408898	34.49%	4.437%
27	4.608	1091	1094	1096	rBV	323	208	0.02%	0.002%
28	4.698	1118	1122	1123	rBV	227	156	0.01%	0.002%
29	4.733	1131	1133	1136	rVB2	278	108	0.01%	0.001%
30	4.798	1149	1153	1155	rBV2	414	231	0.02%	0.003%
31	4.881	1176	1179	1181	rBV	143	115	0.01%	0.001%
32	4.945	1192	1199	1201	rBV	372	420	0.04%	0.005%
33	5.007	1216	1218	1220	rBV	200	93	0.01%	0.001%
34	5.071	1220	1238	1264	rBV2	391509	1009986	85.18%	10.959%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100320\
 Data File : VV018656.D
 Acq On : 03 Oct 2020 15:46
 Operator : SY/MD
 Sample : L4237-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	5.454	1354	1357	1359	rVB	382	200	0.02%	0.002%
36	5.489	1365	1368	1370	rBV	236	118	0.01%	0.001%
37	5.508	1371	1374	1375	rBV2	191	91	0.01%	0.001%
38	5.572	1393	1394	1398	rVB2	173	50	0.00%	0.001%
39	5.595	1398	1401	1403	rVB	209	114	0.01%	0.001%
40	5.640	1403	1415	1443	rBV	351420	696017	58.70%	7.552%
41	5.936	1492	1507	1533	rBV	601379	1185697	100.00%	12.865%
42	6.093	1543	1556	1577	rBV	227476	457106	38.55%	4.960%
43	6.270	1610	1611	1616	rVB3	428	242	0.02%	0.003%
44	6.312	1622	1624	1625	rBV	313	106	0.01%	0.001%
45	6.351	1634	1636	1638	rVB	411	162	0.01%	0.002%
46	6.376	1638	1644	1648	rBV2	358	384	0.03%	0.004%
47	6.396	1648	1650	1652	rBV2	195	97	0.01%	0.001%
48	6.428	1658	1660	1661	rBV2	254	117	0.01%	0.001%
49	6.482	1673	1677	1682	rVB2	393	287	0.02%	0.003%
50	6.511	1683	1686	1687	rBV	208	123	0.01%	0.001%
51	6.560	1699	1701	1703	rVB	286	100	0.01%	0.001%
52	6.572	1703	1705	1706	rBV	148	69	0.01%	0.001%
53	6.624	1718	1721	1722	rBV	193	93	0.01%	0.001%
54	6.711	1744	1748	1753	rVB2	380	290	0.02%	0.003%
55	6.833	1784	1786	1787	rBV2	164	58	0.00%	0.001%
56	7.007	1829	1840	1859	rBV	126169	225147	18.99%	2.443%
57	7.203	1899	1901	1902	rBV	336	189	0.02%	0.002%
58	7.244	1911	1914	1916	rVB3	515	314	0.03%	0.003%
59	7.277	1920	1924	1931	rVB3	450	454	0.04%	0.005%
60	7.338	1931	1943	1968	rBV	468846	808436	68.18%	8.772%
61	7.640	2027	2037	2057	rBV2	90152	158528	13.37%	1.720%
62	7.839	2096	2099	2102	rVB3	578	374	0.03%	0.004%
63	7.900	2117	2118	2120	rBV	151	45	0.00%	0.000%
64	7.958	2127	2136	2143	rBV2	845	1338	0.11%	0.015%
65	7.997	2145	2148	2153	rVB4	742	605	0.05%	0.007%
66	8.074	2170	2172	2173	rBV	128	57	0.00%	0.001%
67	8.109	2173	2183	2214	rBV2	188022	381852	32.20%	4.143%
68	8.479	2296	2298	2299	rBV	156	39	0.00%	0.000%
69	8.508	2305	2307	2311	rVB	304	166	0.01%	0.002%
70	8.531	2311	2314	2316	rBV	196	140	0.01%	0.002%
71	8.621	2340	2342	2344	rVB	160	46	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100320\
 Data File : VV018656.D
 Acq On : 03 Oct 2020 15:46
 Operator : SY/MD
 Sample : L4237-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	8.643	2344	2349	2353	rBV2	438	375	0.03%	0.004%
73	8.791	2392	2395	2396	rBV	224	128	0.01%	0.001%
74	8.871	2409	2420	2438	rBV	548431	879770	74.20%	9.546%
75	9.087	2485	2487	2488	rBV	231	72	0.01%	0.001%
76	9.167	2510	2512	2513	rBV	242	112	0.01%	0.001%
77	9.203	2521	2523	2526	rVB	183	68	0.01%	0.001%
78	9.444	2596	2598	2601	rBV	202	99	0.01%	0.001%
79	9.550	2629	2631	2633	rBV	190	80	0.01%	0.001%
80	9.566	2633	2636	2637	rBV	201	92	0.01%	0.001%
81	9.939	2749	2752	2753	rBV	158	94	0.01%	0.001%
82	10.235	2833	2844	2865	rBV	262090	412212	34.77%	4.473%
83	10.495	2923	2925	2930	rVB2	414	256	0.02%	0.003%
84	10.527	2930	2935	2937	rBV	266	249	0.02%	0.003%
85	10.566	2944	2947	2950	rBV2	263	175	0.01%	0.002%
86	10.720	2990	2995	2997	rBV	222	226	0.02%	0.002%
87	10.874	3041	3043	3047	rVB	361	170	0.01%	0.002%
88	10.939	3060	3063	3068	rBV3	393	350	0.03%	0.004%
89	11.026	3088	3090	3093	rBV	232	188	0.02%	0.002%
90	11.064	3099	3102	3108	rBV2	358	444	0.04%	0.005%
91	11.170	3129	3135	3138	rBV2	309	295	0.02%	0.003%
92	11.206	3143	3146	3150	rVB2	237	174	0.01%	0.002%
93	11.270	3154	3166	3190	rBV	550203	848500	71.56%	9.207%
94	11.566	3251	3258	3266	rBV5	1335	1891	0.16%	0.021%
95	11.646	3271	3283	3298	rBV	516181	798671	67.36%	8.666%
96	11.862	3347	3350	3353	rBV	364	207	0.02%	0.002%
97	11.881	3353	3356	3360	rBV	339	253	0.02%	0.003%
98	11.900	3360	3362	3363	rBV	247	81	0.01%	0.001%
99	12.961	3689	3692	3695	rBV2	224	179	0.02%	0.002%
100	13.283	3788	3792	3796	rBV3	395	307	0.03%	0.003%


Sum of corrected areas: 9216102

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100320\
Data File : VV018656.D
Acq On : 03 Oct 2020 15:46
Operator : SY/MD
Sample : L4237-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

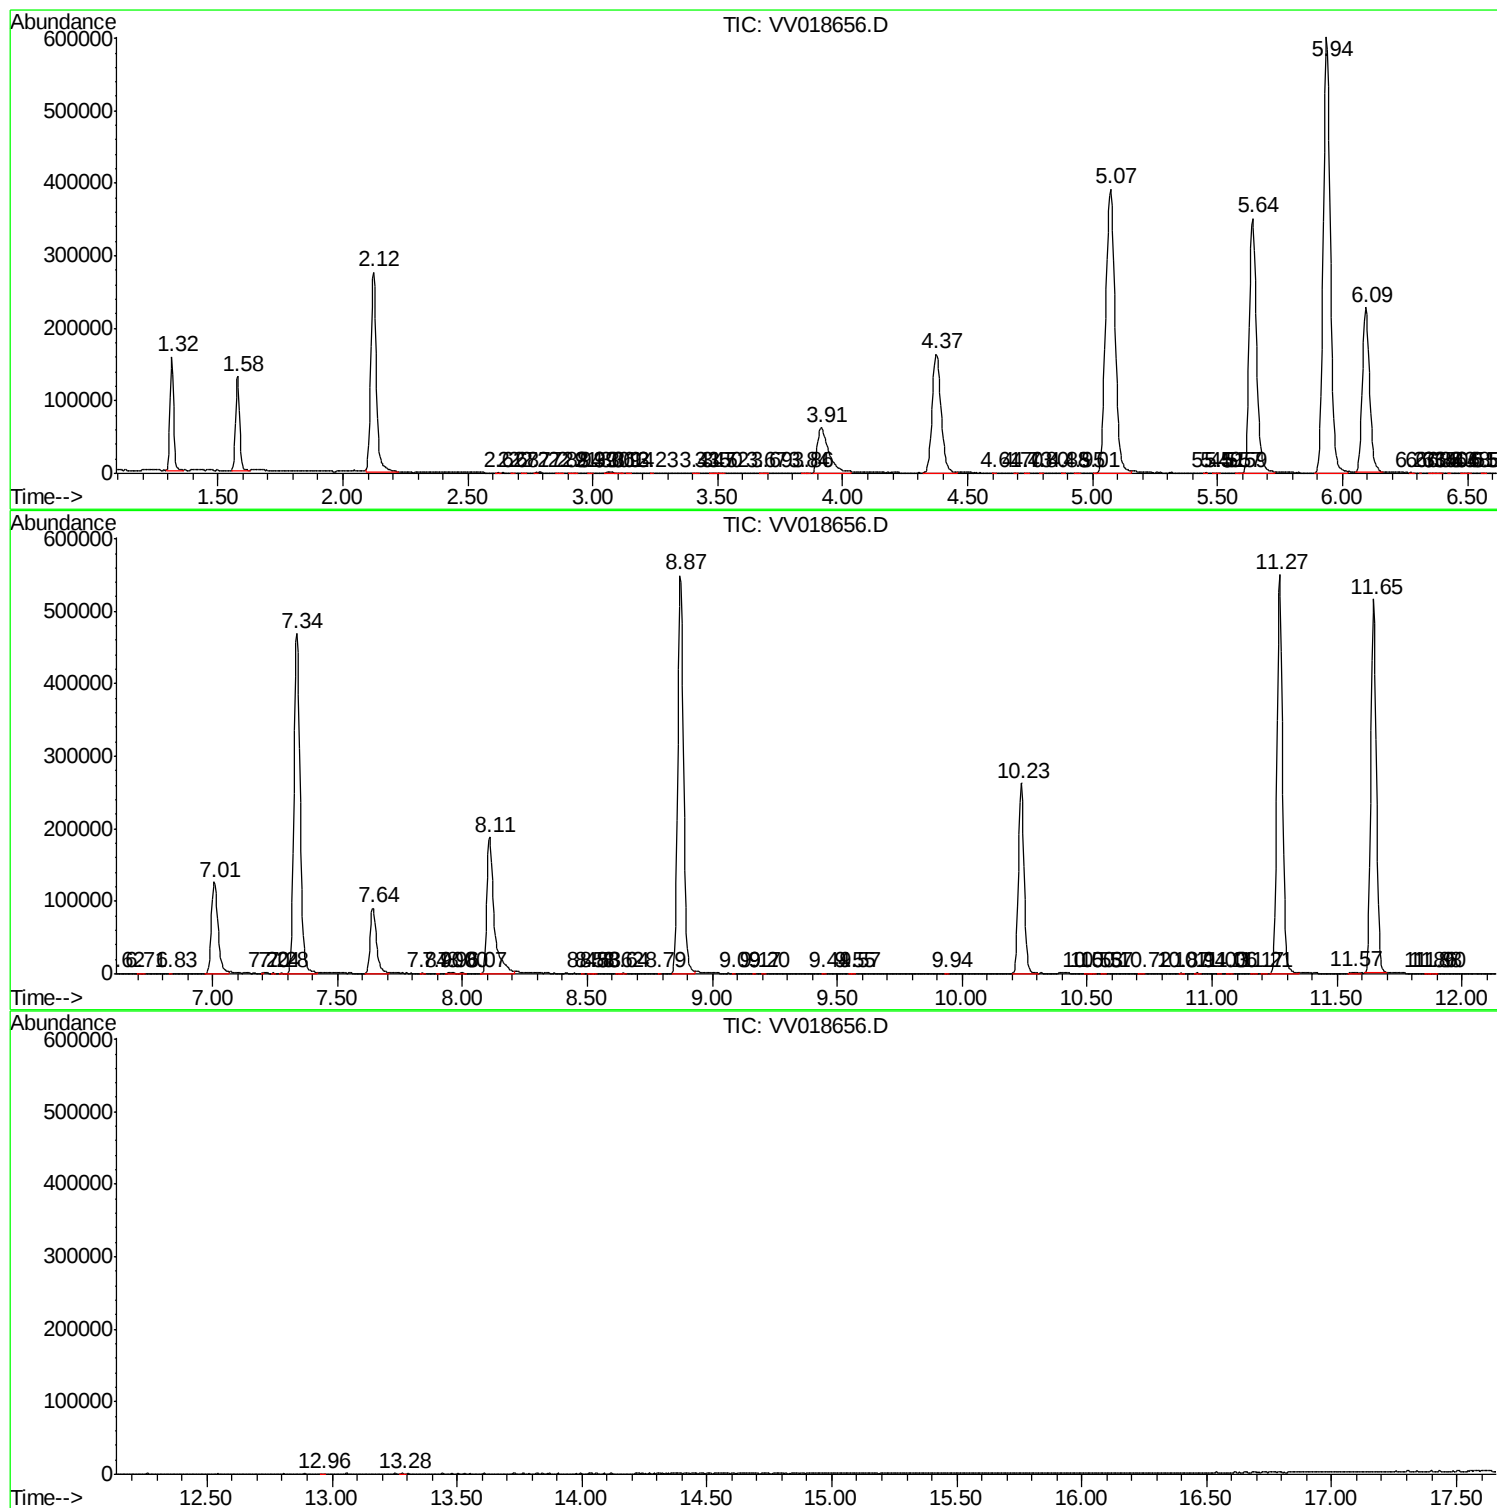

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100320\
Data File : VV018656.D
Acq On : 03 Oct 2020 15:46
Operator : SY/MD
Sample : L4237-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV100320\
Data File : VV018656.D
Acq On : 03 Oct 2020 15:46
Operator : SY/MD
Sample : L4237-11
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
E0AC6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc