

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100320\
 Data File : VV018657.D
 Acq On : 03 Oct 2020 16:09
 Operator : SY/MD
 Sample : L4237-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	80	rBV	123250	123778	2.47%	0.982%
2	1.576	144	151	165	rVB	122921	136204	2.72%	1.080%
3	2.119	311	320	351	rVB	240420	376381	7.52%	2.986%
4	2.515	439	443	448	rBV4	733	776	0.02%	0.006%
5	2.602	467	470	474	rBV3	452	303	0.01%	0.002%
6	2.720	505	507	509	rBV	286	157	0.00%	0.001%
7	2.778	519	525	533	rVB5	1002	1780	0.04%	0.014%
8	2.888	556	559	560	rVB	258	103	0.00%	0.001%
9	2.955	577	580	585	rBV2	359	297	0.01%	0.002%
10	3.032	602	604	606	rBV2	147	73	0.00%	0.001%
11	3.058	607	612	622	rVB5	978	1608	0.03%	0.013%
12	3.126	632	633	635	rVB	183	70	0.00%	0.001%
13	3.161	640	644	646	rBV	237	196	0.00%	0.002%
14	3.196	652	655	660	rBV	274	235	0.00%	0.002%
15	3.235	665	667	670	rVB	144	40	0.00%	0.000%
16	3.319	690	693	696	rBV	183	158	0.00%	0.001%
17	3.364	700	707	709	rBV2	323	328	0.01%	0.003%
18	3.431	724	728	731	rBV	137	101	0.00%	0.001%
19	3.605	780	782	786	rBV	141	70	0.00%	0.001%
20	3.630	786	790	791	rBV2	209	156	0.00%	0.001%
21	3.656	796	798	800	rBV	250	120	0.00%	0.001%
22	3.913	866	878	910	rBV	60551	205275	4.10%	1.628%
23	4.373	1006	1021	1053	rVB	154996	384422	7.68%	3.049%
24	4.582	1079	1086	1089	rBV3	348	511	0.01%	0.004%
25	4.640	1102	1104	1105	rBV3	203	91	0.00%	0.001%
26	4.759	1140	1141	1144	rVB	149	34	0.00%	0.000%
27	4.907	1185	1187	1189	rBV2	128	83	0.00%	0.001%
28	5.071	1221	1238	1261	rBV3	360909	929038	18.55%	7.370%
29	5.389	1334	1337	1338	rBV	182	79	0.00%	0.001%
30	5.486	1365	1367	1369	rBV	193	92	0.00%	0.001%
31	5.508	1373	1374	1377	rVB	269	123	0.00%	0.001%
32	5.556	1388	1389	1390	rBV	286	89	0.00%	0.001%
33	5.640	1402	1415	1441	rBV	330819	657477	13.13%	5.216%
34	5.868	1482	1486	1489	rBV2	303	225	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100320\
 Data File : VV018657.D
 Acq On : 03 Oct 2020 16:09
 Operator : SY/MD
 Sample : L4237-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	5.936	1492	1507	1540	rBV	2613963	5008020	100.00%	39.727%
36	6.093	1545	1556	1585	rVB	214841	437961	8.75%	3.474%
37	6.318	1623	1626	1629	rBV3	386	253	0.01%	0.002%
38	6.363	1639	1640	1642	rBV	206	105	0.00%	0.001%
39	6.431	1659	1661	1663	rBV	207	108	0.00%	0.001%
40	6.505	1682	1684	1689	rVB2	416	224	0.00%	0.002%
41	6.534	1689	1693	1696	rVB2	356	249	0.00%	0.002%
42	6.556	1698	1700	1704	rVV	273	139	0.00%	0.001%
43	6.576	1704	1706	1708	rVB	147	57	0.00%	0.000%
44	6.611	1715	1717	1720	rBV	196	130	0.00%	0.001%
45	6.627	1720	1722	1724	rBV	185	91	0.00%	0.001%
46	6.653	1728	1730	1731	rBV	237	92	0.00%	0.001%
47	6.714	1746	1749	1752	rBV	222	179	0.00%	0.001%
48	6.775	1765	1768	1772	rVB2	307	220	0.00%	0.002%
49	6.797	1772	1775	1776	rBV	216	104	0.00%	0.001%
50	6.907	1808	1809	1811	rVB	259	96	0.00%	0.001%
51	6.929	1813	1816	1822	rBV3	355	292	0.01%	0.002%
52	6.961	1823	1826	1829	rBV	260	219	0.00%	0.002%
53	7.006	1829	1840	1863	rBV	118556	215060	4.29%	1.706%
54	7.193	1896	1898	1899	rBV	290	94	0.00%	0.001%
55	7.225	1906	1908	1910	rBV	264	108	0.00%	0.001%
56	7.264	1917	1920	1921	rBV	247	126	0.00%	0.001%
57	7.338	1930	1943	1971	rBV	432349	750960	15.00%	5.957%
58	7.585	2017	2020	2022	rBV	222	108	0.00%	0.001%
59	7.640	2025	2037	2056	rBV	83315	147407	2.94%	1.169%
60	7.814	2088	2091	2092	rBV2	340	163	0.00%	0.001%
61	7.897	2116	2117	2118	rBV	142	45	0.00%	0.000%
62	7.907	2118	2120	2124	rVB	293	145	0.00%	0.001%
63	7.958	2129	2136	2139	rBV2	764	954	0.02%	0.008%
64	8.003	2146	2150	2155	rVB4	881	830	0.02%	0.007%
65	8.029	2155	2158	2160	rBV	265	143	0.00%	0.001%
66	8.109	2169	2183	2226	rBV2	172669	360696	7.20%	2.861%
67	8.399	2272	2273	2275	rBV	311	133	0.00%	0.001%
68	8.428	2279	2282	2284	rBV	473	235	0.00%	0.002%
69	8.450	2287	2289	2296	rVB3	392	295	0.01%	0.002%
70	8.518	2307	2310	2312	rBV	482	376	0.01%	0.003%
71	8.633	2342	2346	2350	rBV2	364	363	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100320\
 Data File : VV018657.D
 Acq On : 03 Oct 2020 16:09
 Operator : SY/MD
 Sample : L4237-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	8.740	2377	2379	2382	rVB2	270	162	0.00%	0.001%
73	8.810	2399	2401	2406	rVB	430	313	0.01%	0.002%
74	8.871	2409	2420	2446	rBV	565629	920359	18.38%	7.301%
75	9.135	2500	2502	2503	rBV	242	124	0.00%	0.001%
76	9.203	2521	2523	2529	rBV2	319	241	0.00%	0.002%
77	9.592	2641	2644	2645	rBV	355	204	0.00%	0.002%
78	10.010	2772	2774	2778	rVB2	268	148	0.00%	0.001%
79	10.186	2825	2829	2833	rBV2	253	214	0.00%	0.002%
80	10.238	2833	2845	2866	rVV	245711	388291	7.75%	3.080%
81	10.373	2884	2887	2890	rBV2	281	150	0.00%	0.001%
82	10.395	2890	2894	2895	rBV2	876	579	0.01%	0.005%
83	10.440	2905	2908	2910	rBV2	218	125	0.00%	0.001%
84	10.456	2910	2913	2917	rVV	340	256	0.01%	0.002%
85	10.495	2922	2925	2931	rBV2	262	272	0.01%	0.002%
86	10.643	2968	2971	2977	rVB2	343	231	0.00%	0.002%
87	10.717	2990	2994	2996	rBV	289	238	0.00%	0.002%
88	10.823	3024	3027	3030	rVB	324	188	0.00%	0.001%
89	11.270	3154	3166	3194	rBV	530214	802864	16.03%	6.369%
90	11.505	3236	3239	3244	rBV3	235	217	0.00%	0.002%
91	11.569	3255	3259	3263	rBV3	743	676	0.01%	0.005%
92	11.646	3270	3283	3301	rBV	478932	742011	14.82%	5.886%
93	12.427	3524	3526	3528	rBV	311	147	0.00%	0.001%
94	12.572	3568	3571	3575	rVB	361	216	0.00%	0.002%
95	12.714	3611	3615	3619	rBV2	300	311	0.01%	0.002%
96	13.186	3760	3762	3765	rBV	319	186	0.00%	0.001%
97	13.768	3941	3943	3945	rBV2	326	175	0.00%	0.001%


Sum of corrected areas: 12606151

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100320\
Data File : VV018657.D
Acq On : 03 Oct 2020 16:09
Operator : SY/MD
Sample : L4237-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

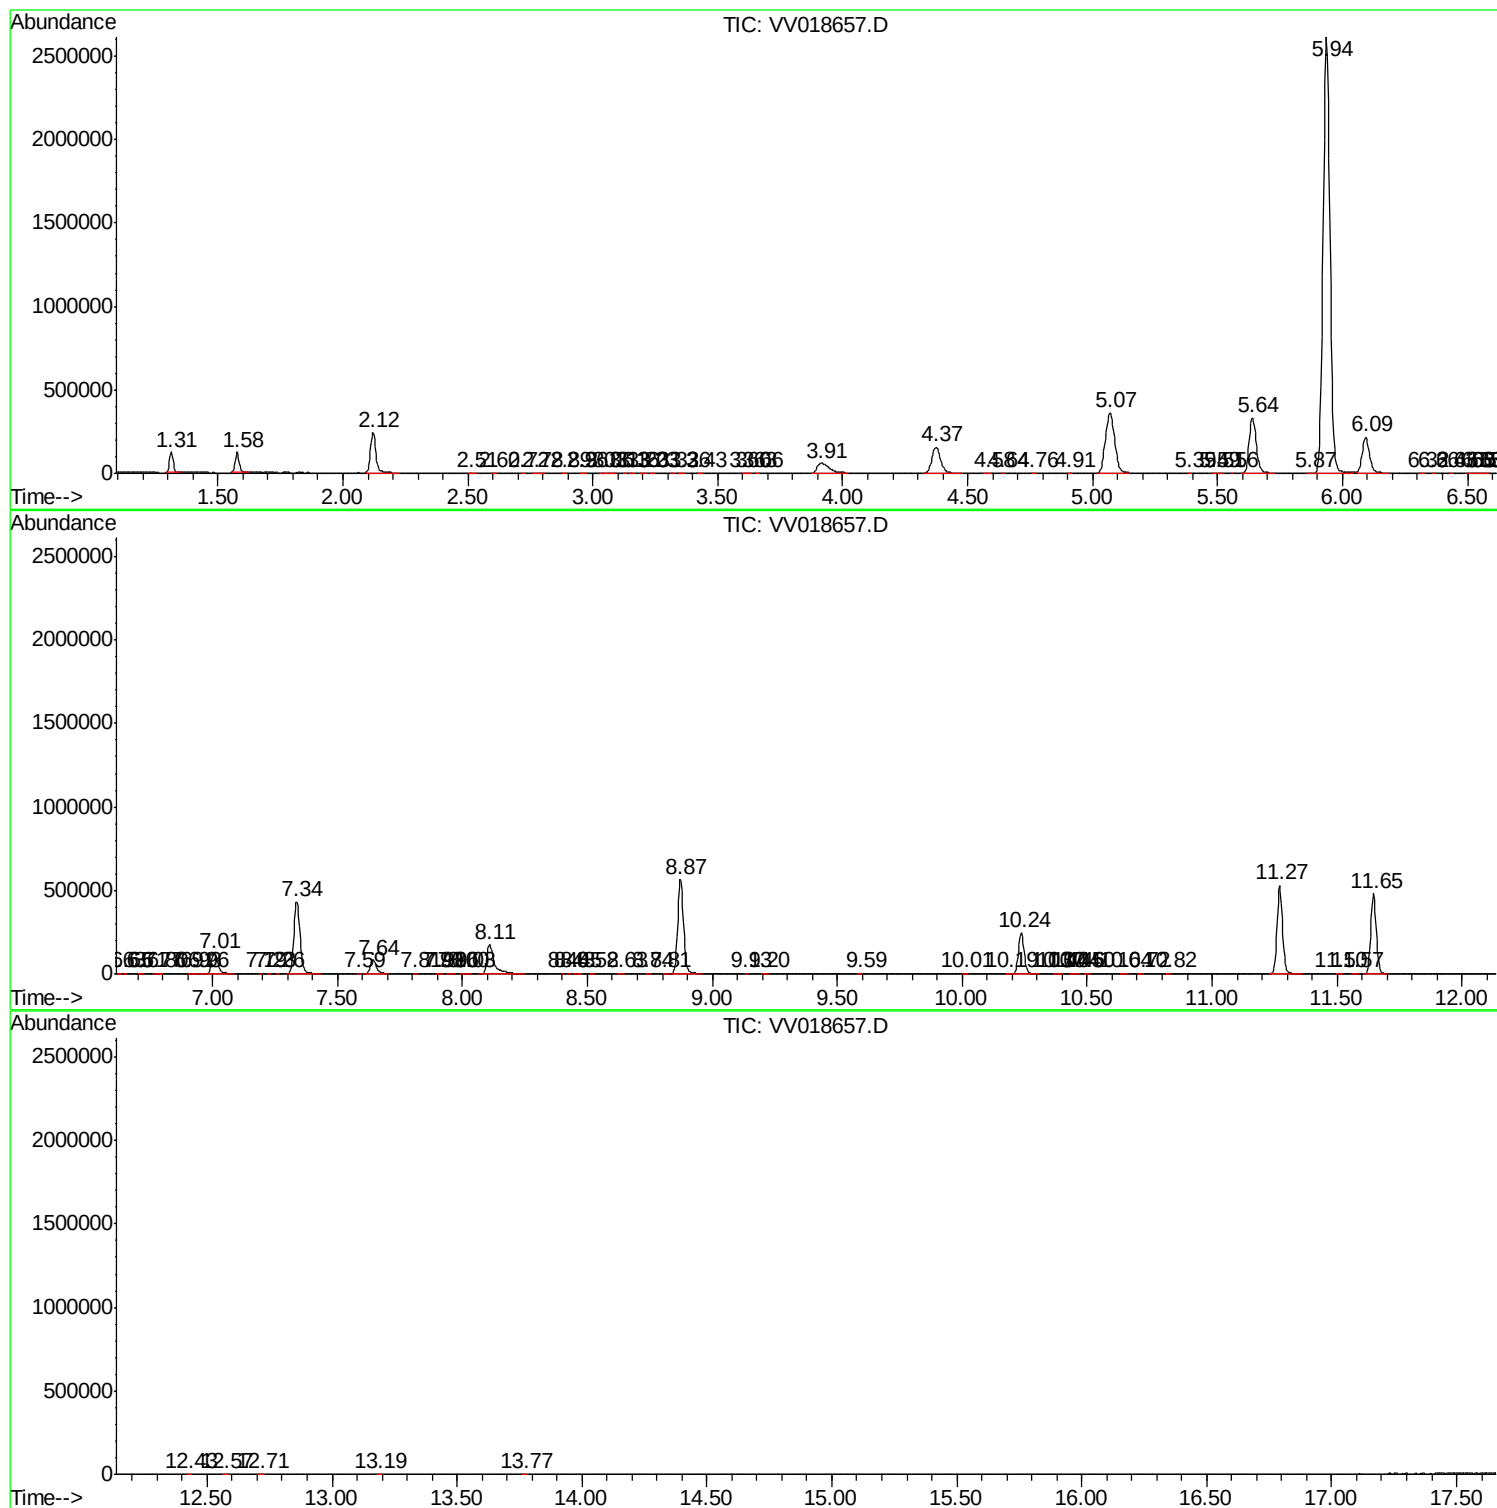

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100320\
Data File : VV018657.D
Acq On : 03 Oct 2020 16:09
Operator : SY/MD
Sample : L4237-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV100320\
Data File : VV018657.D
Acq On : 03 Oct 2020 16:09
Operator : SY/MD
Sample : L4237-01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
E0AB6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc