


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100320\
 Data File : VV018651.D
 Acq On : 03 Oct 2020 13:18
 Operator : SY/MD
 Sample : BFB66
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB66

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis
 Last Update : Mon Oct 05 04:50:26 2020

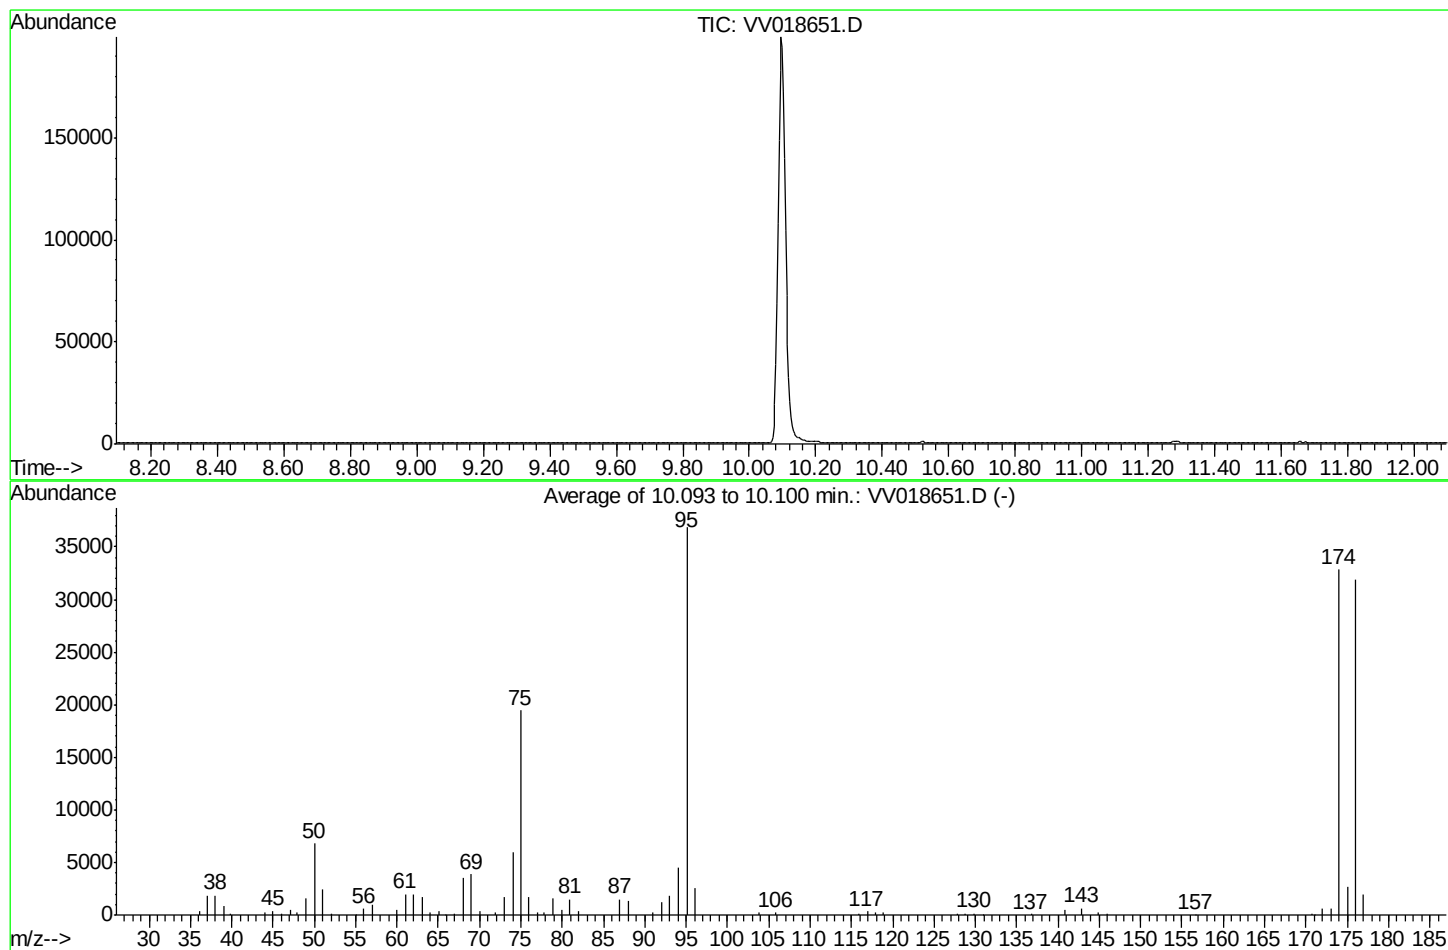

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	6804	PASS
75	95	30	80	52.8	19456	PASS
95	95	100	100	100.0	36866	PASS
96	95	5	9	7.0	2577	PASS
173	174	0.00	2	1.8	604	PASS
174	95	50	120	89.1	32853	PASS
175	174	5	9	8.3	2720	PASS
176	174	95	101	97.0	31866	PASS
177	176	5	9	6.2	1987	PASS

m/z	Abundance
36.00	403.0
37.00	1778.0
38.00	1833.0
39.00	793.0
39.90	153.0
44.00	768.0
45.00	378.0
46.00	141.0
47.10	442.0
47.90	249.0
49.00	1493.0
50.10	6779.0
51.10	2375.0
55.00	112.0
55.90	573.0
57.00	864.0
60.00	424.0
61.00	1737.0
62.00	1802.0
63.00	1653.0
64.00	256.0
65.10	377.0
67.00	150.0
68.00	3525.0
69.00	3913.0
70.00	355.0
72.00	272.0
73.00	1624.0
74.00	5934.0
75.00	18936.0
76.00	1666.0
77.00	165.0
77.90	270.0
78.90	1486.0
80.00	508.0
80.90	1398.0
81.90	331.0
87.00	1532.0
88.00	1267.0
90.90	196.0
92.00	1207.0
93.00	1701.0
94.00	4227.0
95.10	35008.0
96.00	2478.0
103.90	201.0
105.90	237.0
115.90	163.0
116.90	318.0
118.00	198.0
118.80	276.0
127.70	170.0
129.80	172.0
136.80	124.0
140.90	520.0
142.90	611.0
144.90	194.0
146.00	138.0
156.70	129.0
170.80	162.0
171.90	661.0
173.10	588.0
174.00	30184.0
175.00	2616.0
176.00	29696.0
177.00	1898.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
36.10	396.0
37.00	1895.0
38.00	1925.0
39.00	844.0
39.90	184.0
44.00	741.0
45.00	405.0
46.00	105.0
47.00	515.0
47.90	249.0
49.00	1718.0
50.10	7060.0
51.10	2585.0
52.00	114.0
56.00	598.0
57.00	1003.0
60.00	461.0
61.00	2104.0
62.00	2041.0
63.10	1819.0
64.00	271.0
65.10	379.0
67.00	151.0
68.00	3634.0
69.00	4018.0
70.00	372.0
72.00	256.0
73.00	1830.0
74.00	6101.0
75.00	20192.0
76.00	1783.0
77.00	198.0
77.80	261.0
78.90	1666.0
80.00	523.0
80.90	1532.0
81.90	351.0
87.00	1500.0
88.00	1417.0
91.00	225.0
92.00	1353.0
93.00	1883.0
94.00	4644.0
95.10	38208.0
96.00	2662.0
103.80	213.0
105.90	251.0
116.00	173.0
116.90	363.0
118.00	256.0
118.80	331.0
127.80	134.0
128.80	116.0
129.80	156.0
136.70	126.0
140.90	505.0
142.90	692.0
144.90	216.0
146.00	107.0
170.80	158.0
171.90	684.0
173.00	635.0
174.00	34024.0
175.00	2838.0
176.00	33200.0
177.00	2024.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
36.00	398.0
37.00	1852.0
38.00	1767.0
39.00	862.0
39.90	181.0
44.00	660.0
44.90	387.0
47.00	525.0
48.00	225.0
49.00	1671.0
50.00	6575.0
51.00	2424.0
52.10	161.0
56.00	539.0
57.00	1043.0
60.00	439.0
61.00	2131.0
62.00	1925.0
63.10	1760.0
64.00	257.0
65.10	408.0
65.80	112.0
66.90	130.0
68.00	3487.0
69.00	3744.0
70.00	345.0
71.90	214.0
73.00	1778.0
74.00	5718.0
75.00	19240.0
76.00	1763.0
77.10	221.0
77.80	197.0
78.90	1581.0
79.90	518.0
80.90	1557.0
81.90	380.0
87.00	1413.0
88.00	1396.0
91.00	207.0
92.00	1218.0
93.00	1808.0
94.00	4545.0
95.10	37384.0
96.00	2593.0
103.80	200.0
105.90	236.0
115.90	142.0
116.90	376.0
117.90	262.0
118.80	319.0
127.80	122.0
128.80	104.0
129.90	118.0
130.90	126.0
136.70	110.0
140.80	480.0
142.90	682.0
144.90	195.0
171.00	141.0
172.00	644.0
173.00	589.0
174.00	34352.0
175.00	2706.0
176.00	32704.0
177.00	2041.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
44.00	444.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66