

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
 Data File : VV032210.D
 Acq On : 03 Oct 2023 11:09
 Operator : SY/MD
 Sample : VV1003WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 04 04:05:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 04 04:04:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	203675	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	197325	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	97563	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	75109	59.589	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 119.180%			
7) Chloroethane-d5	1.532	69	61651	56.708	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 113.420%			
11) 1,1-Dichloroethene-d2	2.060	65	31109	56.522	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 113.040%			
21) 2-Butanone-d5	3.786	46	94647	83.511	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 83.510%			
24) Chloroform-d	4.253	84	127092	48.184	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 96.360%			
26) 1,2-Dichloroethane-d4	4.944	65	78231	49.295	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 98.580%			
32) Benzene-d6	4.963	84	259858	50.095	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.180%			
36) 1,2-Dichloropropane-d6	5.992	67	86310	49.860	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 99.720%			
41) Toluene-d8	7.246	98	233165	49.271	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 98.540%			
43) trans-1,3-Dichloroprop...	7.558	79	36375	44.172	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 88.340%			
47) 2-Hexanone-d5	8.027	63	57557	76.997	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 77.000%			
56) 1,1,2,2-Tetrachloroeth...	10.156	84	106426	43.227	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 86.460%			
66) 1,2-Dichlorobenzene-d4	11.564	152	88646	50.103	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 100.200%			
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.915	75	2076	0.758	ug/L #	57
61) 1,2,3-Trichloropropane	11.188	75	12536	6.610	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
Data File : VV032210.D
Acq On : 03 Oct 2023 11:09
Operator : SY/MD
Sample : VV1003WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 04 04:05:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 04 04:04:33 2023
Response via : Initial Calibration

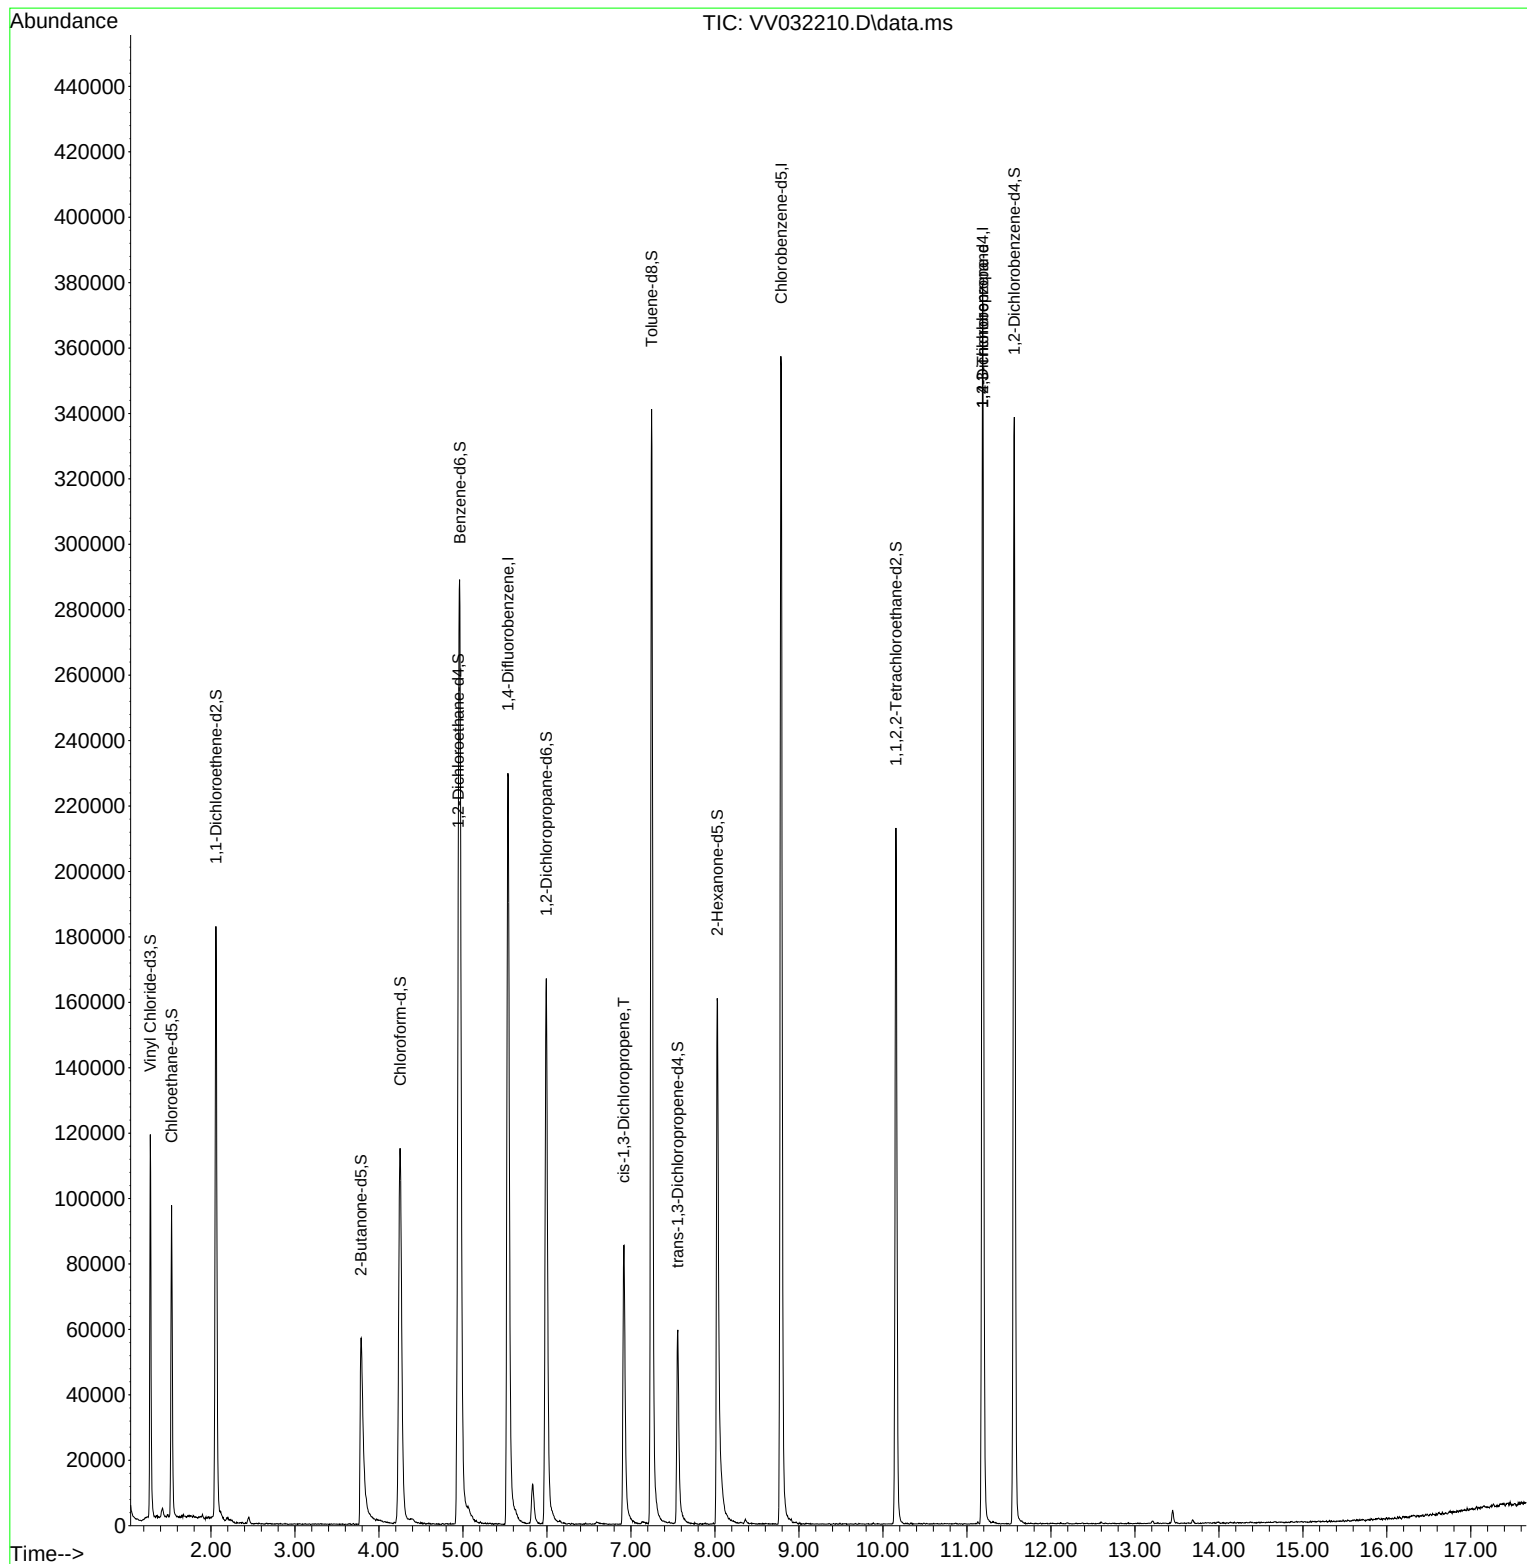

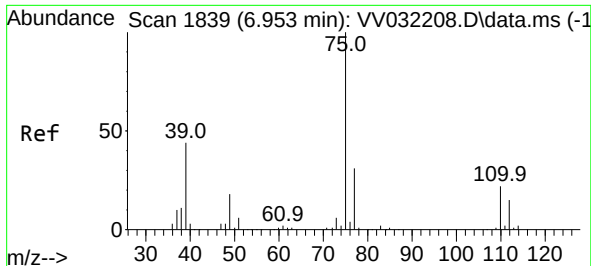

#39

cis-1,3-Dichloropropene

Concen: 0.758 ug/L

RT: 6.915 min Scan# 11

Delta R.T. -0.039 min

Lab File: VV032210.D

Acq: 03 Oct 2023 11:09

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 75 Resp: 2076

Ion Ratio Lower Upper

75 100

77 56.0 22.3 41.5#

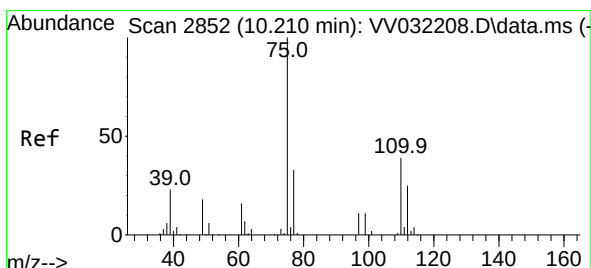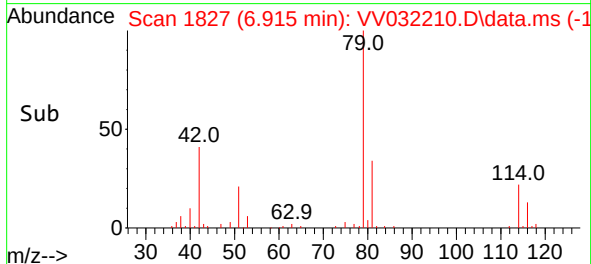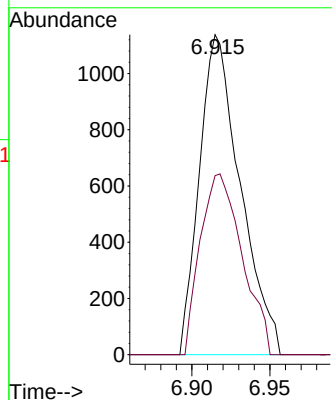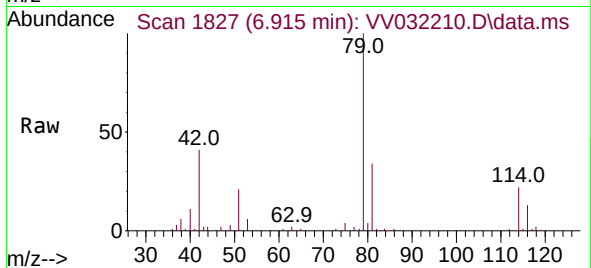

#61

1,2,3-Trichloropropane

Concen: 6.610 ug/L

RT: 11.188 min Scan# 3156

Delta R.T. 0.978 min

Lab File: VV032210.D

Acq: 03 Oct 2023 11:09

Tgt Ion: 75 Resp: 12536

Ion Ratio Lower Upper

75 100

77 33.4 26.1 39.1

110 2.6 30.5 45.7#

