

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
 Data File : VV032209.D
 Acq On : 03 Oct 2023 10:46
 Operator : SY/MD
 Sample : VV1003MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK204

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

Signal : TIC: VV032209.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	124581	130653	15.78%	2.082%
2	1.532	146	153	168	rVB	98609	117090	14.14%	1.866%
3	2.060	308	317	332	rBV	194939	281291	33.98%	4.482%
4	2.445	430	437	447	rBV7	1759	2651	0.32%	0.042%
5	2.629	491	494	497	rBV2	208	182	0.02%	0.003%
6	2.806	547	549	550	rBV	177	78	0.01%	0.001%
7	2.892	575	576	580	rBV2	229	142	0.02%	0.002%
8	2.970	595	600	604	rBV2	278	274	0.03%	0.004%
9	3.047	623	624	625	rBV2	191	44	0.01%	0.001%
10	3.098	637	640	642	rBV	204	174	0.02%	0.003%
11	3.349	716	718	719	rBV	190	53	0.01%	0.001%
12	3.497	760	764	766	rBV2	167	139	0.02%	0.002%
13	3.616	798	801	803	rBV	248	144	0.02%	0.002%
14	3.786	845	854	889	rBV	63507	177078	21.39%	2.821%
15	4.252	982	999	1031	rBV	123912	321716	38.86%	5.126%
16	4.571	1096	1098	1101	rBV2	276	143	0.02%	0.002%
17	4.629	1113	1116	1120	rVB2	189	127	0.02%	0.002%
18	4.648	1120	1122	1125	rBV2	138	86	0.01%	0.001%
19	4.664	1125	1127	1129	rBV2	208	100	0.01%	0.002%
20	4.722	1143	1145	1146	rBV	278	92	0.01%	0.001%
21	4.773	1157	1161	1164	rBV2	182	130	0.02%	0.002%
22	4.793	1164	1167	1171	rVB	226	129	0.02%	0.002%
23	4.815	1171	1174	1177	rBV	201	156	0.02%	0.002%
24	4.902	1199	1201	1202	rBV	165	59	0.01%	0.001%
25	4.960	1202	1219	1249	rBV2	311736	827815	100.00%	13.190%
26	5.317	1328	1330	1331	rBV2	135	42	0.01%	0.001%
27	5.368	1343	1346	1348	rBV2	116	78	0.01%	0.001%
28	5.378	1348	1349	1353	rBV	340	233	0.03%	0.004%
29	5.436	1364	1367	1369	rBV2	94	70	0.01%	0.001%
30	5.449	1369	1371	1375	rVB	259	141	0.02%	0.002%
31	5.494	1382	1385	1387	rBV	111	78	0.01%	0.001%
32	5.535	1387	1398	1451	rBV	237099	504656	60.96%	8.041%
33	5.828	1479	1489	1504	rBV2	12345	26314	3.18%	0.419%
34	5.992	1526	1540	1575	rBV	178259	382305	46.18%	6.091%
35	6.220	1606	1611	1614	rBV4	277	273	0.03%	0.004%
36	6.240	1615	1617	1620	rVV2	287	164	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
 Data File : VV032209.D
 Acq On : 03 Oct 2023 10:46
 Operator : SY/MD
 Sample : VV1003MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK204

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

37	6.278	1627	1629	1632	rBV	229	107	0.01%	0.002%
38	6.326	1641	1644	1647	rBV2	92	64	0.01%	0.001%
39	6.342	1647	1649	1653	rVB2	138	70	0.01%	0.001%
40	6.407	1668	1669	1673	rVB	117	49	0.01%	0.001%
41	6.445	1678	1681	1684	rVB	137	82	0.01%	0.001%
42	6.484	1690	1693	1697	rVB	132	69	0.01%	0.001%
43	6.548	1711	1713	1716	rVB	146	46	0.01%	0.001%
44	6.571	1717	1720	1722	rBV2	402	253	0.03%	0.004%
45	6.712	1762	1764	1767	rBV2	175	121	0.01%	0.002%
46	6.847	1803	1806	1808	rBV2	102	70	0.01%	0.001%
47	6.915	1816	1827	1860	rBV	93251	183952	22.22%	2.931%
48	7.092	1880	1882	1883	rVB	307	81	0.01%	0.001%
49	7.178	1906	1909	1911	rBV2	324	178	0.02%	0.003%
50	7.246	1917	1930	1962	rBV	371157	665544	80.40%	10.604%
51	7.555	2017	2026	2050	rBV	64031	117436	14.19%	1.871%
52	7.876	2124	2126	2129	rBV3	325	190	0.02%	0.003%
53	7.915	2136	2138	2140	rVB	254	82	0.01%	0.001%
54	7.985	2156	2160	2162	rBV2	196	147	0.02%	0.002%
55	8.027	2163	2173	2205	rBV	174663	344703	41.64%	5.492%
56	8.365	2272	2278	2289	rVB5	889	1611	0.19%	0.026%
57	8.452	2303	2305	2310	rBV3	232	142	0.02%	0.002%
58	8.522	2325	2327	2328	rVB2	171	48	0.01%	0.001%
59	8.551	2334	2336	2337	rBV	351	133	0.02%	0.002%
60	8.580	2343	2345	2346	rBV	197	89	0.01%	0.001%
61	8.635	2360	2362	2363	rBV	158	47	0.01%	0.001%
62	8.667	2368	2372	2375	rBV2	298	222	0.03%	0.004%
63	8.686	2375	2378	2380	rBV	141	68	0.01%	0.001%
64	8.728	2390	2391	2392	rBV	143	47	0.01%	0.001%
65	8.786	2398	2409	2435	rBV	359442	605744	73.17%	9.652%
66	9.037	2484	2487	2493	rVB3	347	212	0.03%	0.003%
67	9.085	2499	2502	2504	rBV2	261	187	0.02%	0.003%
68	9.172	2526	2529	2532	rVB	187	119	0.01%	0.002%
69	9.227	2543	2546	2549	rBV	122	77	0.01%	0.001%
70	9.317	2571	2574	2577	rBV	225	121	0.01%	0.002%
71	9.358	2583	2587	2591	rBV2	150	152	0.02%	0.002%
72	9.487	2623	2627	2630	rBV2	292	226	0.03%	0.004%
73	9.513	2633	2635	2636	rBV2	196	83	0.01%	0.001%
74	9.661	2679	2681	2683	rVB	199	65	0.01%	0.001%
75	9.722	2699	2700	2705	rBV	211	150	0.02%	0.002%
76	9.882	2744	2750	2756	rVB3	387	521	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
 Data File : VV032209.D
 Acq On : 03 Oct 2023 10:46
 Operator : SY/MD
 Sample : VV1003MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK204

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

77	9.982	2779	2781	2786	rVB2	242	123	0.01%	0.002%
78	10.156	2822	2835	2859	rBV	229306	365029	44.10%	5.816%
79	10.304	2879	2881	2882	rBV	171	53	0.01%	0.001%
80	10.333	2888	2890	2893	rVB	304	110	0.01%	0.002%
81	10.358	2896	2898	2899	rBV	164	47	0.01%	0.001%
82	10.407	2910	2913	2915	rVB	230	135	0.02%	0.002%
83	10.423	2915	2918	2921	rBV2	188	145	0.02%	0.002%
84	10.526	2948	2950	2953	rBV	286	192	0.02%	0.003%
85	10.853	3048	3052	3055	rBV3	283	284	0.03%	0.005%
86	10.934	3074	3077	3080	rVB	224	100	0.01%	0.002%
87	11.043	3106	3111	3112	rBV2	183	150	0.02%	0.002%
88	11.095	3124	3127	3133	rBV2	212	239	0.03%	0.004%
89	11.127	3134	3137	3138	rBV	453	262	0.03%	0.004%
90	11.188	3145	3156	3183	rBV	392684	604862	73.07%	9.638%
91	11.564	3260	3273	3300	rBV	367200	580442	70.12%	9.248%
92	11.763	3331	3335	3337	rBV2	276	201	0.02%	0.003%
93	11.915	3380	3382	3389	rVB	217	151	0.02%	0.002%
94	12.294	3499	3500	3501	rBV	251	63	0.01%	0.001%
95	12.435	3540	3544	3549	rBV	6173	4151	0.50%	0.066%
96	12.593	3588	3593	3599	rVB3	1148	1320	0.16%	0.021%
97	13.088	3743	3747	3750	rBV2	193	144	0.02%	0.002%
98	13.207	3779	3784	3792	rBV4	1940	2480	0.30%	0.040%
99	13.448	3851	3859	3870	rBV2	9029	13918	1.68%	0.222%
100	13.686	3928	3933	3943	rVB5	2351	3273	0.40%	0.052%




Sum of corrected areas: 6276082

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
Data File : VV032209.D
Acq On : 03 Oct 2023 10:46
Operator : SY/MD
Sample : VV1003MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK204

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

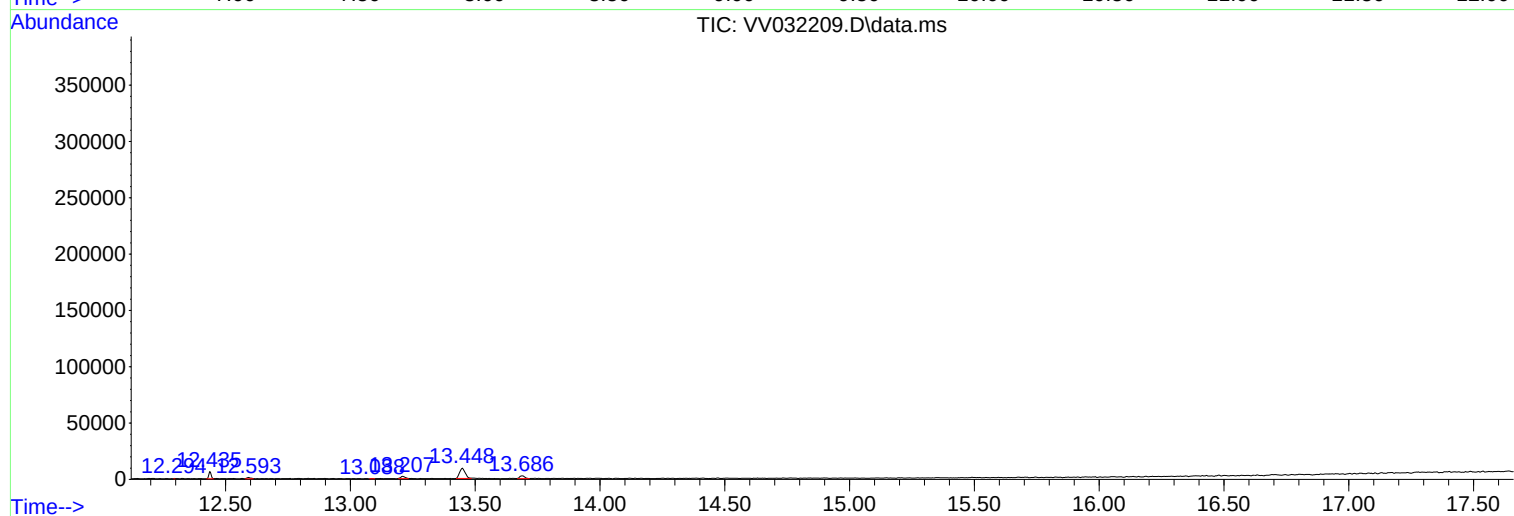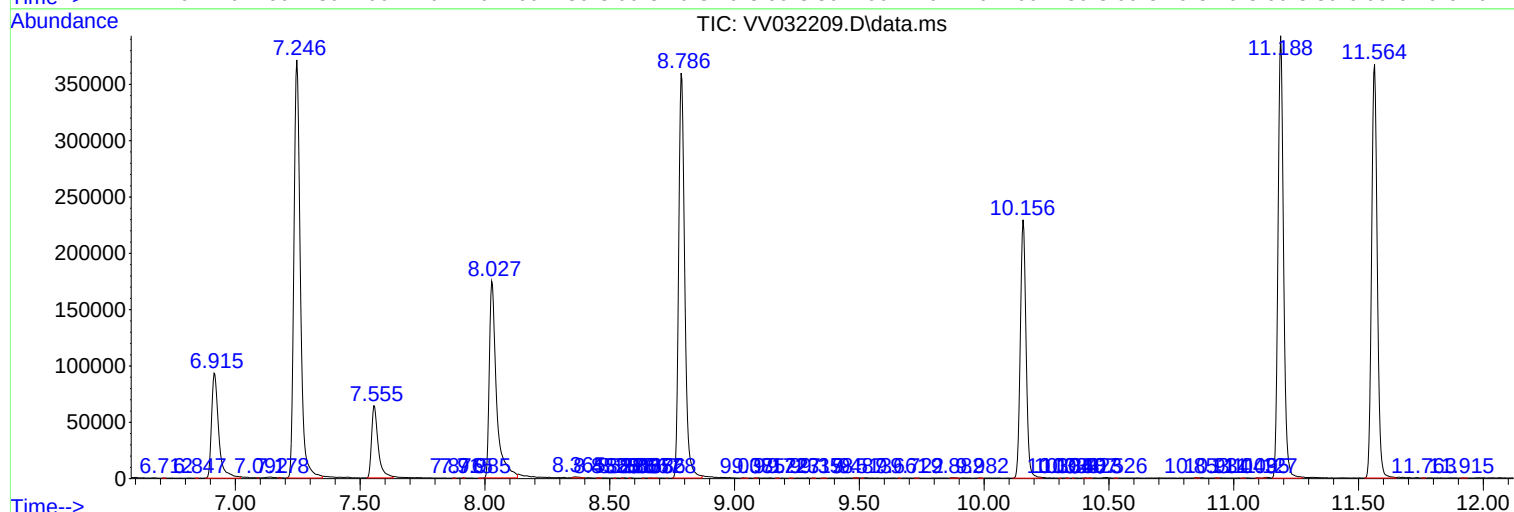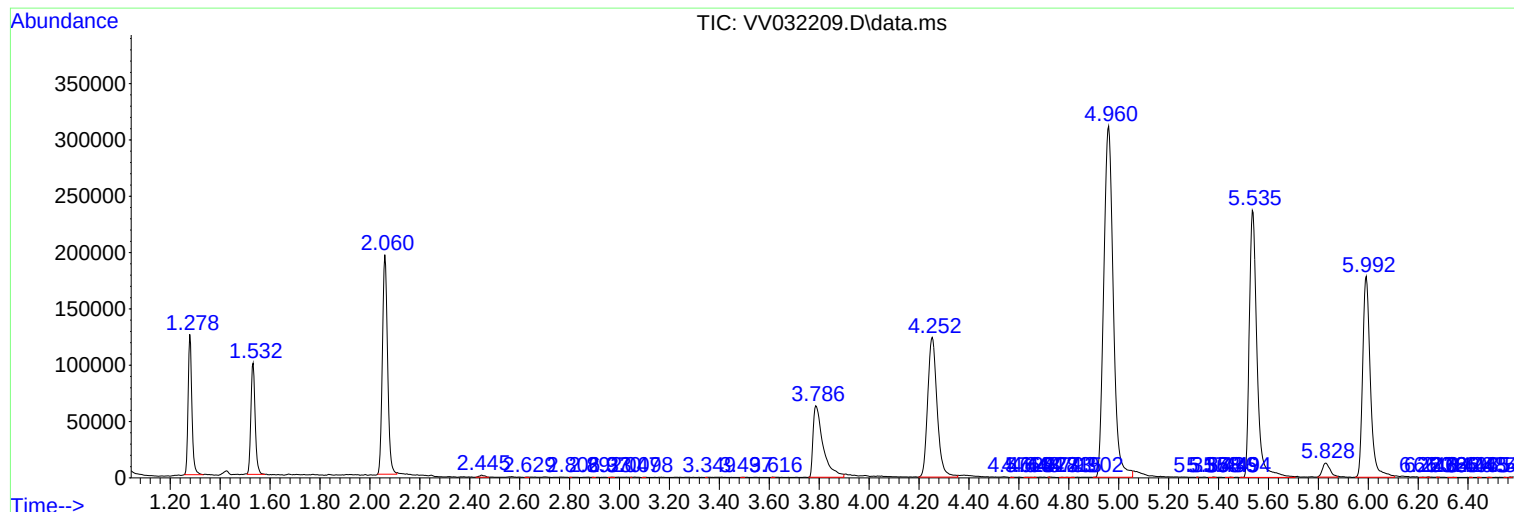

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
Data File : VV032209.D
Acq On : 03 Oct 2023 10:46
Operator : SY/MD
Sample : VV1003MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK204

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
Data File : VV032209.D
Acq On : 03 Oct 2023 10:46
Operator : SY/MD
Sample : VV1003MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK204

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc