

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
 Data File : VV032211.D
 Acq On : 03 Oct 2023 12:43
 Operator : SY/MD
 Sample : VV1003MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK206

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

Signal : TIC: VV032211.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rBV	112692	117826	15.95%	2.027%
2	1.420	111	118	128	rBV7	3363	5697	0.77%	0.098%
3	1.532	145	153	171	rVB	90485	107819	14.59%	1.855%
4	2.060	307	317	333	rBV	177241	257926	34.91%	4.437%
5	2.371	412	414	417	rVB2	419	243	0.03%	0.004%
6	2.420	427	429	431	rVV	449	198	0.03%	0.003%
7	2.449	431	438	451	rVB3	4504	6840	0.93%	0.118%
8	2.516	456	459	463	rVB2	343	255	0.03%	0.004%
9	2.593	480	483	486	rVB2	465	306	0.04%	0.005%
10	2.719	518	522	526	rBV2	229	195	0.03%	0.003%
11	2.789	539	544	550	rBV2	255	398	0.05%	0.007%
12	3.224	677	679	684	rVB	342	273	0.04%	0.005%
13	3.252	684	688	692	rBV	402	340	0.05%	0.006%
14	3.275	692	695	700	rVB	144	159	0.02%	0.003%
15	3.574	786	788	796	rVB2	131	129	0.02%	0.002%
16	3.667	814	817	821	rVB2	169	131	0.02%	0.002%
17	3.789	846	855	879	rBV	54641	140195	18.98%	2.412%
18	4.252	982	999	1029	rBV	110388	290757	39.35%	5.002%
19	4.529	1080	1085	1089	rVB3	324	257	0.03%	0.004%
20	4.551	1089	1092	1094	rBV2	140	119	0.02%	0.002%
21	4.580	1099	1101	1105	rVB2	336	151	0.02%	0.003%
22	4.683	1131	1133	1140	rVB3	320	299	0.04%	0.005%
23	4.725	1140	1146	1147	rBV	162	139	0.02%	0.002%
24	4.738	1147	1150	1152	rVB	201	130	0.02%	0.002%
25	4.873	1190	1192	1197	rVB	190	122	0.02%	0.002%
26	4.960	1201	1219	1245	rBV2	280689	738811	100.00%	12.710%
27	5.265	1313	1314	1318	rVB	324	139	0.02%	0.002%
28	5.288	1318	1321	1322	rBV2	395	220	0.03%	0.004%
29	5.410	1354	1359	1361	rBV3	307	190	0.03%	0.003%
30	5.535	1387	1398	1425	rBV	226582	478533	64.77%	8.233%
31	5.831	1479	1490	1502	rBV2	12233	25559	3.46%	0.440%
32	5.992	1526	1540	1581	rBV	162382	347141	46.99%	5.972%
33	6.198	1602	1604	1608	rVB	254	152	0.02%	0.003%
34	6.230	1612	1614	1619	rVV4	363	252	0.03%	0.004%
35	6.259	1619	1623	1628	rVB4	450	402	0.05%	0.007%
36	6.336	1646	1647	1651	rVB2	256	139	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
 Data File : VV032211.D
 Acq On : 03 Oct 2023 12:43
 Operator : SY/MD
 Sample : VV1003MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK206

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

37	6.365	1651	1656	1661	rVB2	309	342	0.05%	0.006%
38	6.583	1719	1724	1726	rBV3	487	485	0.07%	0.008%
39	6.677	1749	1753	1756	rBV2	213	173	0.02%	0.003%
40	6.699	1758	1760	1763	rVV3	311	165	0.02%	0.003%
41	6.918	1817	1828	1864	rBV	83656	167106	22.62%	2.875%
42	7.127	1890	1893	1895	rBV3	431	306	0.04%	0.005%
43	7.246	1918	1930	1963	rBV	340051	608099	82.31%	10.462%
44	7.558	2016	2027	2050	rBV2	57361	107385	14.53%	1.847%
45	7.770	2089	2093	2096	rVB2	297	145	0.02%	0.002%
46	7.844	2113	2116	2120	rBV2	242	161	0.02%	0.003%
47	7.873	2122	2125	2131	rBV2	286	296	0.04%	0.005%
48	7.973	2153	2156	2160	rBV	188	139	0.02%	0.002%
49	8.030	2164	2174	2211	rBV	153617	314645	42.59%	5.413%
50	8.345	2270	2272	2274	rBV	374	181	0.02%	0.003%
51	8.509	2320	2323	2327	rBV2	219	139	0.02%	0.002%
52	8.529	2327	2329	2333	rVB	222	147	0.02%	0.003%
53	8.574	2339	2343	2347	rVB3	433	363	0.05%	0.006%
54	8.731	2388	2392	2397	rVB2	162	160	0.02%	0.003%
55	8.786	2398	2409	2429	rBV	353202	591639	80.08%	10.178%
56	8.995	2470	2474	2479	rVB2	467	334	0.05%	0.006%
57	9.056	2490	2493	2495	rBV	236	121	0.02%	0.002%
58	9.863	2741	2744	2745	rBV2	268	139	0.02%	0.002%
59	9.924	2757	2763	2768	rBV2	155	251	0.03%	0.004%
60	9.979	2775	2780	2782	rBV2	170	139	0.02%	0.002%
61	10.156	2824	2835	2854	rBV	207077	329244	44.56%	5.664%
62	10.275	2870	2872	2878	rVB	340	161	0.02%	0.003%
63	10.307	2878	2882	2884	rBV	256	166	0.02%	0.003%
64	10.320	2884	2886	2890	rBV	202	170	0.02%	0.003%
65	10.432	2917	2921	2923	rBV2	142	119	0.02%	0.002%
66	10.615	2975	2978	2983	rVB2	167	138	0.02%	0.002%
67	10.741	3014	3017	3021	rBV2	120	127	0.02%	0.002%
68	10.860	3051	3054	3055	rBV2	233	120	0.02%	0.002%
69	11.095	3123	3127	3134	rVB3	222	209	0.03%	0.004%
70	11.127	3134	3137	3138	rBV2	380	236	0.03%	0.004%
71	11.188	3145	3156	3178	rBV	395558	609120	82.45%	10.479%
72	11.564	3261	3273	3294	rBV	345056	544612	73.71%	9.369%
73	11.709	3315	3318	3320	rBV3	203	135	0.02%	0.002%
74	11.744	3325	3329	3331	rBV2	186	156	0.02%	0.003%
75	12.162	3456	3459	3462	rBV2	177	123	0.02%	0.002%
76	12.178	3462	3464	3465	rBV2	319	119	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
 Data File : VV032211.D
 Acq On : 03 Oct 2023 12:43
 Operator : SY/MD
 Sample : VV1003MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK206

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

77	12.429	3540	3542	3548	rVB	293	181	0.02%	0.003%
78	12.468	3553	3554	3557	rVB2	390	149	0.02%	0.003%
79	12.516	3564	3569	3573	rBV	212	230	0.03%	0.004%
80	12.570	3584	3586	3589	rBV2	210	139	0.02%	0.002%
81	12.590	3589	3592	3597	rVB	436	448	0.06%	0.008%
82	12.699	3624	3626	3630	rBV	252	137	0.02%	0.002%
83	12.812	3658	3661	3664	rBV	167	150	0.02%	0.003%
84	12.943	3700	3702	3708	rVB	245	143	0.02%	0.002%
85	13.207	3779	3784	3785	rBV2	781	585	0.08%	0.010%
86	13.281	3804	3807	3812	rBV	217	171	0.02%	0.003%
87	13.451	3852	3860	3871	rBV3	3663	5404	0.73%	0.093%
88	13.493	3871	3873	3876	rVB2	381	145	0.02%	0.002%
89	13.551	3890	3891	3895	rVB	337	161	0.02%	0.003%
90	13.686	3927	3933	3945	rBV6	1223	1771	0.24%	0.030%
91	13.853	3982	3985	3989	rVB	306	212	0.03%	0.004%
92	14.088	4056	4058	4064	rBV3	169	214	0.03%	0.004%
93	14.188	4082	4089	4094	rBV2	339	438	0.06%	0.008%
94	14.213	4094	4097	4098	rBV3	233	154	0.02%	0.003%
95	14.223	4098	4100	4105	rVV2	350	218	0.03%	0.004%
96	14.271	4113	4115	4117	rBV2	256	144	0.02%	0.002%
97	14.718	4251	4254	4256	rBV2	308	212	0.03%	0.004%
98	15.101	4370	4373	4375	rBV	414	217	0.03%	0.004%
99	15.120	4376	4379	4382	rBV2	432	330	0.04%	0.006%
100	15.519	4500	4503	4504	rBV3	484	269	0.04%	0.005%


Sum of corrected areas: 5812679

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
Data File : VV032211.D
Acq On : 03 Oct 2023 12:43
Operator : SY/MD
Sample : VV1003MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK206

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

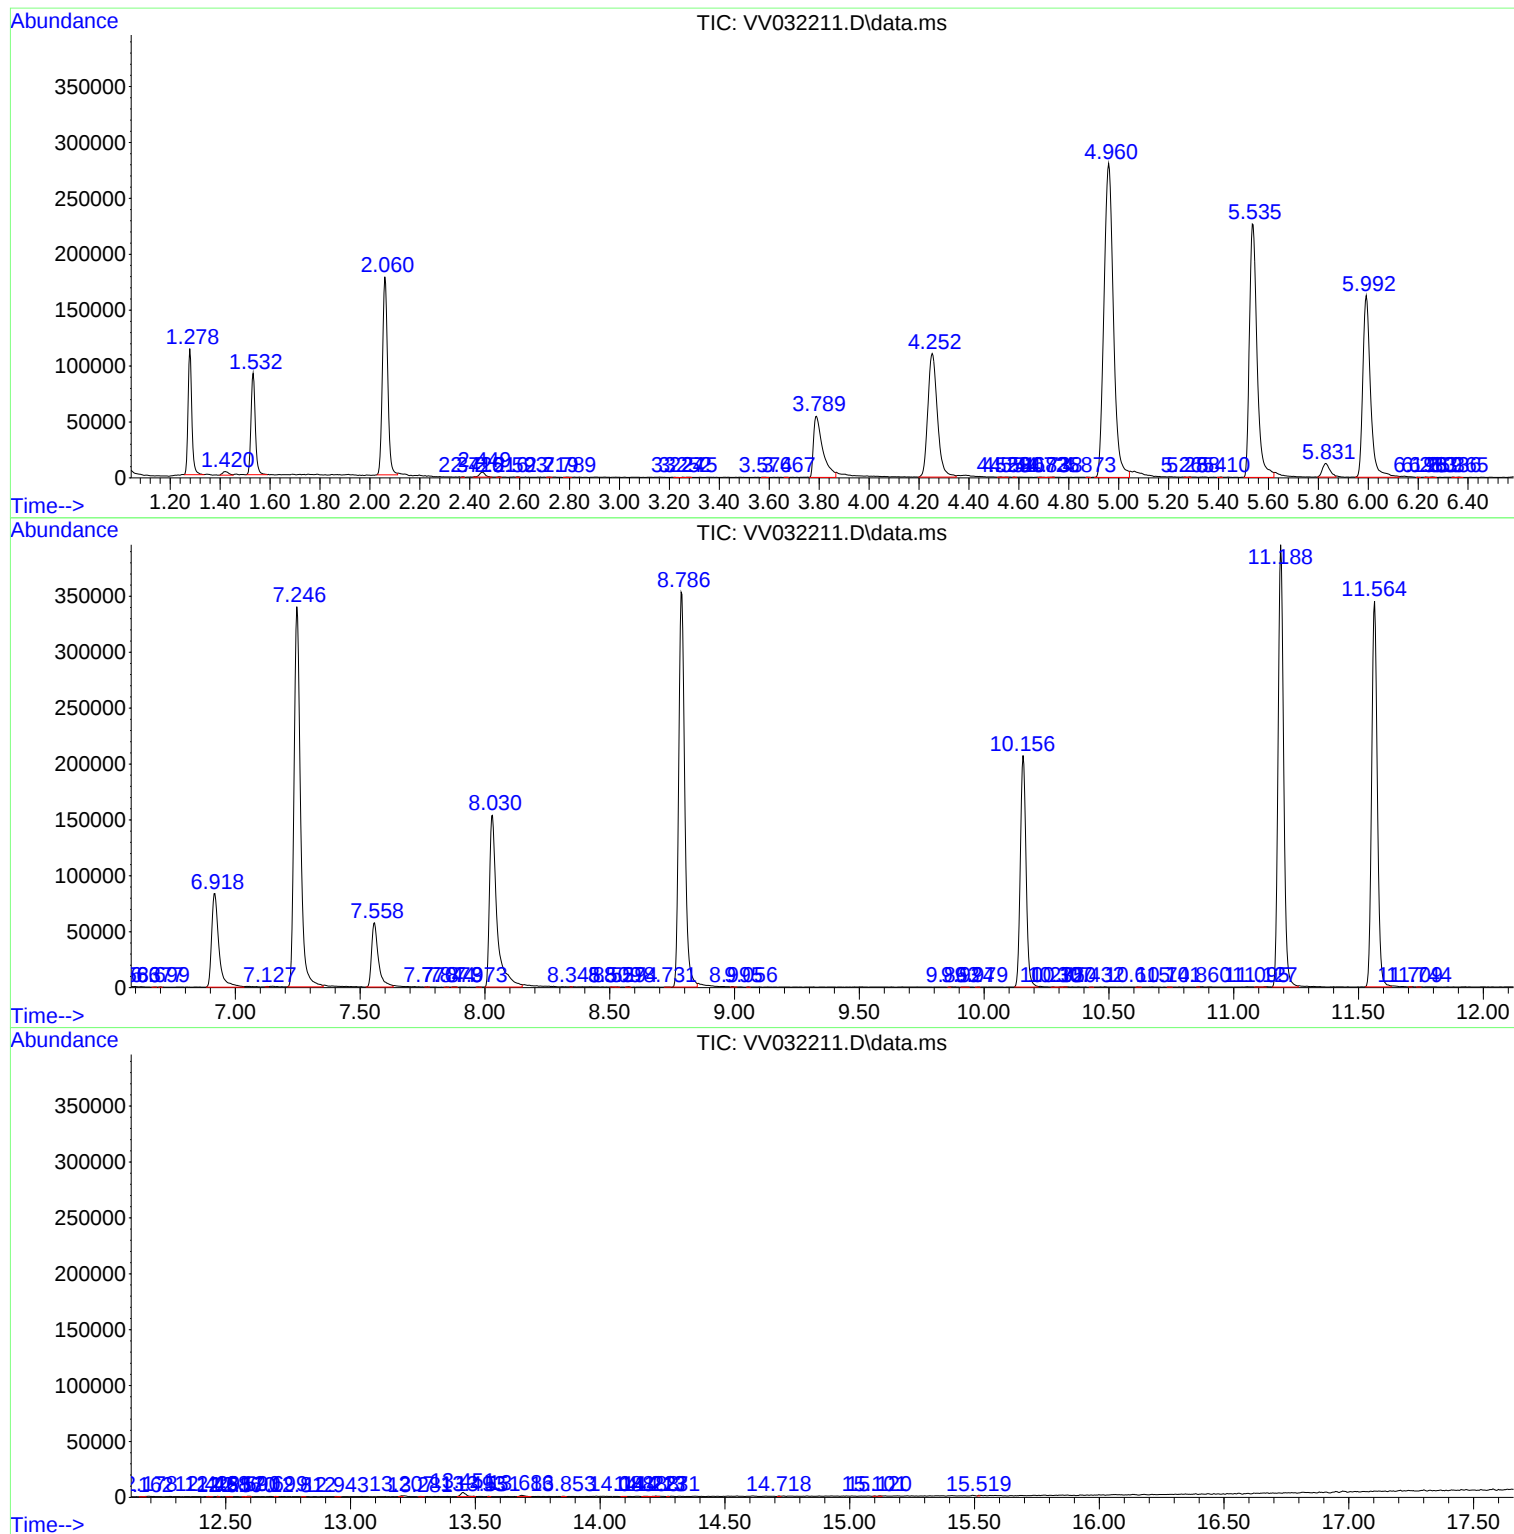

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
Data File : VV032211.D
Acq On : 03 Oct 2023 12:43
Operator : SY/MD
Sample : VV1003MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK206

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
Data File : VV032211.D
Acq On : 03 Oct 2023 12:43
Operator : SY/MD
Sample : VV1003MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK206

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc