

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
 Data File : VV032212.D
 Acq On : 03 Oct 2023 13:05
 Operator : SY/MD
 Sample : 04592-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

Signal : TIC: VV032212.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	108445	113027	15.79%	2.007%
2	1.532	146	153	167	rVB	88833	103669	14.48%	1.841%
3	2.060	308	317	333	rBV	168221	244564	34.17%	4.343%
4	2.343	404	405	409	rBV	249	111	0.02%	0.002%
5	2.397	420	422	426	rVB	398	152	0.02%	0.003%
6	2.449	431	438	449	rVB2	4081	6603	0.92%	0.117%
7	2.587	479	481	484	rBV2	145	85	0.01%	0.002%
8	2.722	521	523	527	rVB3	172	110	0.02%	0.002%
9	2.979	600	603	605	rBV	161	125	0.02%	0.002%
10	3.089	634	637	641	rVB	291	193	0.03%	0.003%
11	3.179	660	665	667	rBV	243	140	0.02%	0.002%
12	3.227	677	680	683	rBV2	207	101	0.01%	0.002%
13	3.246	684	686	689	rVB	211	98	0.01%	0.002%
14	3.265	689	692	694	rBV	114	85	0.01%	0.002%
15	3.278	694	696	698	rVB	252	110	0.02%	0.002%
16	3.343	707	716	720	rBV	281	311	0.04%	0.006%
17	3.452	747	750	755	rVB	202	174	0.02%	0.003%
18	3.532	772	775	777	rBV	100	86	0.01%	0.002%
19	3.626	800	804	808	rBV	146	140	0.02%	0.002%
20	3.693	822	825	829	rVV2	117	104	0.01%	0.002%
21	3.790	846	855	888	rBV	55962	149652	20.91%	2.658%
22	4.172	971	974	976	rBV2	359	231	0.03%	0.004%
23	4.253	983	999	1027	rBV	107194	281844	39.38%	5.005%
24	4.651	1121	1123	1127	rBV2	246	137	0.02%	0.002%
25	4.677	1127	1131	1133	rBV	311	204	0.03%	0.004%
26	4.744	1150	1152	1156	rVB	186	78	0.01%	0.001%
27	4.786	1161	1165	1166	rBV	126	86	0.01%	0.002%
28	4.851	1178	1185	1189	rBV3	337	425	0.06%	0.008%
29	4.902	1198	1201	1202	rBV2	208	119	0.02%	0.002%
30	4.960	1203	1219	1241	rBV2	272135	715703	100.00%	12.710%
31	5.211	1295	1297	1301	rBV2	349	239	0.03%	0.004%
32	5.320	1328	1331	1334	rBV2	159	122	0.02%	0.002%
33	5.371	1345	1347	1349	rBV	106	67	0.01%	0.001%
34	5.468	1374	1377	1379	rBV	100	67	0.01%	0.001%
35	5.484	1379	1382	1385	rBV2	195	118	0.02%	0.002%
36	5.539	1385	1399	1428	rBV	219866	463911	64.82%	8.238%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100323\
 Data File : VW032212.D
 Acq On : 03 Oct 2023 13:05
 Operator : SY/MD
 Sample : 04592-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

37	5.831	1479	1490	1506	rBV4	12465	26879	3.76%	0.477%
38	5.918	1514	1517	1518	rBV	116	70	0.01%	0.001%
39	5.992	1527	1540	1578	rBV	157663	337263	47.12%	5.989%
40	6.236	1614	1616	1618	rVB	282	99	0.01%	0.002%
41	6.272	1624	1627	1629	rBV	179	112	0.02%	0.002%
42	6.291	1630	1633	1639	rVB2	288	260	0.04%	0.005%
43	6.394	1662	1665	1668	rBV	121	90	0.01%	0.002%
44	6.461	1684	1686	1689	rBV2	200	117	0.02%	0.002%
45	6.516	1699	1703	1706	rBV2	106	93	0.01%	0.002%
46	6.574	1714	1721	1722	rBV2	455	310	0.04%	0.006%
47	6.603	1727	1730	1733	rBV4	545	423	0.06%	0.008%
48	6.680	1752	1754	1756	rVV	170	99	0.01%	0.002%
49	6.712	1760	1764	1765	rBV2	215	134	0.02%	0.002%
50	6.725	1766	1768	1772	rVV2	286	197	0.03%	0.003%
51	6.764	1778	1780	1786	rBV	161	91	0.01%	0.002%
52	6.809	1792	1794	1798	rVB	203	123	0.02%	0.002%
53	6.834	1800	1802	1806	rBV2	81	66	0.01%	0.001%
54	6.918	1816	1828	1857	rBV2	81640	161223	22.53%	2.863%
55	7.111	1884	1888	1891	rBV	277	237	0.03%	0.004%
56	7.246	1919	1930	1959	rBV	319074	583657	81.55%	10.365%
57	7.558	2017	2027	2047	rBV	54865	103009	14.39%	1.829%
58	7.777	2093	2095	2100	rVB3	340	139	0.02%	0.002%
59	7.873	2123	2125	2127	rBV3	147	100	0.01%	0.002%
60	7.908	2133	2136	2138	rVB2	124	69	0.01%	0.001%
61	8.027	2164	2173	2212	rBV	153876	318223	44.46%	5.651%
62	8.323	2263	2265	2269	rBV2	260	112	0.02%	0.002%
63	8.471	2309	2311	2313	rBV2	305	172	0.02%	0.003%
64	8.484	2313	2315	2317	rVV2	278	142	0.02%	0.003%
65	8.519	2323	2326	2327	rBV	334	157	0.02%	0.003%
66	8.555	2334	2337	2340	rBV2	207	159	0.02%	0.003%
67	8.571	2340	2342	2346	rBV3	304	167	0.02%	0.003%
68	8.612	2352	2355	2360	rVB2	193	142	0.02%	0.003%
69	8.683	2374	2377	2378	rBV	190	80	0.01%	0.001%
70	8.786	2398	2409	2434	rBV	343093	575317	80.38%	10.217%
71	9.140	2515	2519	2522	rBV2	156	124	0.02%	0.002%
72	9.230	2544	2547	2549	rBV	135	93	0.01%	0.002%
73	9.381	2592	2594	2597	rVB2	238	90	0.01%	0.002%
74	9.445	2612	2614	2617	rVB2	190	81	0.01%	0.001%
75	9.474	2620	2623	2628	rBV3	197	182	0.03%	0.003%
76	9.664	2679	2682	2684	rBV	154	116	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
 Data File : VV032212.D
 Acq On : 03 Oct 2023 13:05
 Operator : SY/MD
 Sample : 04592-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

77	9.831	2731	2734	2738	rVV2	218	137	0.02%	0.002%
78	9.886	2747	2751	2755	rBV2	241	189	0.03%	0.003%
79	9.966	2773	2776	2779	rBV2	118	75	0.01%	0.001%
80	10.075	2806	2810	2815	rBV2	95	99	0.01%	0.002%
81	10.156	2823	2835	2856	rBV	203422	323714	45.23%	5.749%
82	10.281	2869	2874	2877	rBV	294	281	0.04%	0.005%
83	10.297	2877	2879	2882	rVV	145	86	0.01%	0.002%
84	10.760	3018	3023	3026	rBV2	211	237	0.03%	0.004%
85	11.075	3119	3121	3125	rVB2	218	90	0.01%	0.002%
86	11.137	3137	3140	3145	rBV2	254	192	0.03%	0.003%
87	11.188	3145	3156	3178	rBV	375756	583089	81.47%	10.355%
88	11.397	3217	3221	3225	rVB3	329	213	0.03%	0.004%
89	11.564	3261	3273	3298	rBV	336814	527472	73.70%	9.367%
90	11.780	3338	3340	3343	rBV2	171	67	0.01%	0.001%
91	11.902	3376	3378	3380	rBV2	180	106	0.01%	0.002%
92	11.937	3387	3389	3391	rBV	205	90	0.01%	0.002%
93	12.050	3421	3424	3428	rBV2	252	171	0.02%	0.003%
94	12.468	3552	3554	3556	rBV	210	94	0.01%	0.002%
95	12.706	3626	3628	3630	rBV	356	168	0.02%	0.003%
96	12.866	3675	3678	3681	rBV	230	179	0.03%	0.003%
97	12.982	3709	3714	3716	rBV3	235	208	0.03%	0.004%
98	13.204	3781	3783	3784	rBV	366	146	0.02%	0.003%
99	13.558	3887	3893	3897	rBV2	240	412	0.06%	0.007%
100	13.805	3966	3970	3973	rBV2	439	299	0.04%	0.005%




Sum of corrected areas: 5631022

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
Data File : VV032212.D
Acq On : 03 Oct 2023 13:05
Operator : SY/MD
Sample : 04592-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

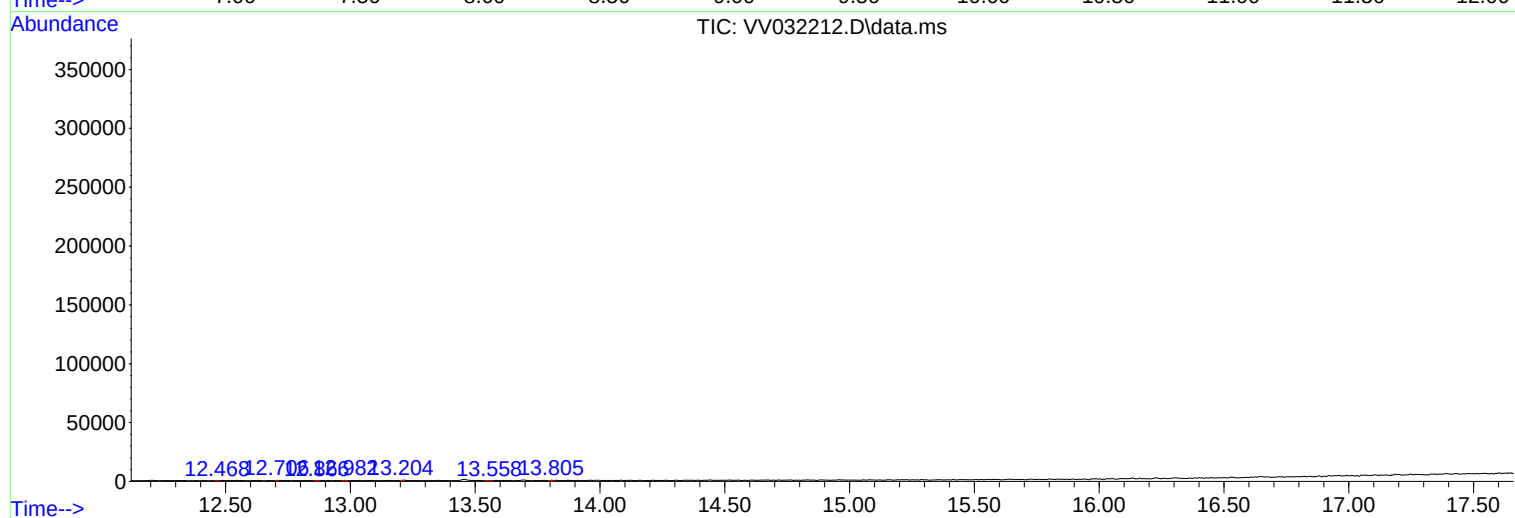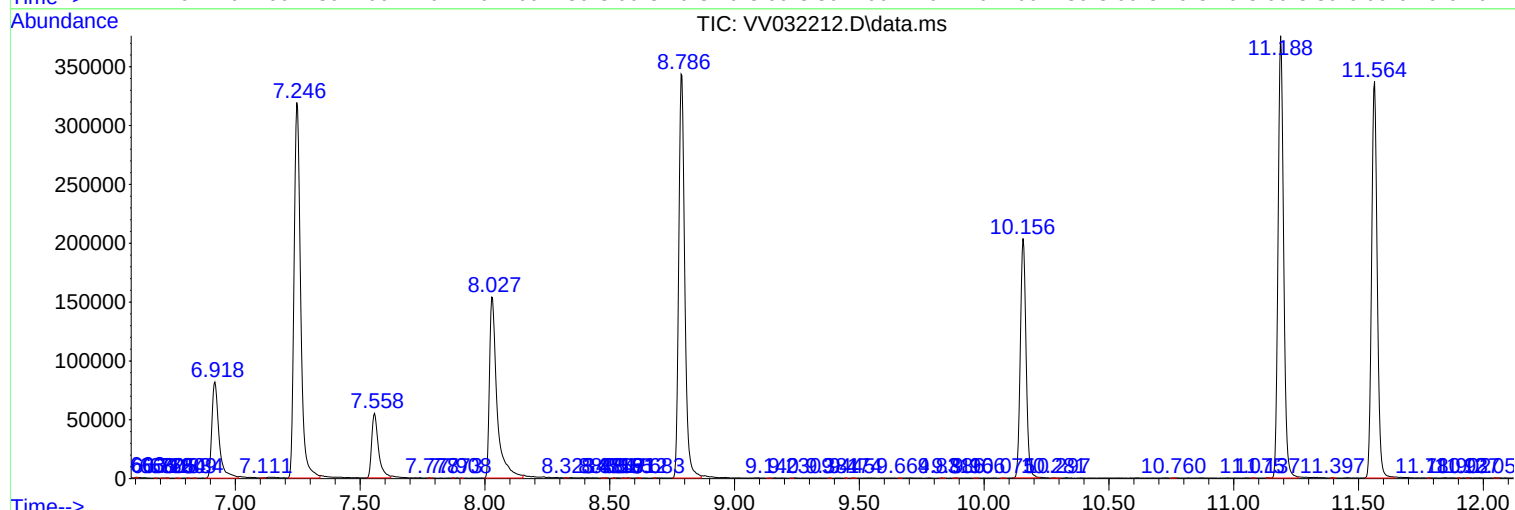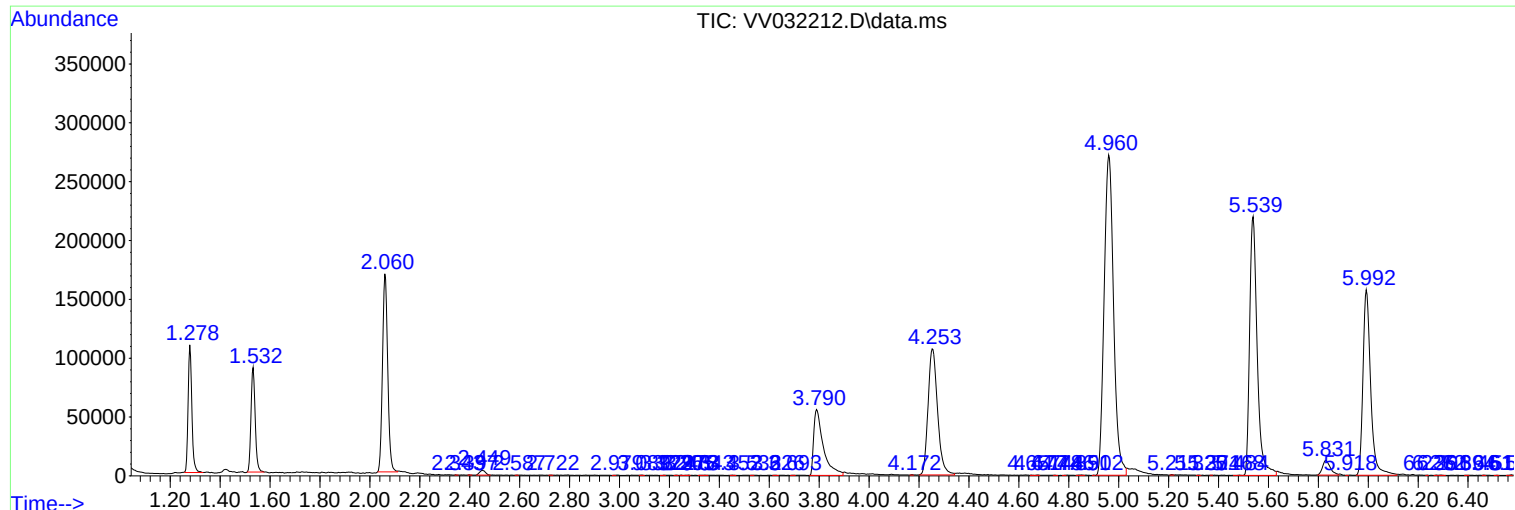

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
Data File : VV032212.D
Acq On : 03 Oct 2023 13:05
Operator : SY/MD
Sample : 04592-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
Data File : VV032212.D
Acq On : 03 Oct 2023 13:05
Operator : SY/MD
Sample : 04592-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------