


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100323\
Data File : VV032206.D
Acq On : 03 Oct 2023 08:47
Operator : SY/MD
Sample : BFB219
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB219

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Title : VOC Analysis
Last Update : Wed Oct 04 04:04:33 2023

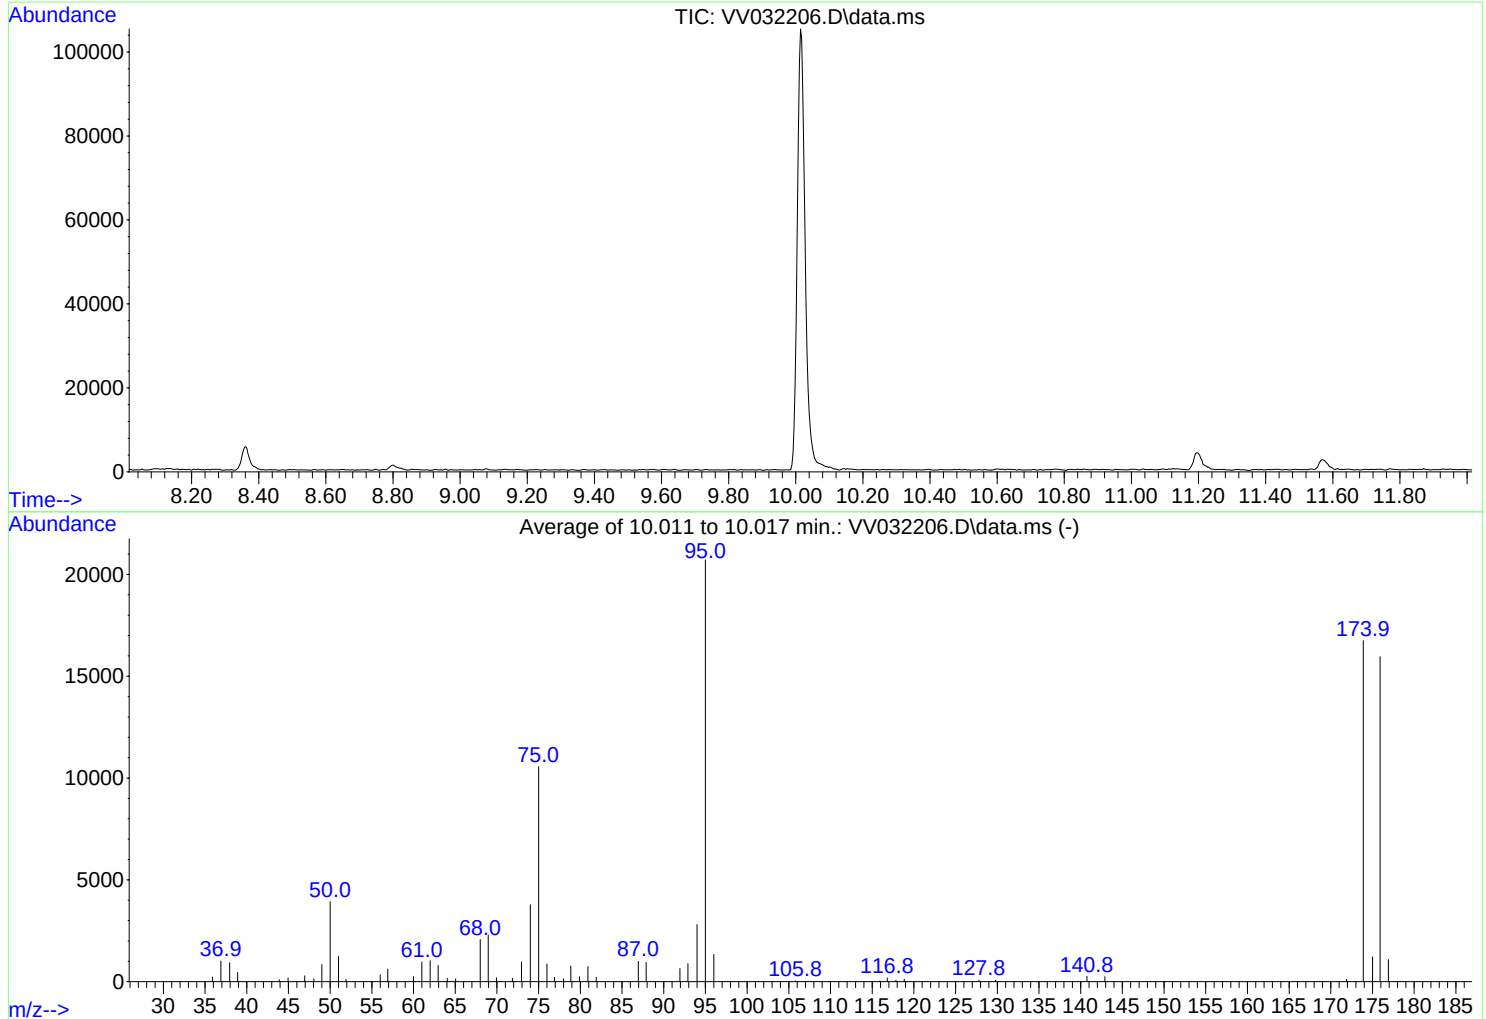

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	3921	PASS
75	95	30	80	51.0	10557	PASS
95	95	100	100	100.0	20717	PASS
96	95	5	9	6.5	1338	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.9	16750	PASS
175	174	5	9	7.3	1219	PASS
176	174	95	105	95.3	15964	PASS
177	176	5	10	6.8	1088	PASS

m/z	Abundance
39.90	175.0
44.00	286.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

m/z	Abundance
36.00	215.0
36.90	985.0
37.90	949.0
38.90	417.0
39.90	185.0
43.90	386.0
45.00	174.0
46.90	290.0
48.10	129.0
49.00	803.0
50.00	3937.0
51.00	1162.0
51.90	110.0
56.00	334.0
56.90	581.0
60.00	240.0
61.00	972.0
62.00	977.0
63.00	823.0
64.00	188.0
65.10	107.0
68.00	1999.0
68.90	2404.0
69.90	197.0
71.80	145.0
73.00	956.0
74.00	3675.0
75.00	10437.0
76.00	834.0
76.90	193.0
78.00	122.0
78.80	773.0
79.90	232.0
80.90	707.0
81.90	197.0
87.00	911.0
87.90	935.0
91.90	605.0
92.90	798.0
94.00	2659.0
95.00	19832.0
96.00	1257.0
105.80	129.0
116.80	189.0
118.90	120.0
127.80	115.0
129.80	104.0
140.70	231.0
142.90	214.0
171.90	125.0
173.90	15513.0
175.00	1157.0
175.90	14620.0
176.90	1054.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

m/z	Abundance
35.90	219.0
36.90	1047.0
37.90	985.0
38.90	476.0
39.80	189.0
43.90	382.0
45.00	182.0
47.00	297.0
48.00	136.0
49.00	853.0
50.00	4064.0
51.00	1266.0
51.90	129.0
56.00	347.0
56.90	632.0
60.00	259.0
61.00	1000.0
62.00	1090.0
63.00	858.0
64.10	149.0
65.10	145.0
68.00	2130.0
68.90	2385.0
69.90	180.0
71.80	169.0
73.00	1011.0
74.00	3909.0
75.00	10893.0
76.00	914.0
76.90	211.0
78.00	147.0
78.90	801.0
79.90	252.0
80.90	744.0
81.90	219.0
86.90	1051.0
87.90	947.0
91.90	662.0
92.90	904.0
94.00	2931.0
95.00	21408.0
96.00	1388.0
116.80	188.0
117.90	100.0
118.80	117.0
127.80	107.0
129.80	106.0
140.80	273.0
142.90	254.0
171.90	116.0
173.90	17344.0
175.00	1233.0
175.90	16544.0
176.90	1122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

m/z	Abundance
35.00	247.0
36.00	1008.0
38.00	861.0
38.00	461.0
39.00	176.0
43.00	373.0
44.00	191.0
47.00	263.0
48.00	163.0
49.00	873.0
50.00	3763.0
51.00	1299.0
51.00	125.0
56.00	322.0
56.00	621.0
60.00	244.0
61.00	925.0
62.00	1033.0
62.00	733.0
64.00	124.0
65.00	155.0
68.00	2077.0
69.00	2070.0
70.00	180.0
71.00	171.0
72.00	933.0
74.00	3746.0
75.00	10340.0
76.00	864.0
76.00	215.0
78.00	147.0
78.00	738.0
79.00	246.0
80.00	763.0
81.00	222.0
86.00	1036.0
87.00	956.0
92.00	675.0
92.00	931.0
94.00	2819.0
95.00	20912.0
96.00	1369.0
115.00	101.0
116.00	167.0
117.00	109.0
118.00	132.0
140.00	271.0
142.00	265.0
171.00	120.0
173.00	17392.0
175.00	1268.0
175.00	16728.0
176.00	1087.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219