

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
 Data File : VV037726.D
 Acq On : 03 Oct 2024 13:49
 Operator : SY/MD
 Sample : P4284-05
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD4

Quant Time: Oct 04 02:28:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 04 02:26:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	665974	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	648140	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	300837	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	225708	38.608	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	77.220%		
7) Chloroethane-d5	1.532	69	193193	42.573	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	85.140%		
11) 1,1-Dichloroethene-d2	2.059	65	100189	41.019	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.040%		
21) 2-Butanone-d5	3.789	46	172691	82.933	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	82.930%		
24) Chloroform-d	4.239	84	442777	42.570	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.140%		
26) 1,2-Dichloroethane-d4	4.931	65	266530	43.779	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.560%		
32) Benzene-d6	4.950	84	864086	42.604	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.200%		
36) 1,2-Dichloropropane-d6	5.979	67	278682	43.151	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	86.300%		
41) Toluene-d8	7.236	98	735871	40.013	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	80.020%		
43) trans-1,3-Dichloroprop...	7.548	79	119086	39.694	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	79.380%		
47) 2-Hexanone-d5	8.021	63	96958	71.098	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	71.100%		
56) 1,1,2,2-Tetrachloroeth...	10.143	84	298991	39.844	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	79.680%		
66) 1,2-Dichlorobenzene-d4	11.551	152	290377	45.806	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.620%		
Target Compounds					Qvalue	
13) Acetone	2.111	43	64029	31.367	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
Data File : VV037726.D
Acq On : 03 Oct 2024 13:49
Operator : SY/MD
Sample : P4284-05
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD4

Quant Time: Oct 04 02:28:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 04 02:26:43 2024
Response via : Initial Calibration

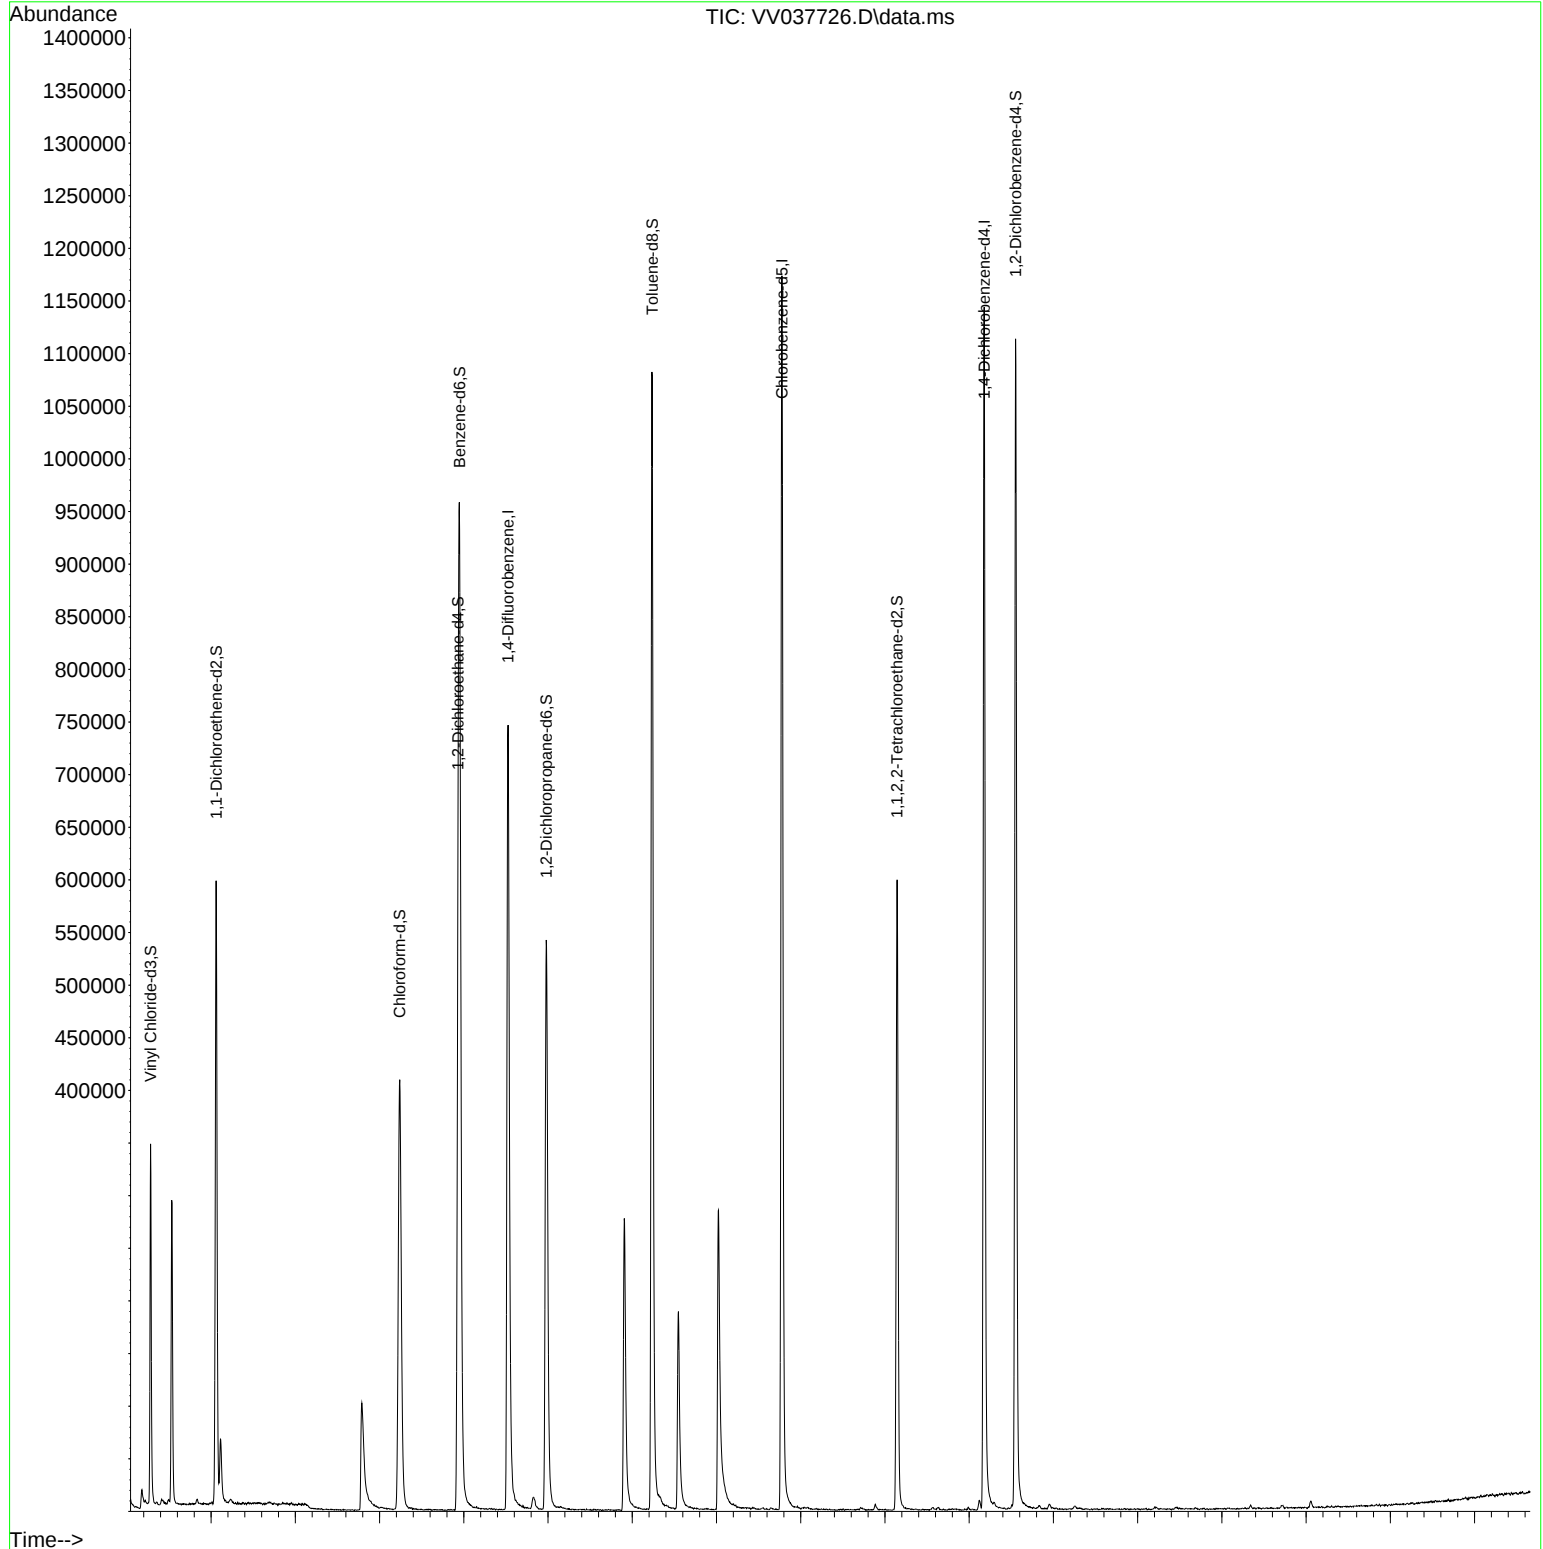

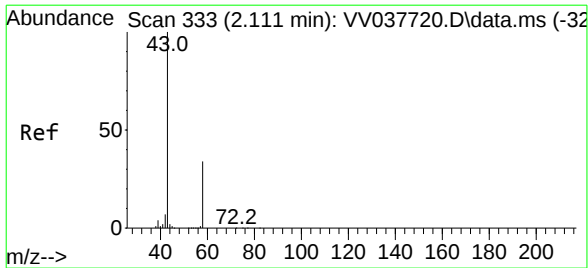

#13
Acetone
Concen: 31.367 ug/L
RT: 2.111 min Scan# 33
Delta R.T. 0.000 min
Lab File: VV037726.D
Acq: 03 Oct 2024 13:49

Instrument :
MSVOA_V
ClientSampleId :
A4FD4

Tgt Ion: 43	Resp: 64029
Ion Ratio	Lower Upper
43	100
58	33.5 0.0 66.6

