

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
 Data File : VV037722.D
 Acq On : 03 Oct 2024 09:18
 Operator : SY/MD
 Sample : VV1003WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK229

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.182	36	44	51	rBV	5757	10779	0.39%	0.056%
2	1.282	67	75	90	rBV	393626	430799	15.74%	2.256%
3	1.532	145	153	166	rVB	330284	390457	14.26%	2.045%
4	2.060	307	317	341	rVB	692610	996457	36.40%	5.218%
5	3.317	704	708	711	rBV5	872	899	0.03%	0.005%
6	3.423	737	741	744	rBV2	858	622	0.02%	0.003%
7	3.462	750	753	755	rVB4	991	533	0.02%	0.003%
8	3.542	771	778	780	rBV5	663	644	0.02%	0.003%
9	3.696	822	826	833	rVB4	1174	1082	0.04%	0.006%
10	3.741	838	840	845	rBV3	565	427	0.02%	0.002%
11	3.793	848	856	885	rBV	103871	298480	10.90%	1.563%
12	4.153	965	968	972	rVV4	1264	870	0.03%	0.005%
13	4.243	978	996	1029	rBV	440816	1126650	41.16%	5.900%
14	4.426	1050	1053	1058	rVB5	822	618	0.02%	0.003%
15	4.484	1067	1071	1074	rVB4	867	720	0.03%	0.004%
16	4.506	1074	1078	1080	rBV3	718	586	0.02%	0.003%
17	4.574	1095	1099	1103	rVB4	557	492	0.02%	0.003%
18	4.638	1114	1119	1124	rBV5	1127	1193	0.04%	0.006%
19	4.670	1124	1129	1132	rVB4	699	709	0.03%	0.004%
20	4.783	1159	1164	1166	rBV4	520	446	0.02%	0.002%
21	4.950	1200	1216	1248	rBV2	1087108	2737514	100.00%	14.336%
22	5.307	1324	1327	1330	rBV3	1498	1057	0.04%	0.006%
23	5.368	1344	1346	1348	rBV3	1013	418	0.02%	0.002%
24	5.400	1352	1356	1362	rVB4	1161	1309	0.05%	0.007%
25	5.432	1362	1366	1371	rBV3	1327	1397	0.05%	0.007%
26	5.529	1385	1396	1431	rBV	689446	1432170	52.32%	7.500%
27	5.828	1479	1489	1501	rBV5	10416	23867	0.87%	0.125%
28	5.982	1523	1537	1561	rBV	600358	1245143	45.48%	6.521%
29	6.288	1630	1632	1636	rVB3	913	608	0.02%	0.003%
30	6.378	1654	1660	1662	rBV5	765	647	0.02%	0.003%
31	6.413	1666	1671	1673	rBV3	856	729	0.03%	0.004%
32	6.439	1673	1679	1682	rBV4	845	757	0.03%	0.004%
33	6.490	1693	1695	1703	rVB4	774	817	0.03%	0.004%
34	6.532	1703	1708	1714	rVB5	1059	1023	0.04%	0.005%
35	6.564	1714	1718	1719	rBV	737	541	0.02%	0.003%
36	6.629	1733	1738	1740	rBV3	790	506	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
Data File : VV037722.D
Acq On : 03 Oct 2024 09:18
Operator : SY/MD
Sample : VV1003WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

37	6.654	1743	1746	1750	rBV3	846	547	0.02%	0.003%
38	6.686	1751	1756	1757	rBV2	770	536	0.02%	0.003%
39	6.908	1814	1825	1858	rBV	305853	598826	21.87%	3.136%
40	7.236	1916	1927	1969	rBV	1241518	2196081	80.22%	11.501%
41	7.548	2015	2024	2064	rBV	204843	393725	14.38%	2.062%
42	7.805	2101	2104	2107	rBV3	927	619	0.02%	0.003%
43	7.911	2132	2137	2138	rBV5	769	636	0.02%	0.003%
44	7.953	2144	2150	2152	rBV4	790	842	0.03%	0.004%
45	8.024	2163	2172	2218	rVV2	301353	679907	24.84%	3.561%
46	8.490	2314	2317	2321	rBV3	721	661	0.02%	0.003%
47	8.529	2324	2329	2330	rBV4	764	561	0.02%	0.003%
48	8.548	2330	2335	2339	rBV6	1420	1423	0.05%	0.007%
49	8.677	2374	2375	2381	rVB4	859	505	0.02%	0.003%
50	8.709	2384	2385	2390	rVB4	758	520	0.02%	0.003%
51	8.780	2395	2407	2443	rBV	1083385	1807974	66.04%	9.468%
52	9.136	2516	2518	2522	rVB4	1028	497	0.02%	0.003%
53	9.169	2524	2528	2531	rBV3	1090	683	0.02%	0.004%
54	9.323	2573	2576	2581	rVB3	867	615	0.02%	0.003%
55	9.368	2587	2590	2593	rBV4	810	628	0.02%	0.003%
56	9.635	2667	2673	2675	rBV5	918	862	0.03%	0.005%
57	9.677	2684	2686	2693	rVB4	616	478	0.02%	0.003%
58	9.744	2700	2707	2710	rBV3	690	600	0.02%	0.003%
59	9.985	2777	2782	2784	rBV4	597	461	0.02%	0.002%
60	10.146	2820	2832	2855	rBV	657758	1054342	38.51%	5.521%
61	10.387	2904	2907	2911	rVB4	867	655	0.02%	0.003%
62	10.423	2911	2918	2920	rBV5	522	581	0.02%	0.003%
63	10.481	2933	2936	2937	rVV2	776	452	0.02%	0.002%
64	10.628	2978	2982	2984	rBV2	657	600	0.02%	0.003%
65	10.683	2996	2999	3004	rVB4	758	491	0.02%	0.003%
66	10.786	3025	3031	3035	rBV6	1373	1278	0.05%	0.007%
67	10.918	3068	3072	3079	rVB4	865	726	0.03%	0.004%
68	11.130	3130	3138	3139	rBV3	2228	2436	0.09%	0.013%
69	11.178	3142	3153	3177	rBV	1044699	1654440	60.44%	8.664%
70	11.551	3258	3269	3298	rBV	1190817	1930248	70.51%	10.109%
71	11.969	3396	3399	3401	rBV3	813	476	0.02%	0.002%
72	12.014	3411	3413	3416	rVB4	1032	548	0.02%	0.003%
73	12.030	3416	3418	3421	rBV3	745	505	0.02%	0.003%
74	12.050	3421	3424	3427	rBV	742	565	0.02%	0.003%
75	12.120	3442	3446	3449	rBV4	759	564	0.02%	0.003%
76	12.194	3466	3469	3473	rBV3	960	719	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
 Data File : VV037722.D
 Acq On : 03 Oct 2024 09:18
 Operator : SY/MD
 Sample : VV1003WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK229

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.233	3478	3481	3485	rBV3	754	668	0.02%	0.003%
78	12.542	3575	3577	3580	rVB2	789	520	0.02%	0.003%
79	12.590	3583	3592	3593	rBV5	1770	2072	0.08%	0.011%
80	12.696	3621	3625	3628	rBV3	765	568	0.02%	0.003%
81	12.857	3671	3675	3677	rBV2	784	621	0.02%	0.003%
82	12.908	3689	3691	3696	rVB4	693	489	0.02%	0.003%
83	12.963	3705	3708	3713	rVV4	937	801	0.03%	0.004%
84	12.988	3714	3716	3719	rVB2	939	525	0.02%	0.003%
85	13.127	3756	3759	3764	rVB2	924	625	0.02%	0.003%
86	13.210	3779	3785	3791	rVV7	3935	6465	0.24%	0.034%
87	13.236	3791	3793	3799	rVB5	2038	1634	0.06%	0.009%
88	13.406	3843	3846	3850	rBV2	606	471	0.02%	0.002%
89	13.448	3850	3859	3870	rBV	7407	15011	0.55%	0.079%
90	13.680	3924	3931	3943	rVV8	4252	7606	0.28%	0.040%
91	13.770	3957	3959	3963	rVB3	1290	644	0.02%	0.003%
92	13.889	3992	3996	3999	rBV4	704	733	0.03%	0.004%
93	13.905	3999	4001	4004	rVV2	821	573	0.02%	0.003%
94	14.101	4058	4062	4068	rBV4	967	1121	0.04%	0.006%
95	14.130	4068	4071	4076	rBV3	849	740	0.03%	0.004%
96	14.210	4089	4096	4099	rBV5	903	1228	0.04%	0.006%
97	14.561	4203	4205	4208	rBV3	732	453	0.02%	0.002%
98	14.721	4251	4255	4256	rBV3	843	759	0.03%	0.004%
99	14.876	4301	4303	4304	rBV2	1006	431	0.02%	0.002%
100	15.323	4440	4442	4444	rBV	1209	710	0.03%	0.004%




Sum of corrected areas: 19095247

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
Data File : VV037722.D
Acq On : 03 Oct 2024 09:18
Operator : SY/MD
Sample : VV1003WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

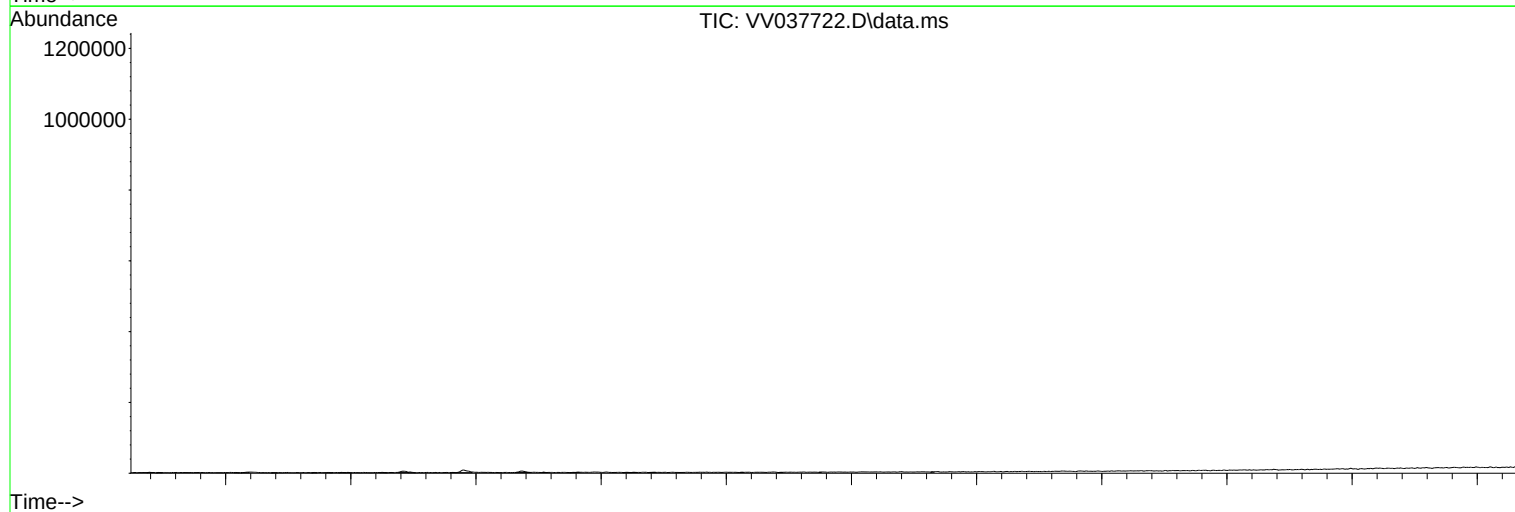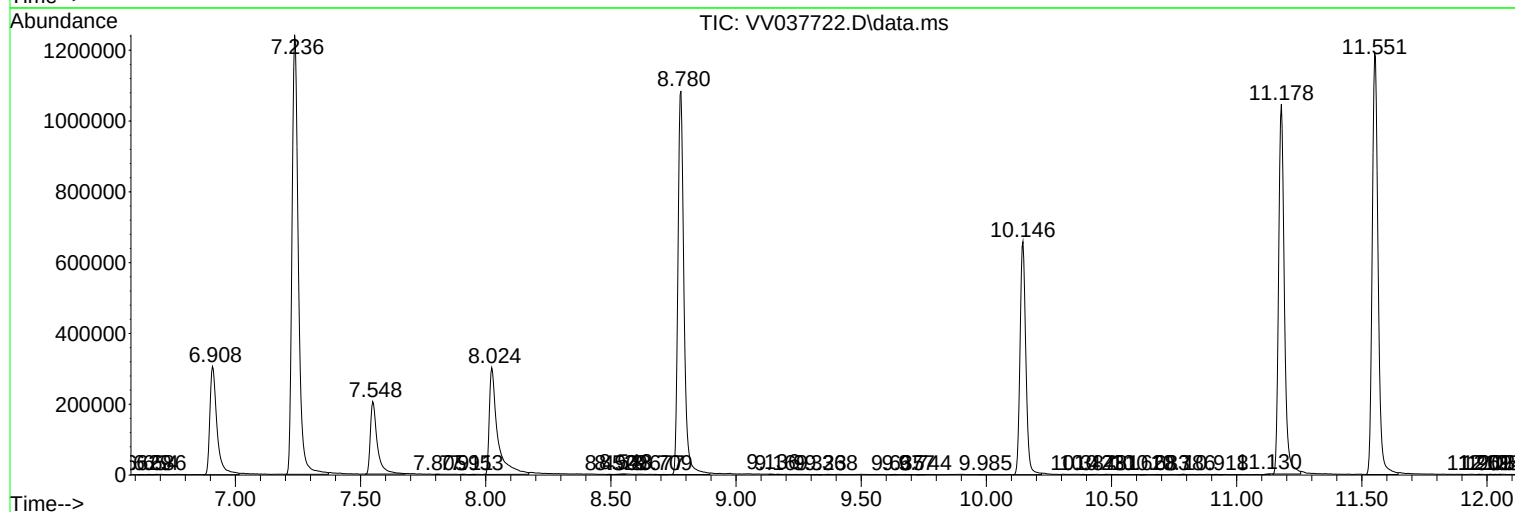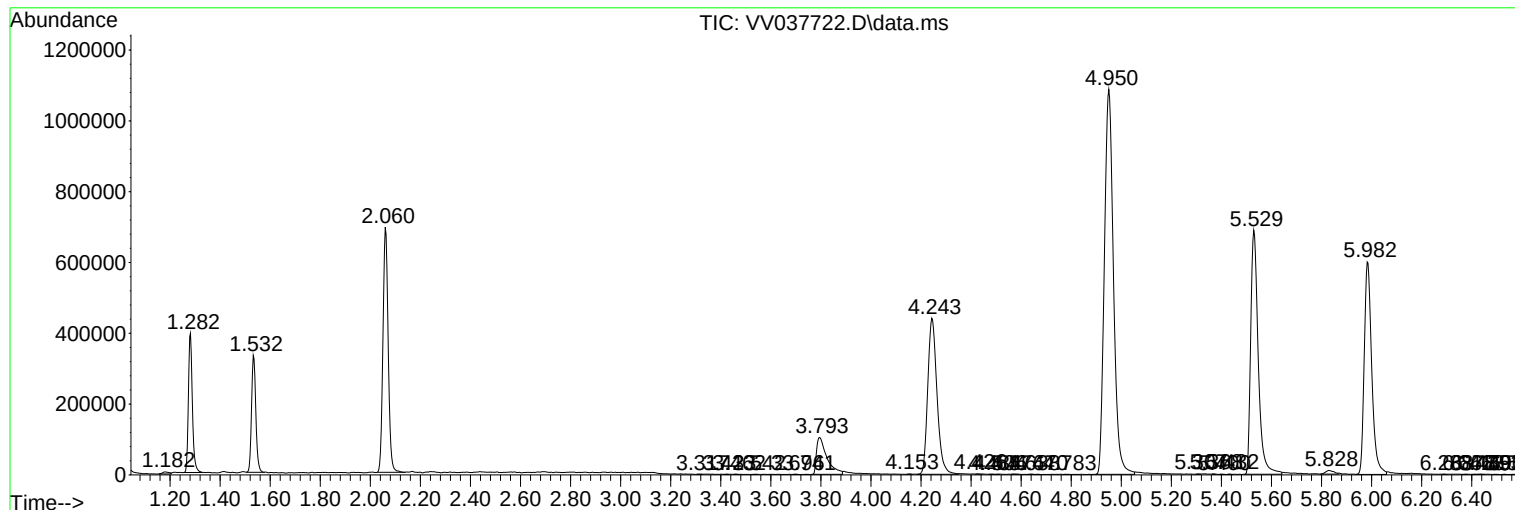

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
Data File : VV037722.D
Acq On : 03 Oct 2024 09:18
Operator : SY/MD
Sample : VV1003WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
Data File : VV037722.D
Acq On : 03 Oct 2024 09:18
Operator : SY/MD
Sample : VV1003WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
