

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
 Data File : VV037723.D
 Acq On : 03 Oct 2024 09:39
 Operator : SY/MD
 Sample : P4218-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	37	43	51	rBV	8207	13790	0.51%	0.072%
2	1.282	67	75	92	rBV	386872	419127	15.48%	2.196%
3	1.532	146	153	171	rVB	325634	389025	14.37%	2.038%
4	2.060	307	317	339	rVB	671249	976385	36.06%	5.115%
5	3.294	699	701	705	rVB4	1274	720	0.03%	0.004%
6	3.796	848	857	887	rBV	99939	286928	10.60%	1.503%
7	4.243	979	996	1021	rBV	435665	1111959	41.06%	5.826%
8	4.433	1051	1055	1057	rBV4	924	728	0.03%	0.004%
9	4.654	1119	1124	1130	rBV7	669	851	0.03%	0.004%
10	4.683	1130	1133	1138	rVB3	957	844	0.03%	0.004%
11	4.719	1138	1144	1146	rBV3	1008	1064	0.04%	0.006%
12	4.847	1179	1184	1185	rBV2	684	421	0.02%	0.002%
13	4.950	1200	1216	1254	rBV2	1063978	2707842	100.00%	14.187%
14	5.191	1289	1291	1296	rVB5	1211	655	0.02%	0.003%
15	5.227	1300	1302	1308	rVB4	929	782	0.03%	0.004%
16	5.310	1325	1328	1331	rBV4	656	590	0.02%	0.003%
17	5.474	1376	1379	1384	rVB5	874	557	0.02%	0.003%
18	5.529	1384	1396	1432	rBV	717239	1496455	55.26%	7.840%
19	5.828	1481	1489	1503	rBV6	8398	19182	0.71%	0.100%
20	5.982	1525	1537	1567	rBV	595794	1232794	45.53%	6.459%
21	6.236	1613	1616	1619	rVB5	1537	941	0.03%	0.005%
22	6.281	1628	1630	1632	rVV3	1123	503	0.02%	0.003%
23	6.310	1635	1639	1644	rVB5	909	986	0.04%	0.005%
24	6.336	1644	1647	1648	rBV	741	471	0.02%	0.002%
25	6.355	1651	1653	1658	rVB4	1237	723	0.03%	0.004%
26	6.458	1679	1685	1687	rVV4	1009	809	0.03%	0.004%
27	6.481	1690	1692	1694	rVV3	997	540	0.02%	0.003%
28	6.764	1778	1780	1786	rVB4	628	442	0.02%	0.002%
29	6.799	1788	1791	1795	rVB3	705	559	0.02%	0.003%
30	6.828	1795	1800	1805	rBV4	709	840	0.03%	0.004%
31	6.863	1808	1811	1813	rBV2	682	517	0.02%	0.003%
32	6.908	1813	1825	1858	rBV	303632	587114	21.68%	3.076%
33	7.236	1916	1927	1973	rVV	1232455	2181081	80.55%	11.427%
34	7.548	2014	2024	2061	rBV	202872	387821	14.32%	2.032%
35	7.783	2095	2097	2102	rVB4	1347	1088	0.04%	0.006%
36	7.809	2102	2105	2108	rVB3	1160	781	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
 Data File : VV037723.D
 Acq On : 03 Oct 2024 09:39
 Operator : SY/MD
 Sample : P4218-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.969	2151	2155	2159	rVB4	917	811	0.03%	0.004%
38	7.995	2159	2163	2164	rBV4	682	447	0.02%	0.002%
39	8.024	2164	2172	2217	rBV2	292372	672737	24.84%	3.525%
40	8.423	2293	2296	2297	rBV3	891	482	0.02%	0.003%
41	8.468	2305	2310	2314	rBV6	1091	1178	0.04%	0.006%
42	8.664	2368	2371	2373	rBV4	907	530	0.02%	0.003%
43	8.725	2387	2390	2391	rBV2	1066	550	0.02%	0.003%
44	8.780	2396	2407	2433	rBV	1120653	1871011	69.10%	9.803%
45	9.227	2544	2546	2550	rVB2	1069	751	0.03%	0.004%
46	9.252	2550	2554	2557	rBV4	1103	917	0.03%	0.005%
47	9.317	2571	2574	2579	rVB4	684	456	0.02%	0.002%
48	9.362	2584	2588	2590	rBV3	716	670	0.02%	0.004%
49	9.432	2608	2610	2615	rVB4	707	481	0.02%	0.003%
50	9.493	2626	2629	2632	rBV4	873	631	0.02%	0.003%
51	9.535	2636	2642	2645	rBV2	633	729	0.03%	0.004%
52	9.728	2700	2702	2706	rBV4	767	591	0.02%	0.003%
53	9.850	2736	2740	2743	rBV4	641	516	0.02%	0.003%
54	9.899	2752	2755	2761	rVB3	1138	1040	0.04%	0.005%
55	9.940	2761	2768	2771	rBV4	560	647	0.02%	0.003%
56	9.966	2773	2776	2779	rBV3	793	502	0.02%	0.003%
57	10.146	2818	2832	2859	rBV	654795	1036772	38.29%	5.432%
58	10.500	2935	2942	2945	rVV5	678	750	0.03%	0.004%
59	10.532	2949	2952	2956	rVB5	856	582	0.02%	0.003%
60	10.564	2956	2962	2964	rBV5	547	495	0.02%	0.003%
61	10.648	2983	2988	2989	rBV3	685	607	0.02%	0.003%
62	10.744	3014	3018	3021	rVB2	616	429	0.02%	0.002%
63	10.767	3021	3025	3027	rBV3	807	541	0.02%	0.003%
64	10.780	3027	3029	3031	rBV	781	490	0.02%	0.003%
65	10.847	3044	3050	3051	rBV4	882	832	0.03%	0.004%
66	10.924	3071	3074	3077	rVB3	881	475	0.02%	0.002%
67	11.011	3099	3101	3104	rVB2	697	437	0.02%	0.002%
68	11.059	3110	3116	3120	rBV5	669	707	0.03%	0.004%
69	11.130	3132	3138	3141	rBV5	1535	1670	0.06%	0.009%
70	11.178	3142	3153	3186	rBV	1069902	1727297	63.79%	9.050%
71	11.551	3257	3269	3303	rBV	1188308	1904308	70.33%	9.977%
72	11.924	3382	3385	3387	rVV4	870	553	0.02%	0.003%
73	11.972	3398	3400	3403	rVB3	901	442	0.02%	0.002%
74	12.024	3413	3416	3419	rBV3	733	455	0.02%	0.002%
75	12.062	3423	3428	3434	rVB5	1129	1446	0.05%	0.008%
76	12.140	3449	3452	3454	rVB2	851	512	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
 Data File : VV037723.D
 Acq On : 03 Oct 2024 09:39
 Operator : SY/MD
 Sample : P4218-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.162	3456	3459	3461	rBV2	893	523	0.02%	0.003%
78	12.268	3487	3492	3495	rBV4	794	588	0.02%	0.003%
79	12.323	3503	3509	3510	rBV4	587	450	0.02%	0.002%
80	12.403	3528	3534	3535	rBV2	722	643	0.02%	0.003%
81	12.497	3559	3563	3567	rBV4	735	582	0.02%	0.003%
82	12.583	3587	3590	3591	rBV2	923	545	0.02%	0.003%
83	12.593	3591	3593	3601	rVB4	1245	1341	0.05%	0.007%
84	12.657	3610	3613	3617	rBV2	746	546	0.02%	0.003%
85	12.686	3617	3622	3623	rBV	478	422	0.02%	0.002%
86	12.767	3644	3647	3651	rVB2	602	414	0.02%	0.002%
87	12.834	3665	3668	3671	rVB2	809	510	0.02%	0.003%
88	12.889	3682	3685	3689	rBV4	691	681	0.03%	0.004%
89	13.078	3739	3744	3746	rBV3	788	667	0.02%	0.003%
90	13.242	3793	3795	3798	rVB4	1052	575	0.02%	0.003%
91	13.451	3854	3860	3873	rBV7	3576	7023	0.26%	0.037%
92	13.683	3927	3932	3933	rBV4	2450	2170	0.08%	0.011%
93	13.850	3981	3984	3986	rBV3	673	441	0.02%	0.002%
94	13.937	4008	4011	4013	rBV2	867	446	0.02%	0.002%
95	14.143	4071	4075	4077	rVB3	601	420	0.02%	0.002%
96	14.361	4141	4143	4148	rVB3	931	615	0.02%	0.003%
97	14.403	4151	4156	4159	rBV4	1404	1289	0.05%	0.007%
98	14.551	4198	4202	4205	rBV5	817	564	0.02%	0.003%
99	15.532	4503	4507	4511	rBV5	2048	2230	0.08%	0.012%
100	15.660	4544	4547	4551	rBV2	1711	1747	0.06%	0.009%




Sum of corrected areas: 19086824

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
Data File : VV037723.D
Acq On : 03 Oct 2024 09:39
Operator : SY/MD
Sample : P4218-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

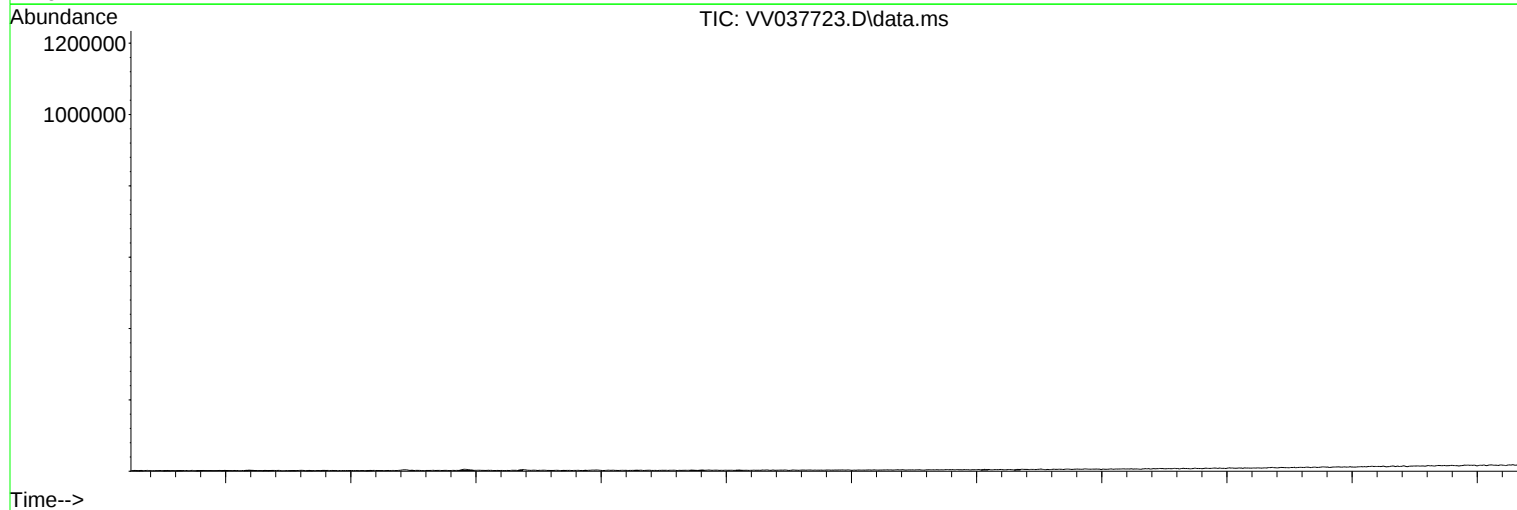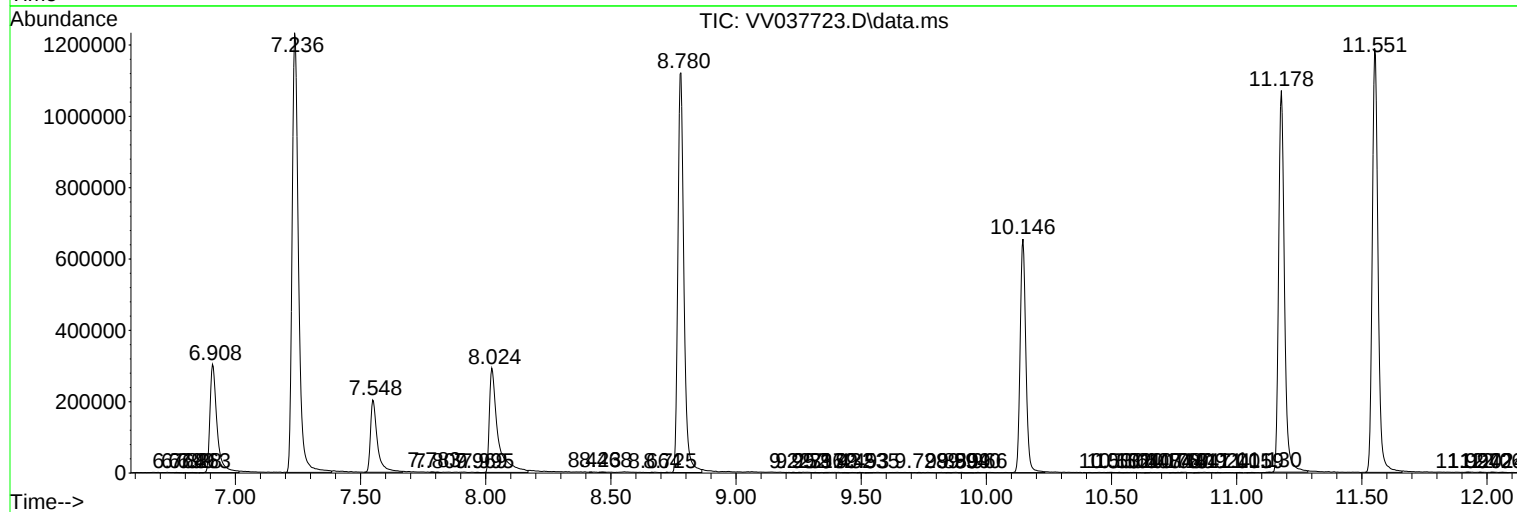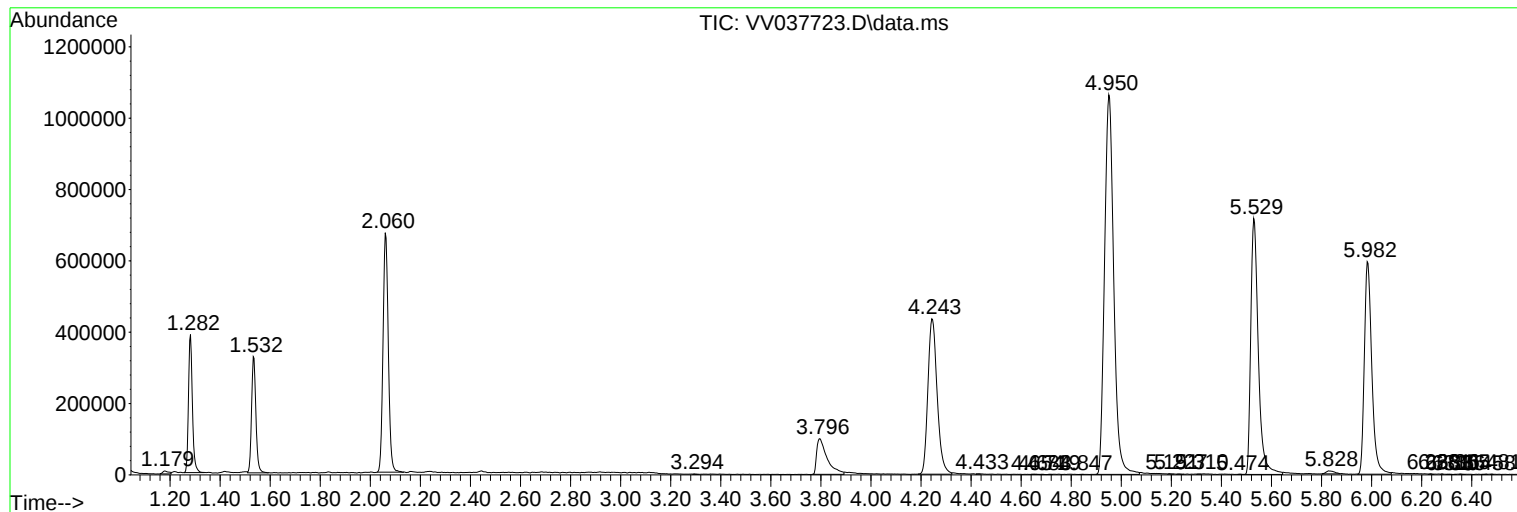

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
Data File : VV037723.D
Acq On : 03 Oct 2024 09:39
Operator : SY/MD
Sample : P4218-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
Data File : VV037723.D
Acq On : 03 Oct 2024 09:39
Operator : SY/MD
Sample : P4218-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------