
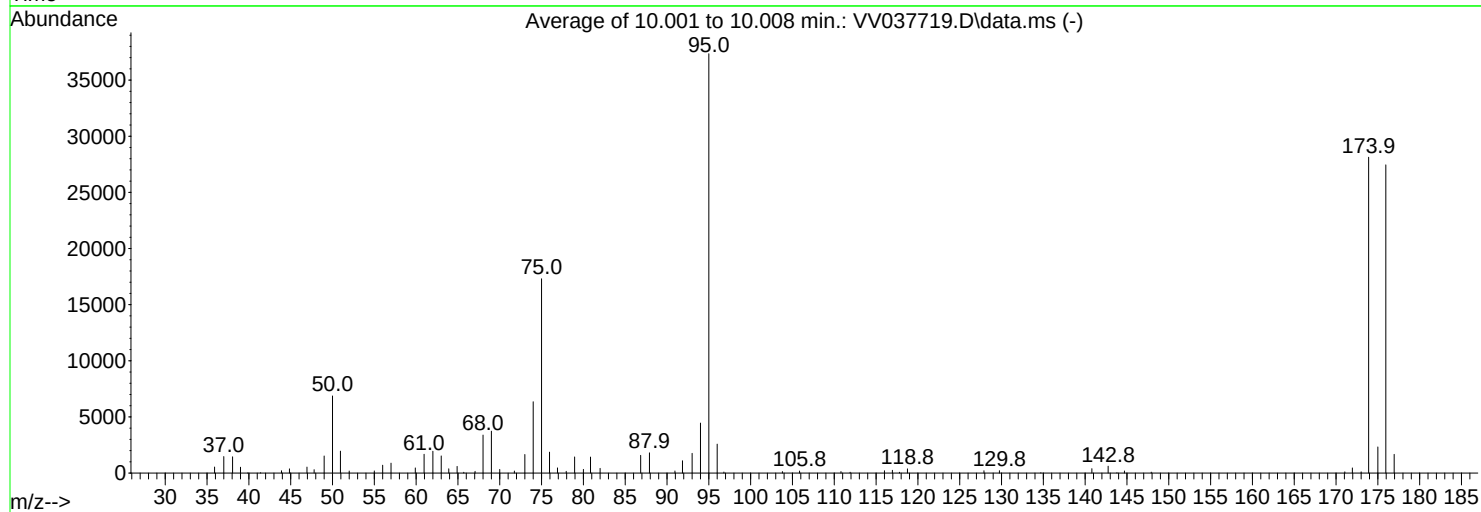


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100324\
Data File : VV037719.D
Acq On : 03 Oct 2024 07:51
Operator : SY/MD
Sample : BFB386
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB386

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Fri Oct 04 02:26:43 2024

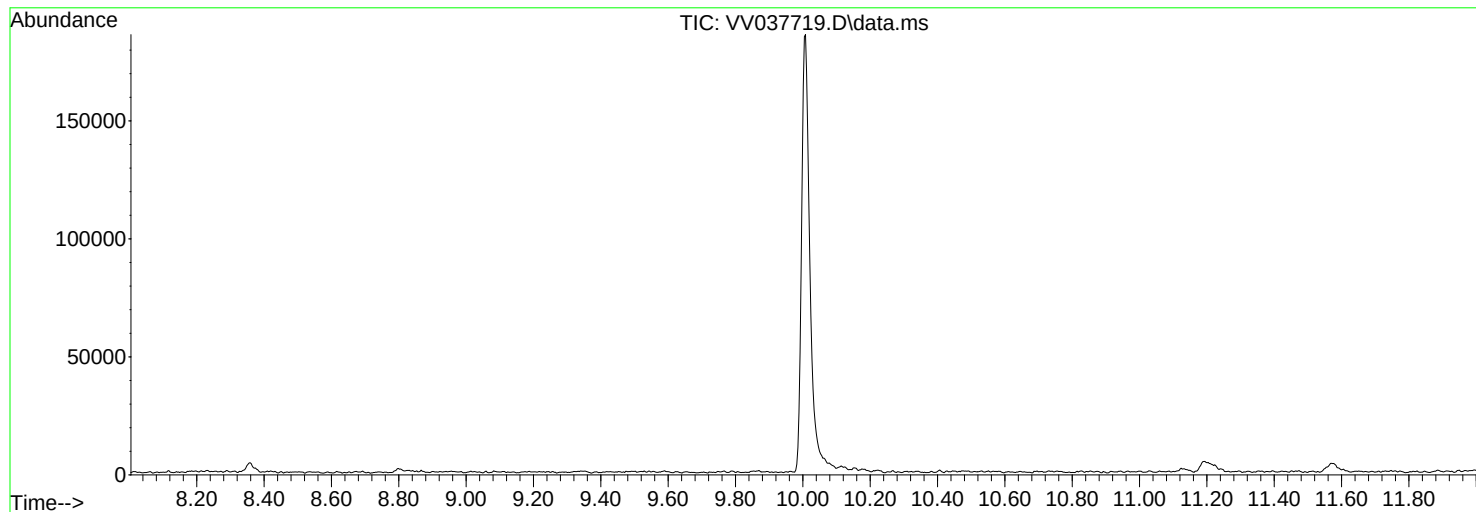

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	6871	PASS
75	95	30	80	46.3	17304	PASS
95	95	100	100	100.0	37349	PASS
96	95	5	9	6.9	2577	PASS
173	174	0.00	2	0.4	113	PASS
174	95	50	120	75.3	28133	PASS
175	174	5	9	8.3	2327	PASS
176	174	95	105	97.6	27451	PASS
177	176	5	10	6.1	1669	PASS

m/z	Abundance
38.30	104.0
39.10	113.0
40.00	323.0
44.00	608.0
77.30	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB386

m/z	Abundance
35.90	545.0
37.00	1407.0
38.10	1244.0
39.00	542.0
39.80	354.0
41.40	111.0
43.90	828.0
44.90	369.0
47.00	564.0
47.80	235.0
49.00	1501.0
50.00	6501.0
51.00	1872.0
52.00	208.0
55.00	180.0
56.00	717.0
57.00	1001.0
59.90	470.0
60.90	1497.0
62.00	1814.0
63.00	1219.0
63.90	386.0
64.90	477.0
65.70	105.0
67.00	149.0
68.00	3289.0
69.00	3481.0
70.00	399.0
71.80	190.0
73.00	1498.0
74.00	5941.0
75.00	16592.0
76.00	1708.0
76.90	423.0
77.90	131.0
79.00	1316.0
80.00	275.0
80.90	1244.0
82.00	394.0
86.80	1314.0
87.90	1633.0
90.90	188.0
91.90	968.0
93.00	1694.0
94.00	4026.0
95.00	34464.0
96.00	2408.0
105.80	175.0
110.80	117.0
116.00	147.0
116.90	198.0
118.80	337.0
127.90	176.0
129.70	204.0
140.80	391.0
142.70	598.0
144.60	194.0
171.10	106.0
171.90	404.0
173.00	339.0
173.90	25184.0
175.00	2190.0
175.90	24696.0
176.90	1514.0

Instrument :
MSVOA_V
ClientSampleId :
BFB386

m/z	Abundance
35.90	595.0
37.00	1538.0
38.00	1520.0
39.00	655.0
39.80	349.0
43.90	843.0
44.90	389.0
47.00	494.0
47.80	318.0
49.00	1567.0
50.00	7141.0
51.00	2036.0
52.00	200.0
55.00	214.0
56.00	744.0
57.00	899.0
59.90	488.0
60.90	1676.0
62.00	2048.0
63.00	1570.0
63.90	399.0
64.90	612.0
65.70	112.0
67.00	169.0
68.00	3445.0
69.00	3904.0
70.00	317.0
71.70	196.0
73.00	1709.0
74.00	6576.0
75.00	17976.0
75.90	1955.0
76.90	490.0
77.90	164.0
78.90	1486.0
80.00	350.0
80.90	1492.0
82.00	445.0
86.90	1620.0
87.90	1904.0
90.90	211.0
91.90	1118.0
93.00	1842.0
94.00	4640.0
95.00	38928.0
96.00	2668.0
96.80	131.0
103.80	172.0
105.90	192.0
110.80	156.0
111.90	117.0
116.00	229.0
116.90	254.0
117.80	104.0
118.70	402.0
127.90	226.0
129.80	235.0
140.80	406.0
142.70	620.0
144.70	201.0
147.90	121.0
171.10	112.0
172.00	481.0
173.90	28920.0
175.00	2420.0
176.00	28464.0
177.00	1744.0

Instrument :
MSVOA_V
ClientSampleId :
BFB386

m/z	Abundance
35.90	474.0
37.00	1471.0
38.00	1581.0
39.00	703.0
39.80	300.0
43.90	782.0
44.80	374.0
46.90	543.0
47.80	356.0
49.00	1496.0
50.00	6971.0
50.90	1949.0
52.00	148.0
55.00	182.0
56.00	645.0
57.00	756.0
59.90	418.0
61.00	1850.0
62.00	1975.0
63.00	1797.0
63.90	354.0
64.90	692.0
67.10	150.0
68.00	3429.0
69.00	3810.0
70.00	256.0
71.70	160.0
73.00	1755.0
74.00	6544.0
75.00	17344.0
75.90	1925.0
76.90	475.0
78.00	188.0
78.90	1514.0
80.00	359.0
80.80	1546.0
82.00	420.0
86.90	1801.0
87.90	1884.0
91.00	175.0
91.80	1216.0
93.00	1737.0
94.00	4695.0
95.00	38656.0
96.00	2655.0
96.80	153.0
103.80	224.0
105.90	190.0
110.80	139.0
111.90	119.0
116.00	247.0
117.00	287.0
117.80	118.0
118.70	394.0
127.90	222.0
129.80	201.0
134.70	104.0
140.80	386.0
142.80	627.0
143.80	105.0
144.80	178.0
147.90	136.0
171.00	114.0
172.00	488.0
173.90	30296.0
175.00	2370.0
176.00	29192.0
177.00	1748.0

Instrument :
MSVOA_V
ClientSampleId :
BFB386