

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100325\
 Data File : VV039243.D
 Acq On : 03 Oct 2025 11:04
 Operator : SY/MD
 Sample : VV1003MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VV1003MBL01

Quant Time: Oct 04 01:07:34 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 24 08:08:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	4.600	168	467975	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	5.532	114	930371	50.000	ug/l	0.00
63) Chlorobenzene-d5	8.773	117	902501	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.172	152	400925	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	4.940	65	401214	59.237	ug/l	0.00
Spiked Amount 50.000	Range 81 - 118		Recovery = 118.480%#			
35) Dibromofluoromethane	4.500	113	358319	47.907	ug/l	0.00
Spiked Amount 50.000	Range 80 - 119		Recovery = 95.820%			
50) Toluene-d8	7.236	98	1125382	51.230	ug/l	0.00
Spiked Amount 50.000	Range 89 - 112		Recovery = 102.460%			
62) 4-Bromofluorobenzene	10.001	95	358770	39.673	ug/l	0.00
Spiked Amount 50.000	Range 85 - 114		Recovery = 79.340%#			
Target Compounds			Qvalue			
5) Bromomethane	1.506	94	1838	0.342	ug/l #	65
6) Chloroethane	1.564	64	335	Below Cal	#	44
10) Methyl Iodide	2.207	142	3920	0.561	ug/l	90
11) Tert butyl alcohol	2.574	59	1277	0.892	ug/l	95
13) Acrolein	2.014	56	79	0.318	ug/l #	1
15) Acrylonitrile	2.686	53	1377	0.300	ug/l #	23
16) Acetone	2.133	43	3869	Below Cal		90
17) Carbon Disulfide	2.256	76	10633	0.493	ug/l #	93
20) Methylene Chloride	2.455	84	2745	Below Cal	#	92
31) Cyclohexane	4.590	56	10545	0.873	ug/l #	1
36) 1,1-Dichloropropene	4.603	75	36983	3.270	ug/l #	50
38) Carbon Tetrachloride	4.600	117	48161	3.485	ug/l #	17
41) Methacrylonitrile	4.156	41	151	1.934	ug/l #	1
49) 1,4-Dioxane	6.355	88	145	1.059	ug/l #	1
58) 2-Chloroethyl Vinyl ether	6.741	63	71	9.633	ug/l #	47
59) 2-Hexanone	8.259	43	198	2.345	ug/l	83
70) Styrene	9.529	104	279	1.571	ug/l #	33
76) 1,2,3-Trichloropropane	10.001	75	175312	19.205	ug/l #	54
79) 2-Chlorotoluene	10.361	91	4537	0.214	ug/l	88
81) trans-1,4-Dichloro-2-b...	10.001	75	175312	46.105	ug/l #	13
82) 4-Chlorotoluene	10.490	91	4935	0.201	ug/l	88
87) 1,3-Dichlorobenzene	11.127	146	3983	0.261	ug/l	98
88) 1,4-Dichlorobenzene	11.127	146	3983	0.238	ug/l	98
90) Hexachloroethane	11.821	117	1703	0.260	ug/l	98
91) 1,2-Dichlorobenzene	11.586	146	3005	0.211	ug/l	91
92) 1,2-Dibromo-3-Chloropr...	12.374	75	166	Below Cal	#	5
93) 1,2,4-Trichlorobenzene	13.201	180	3584	0.438	ug/l	88
94) Hexachlorobutadiene	13.374	225	1983	0.467	ug/l	82
96) 1,2,3-Trichlorobenzene	13.676	180	3306	0.395	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100325\
Data File : VV039243.D
Acq On : 03 Oct 2025 11:04
Operator : SY/MD
Sample : VV1003MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01

Quant Time: Oct 04 01:07:34 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 24 08:08:08 2025
Response via : Initial Calibration




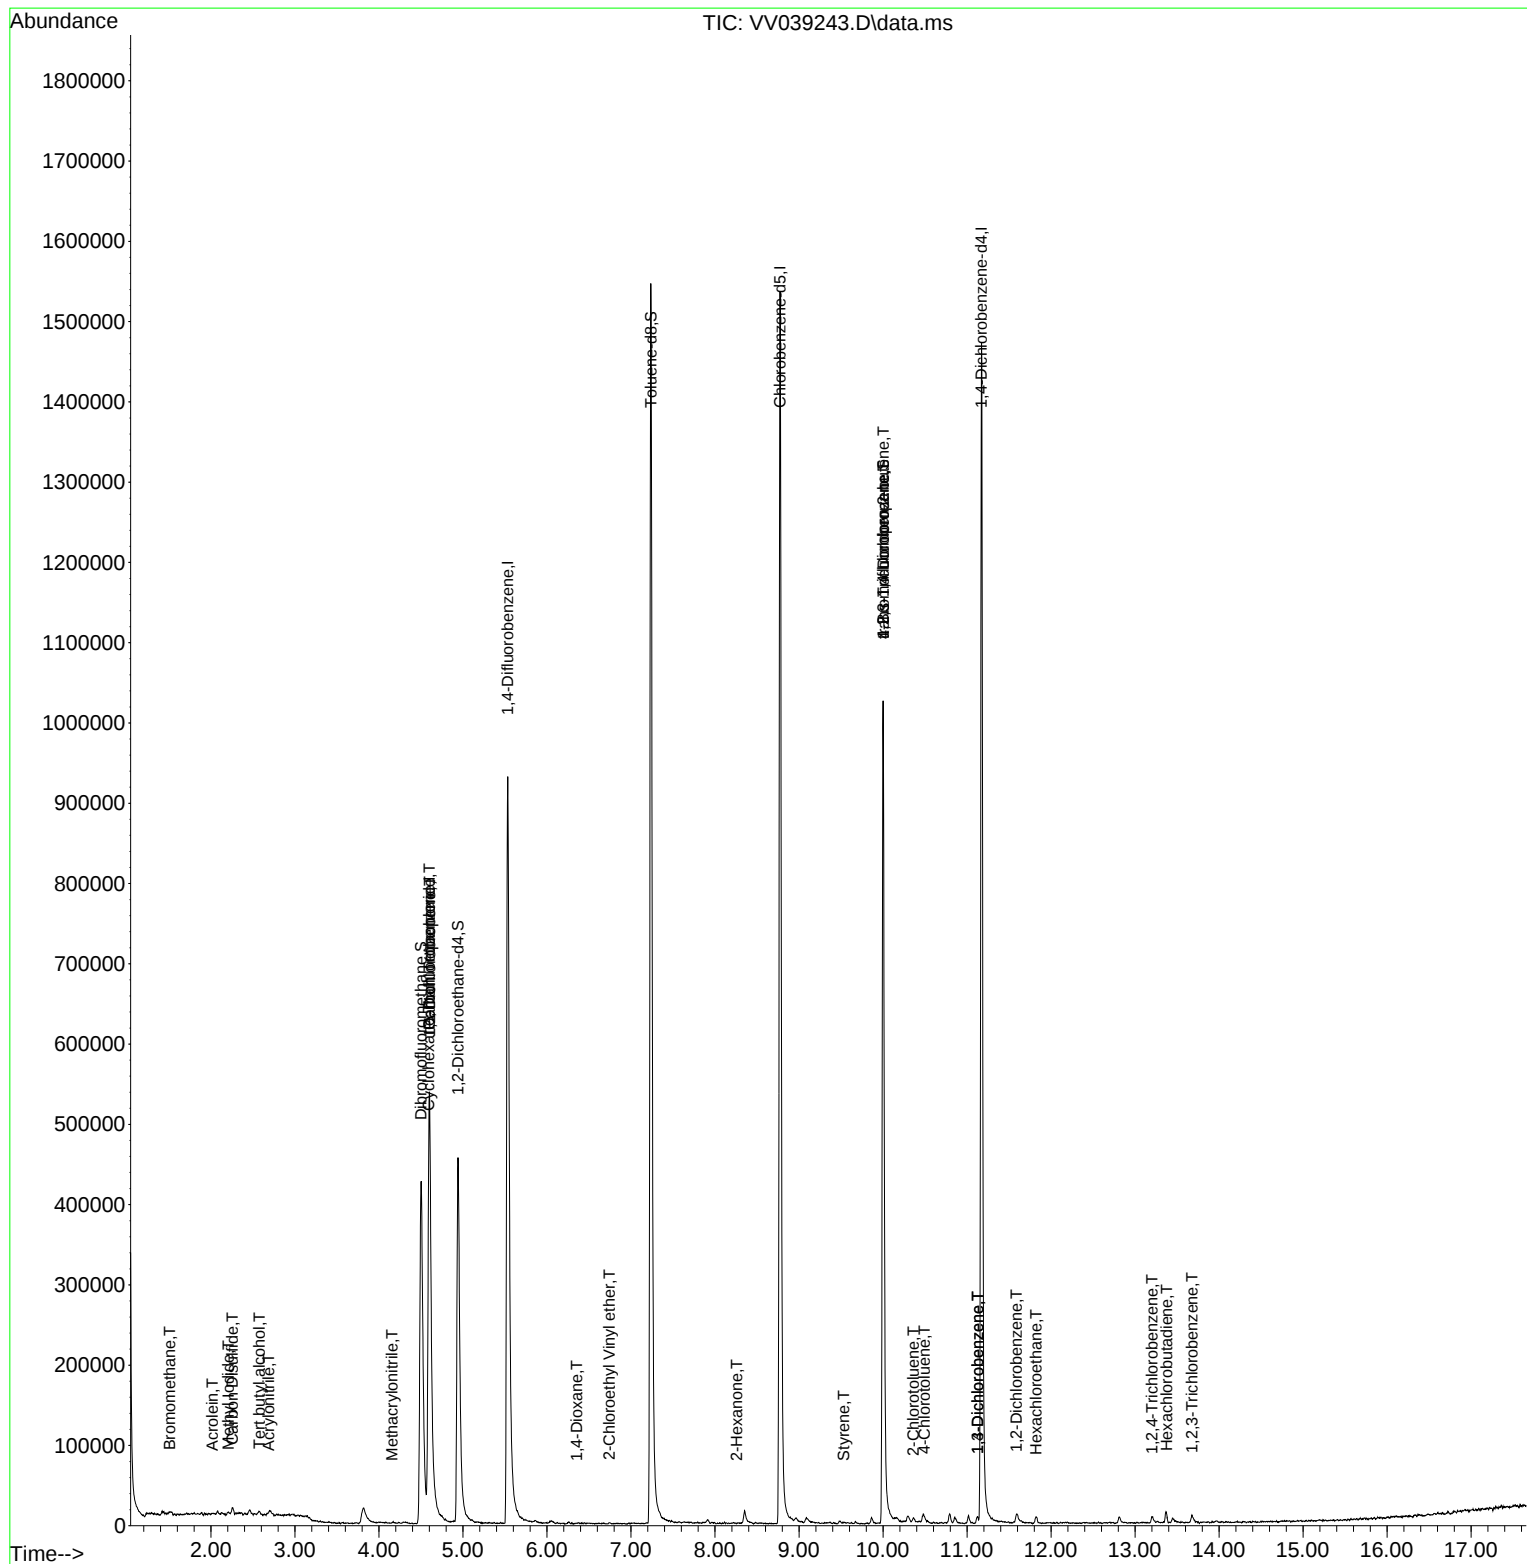


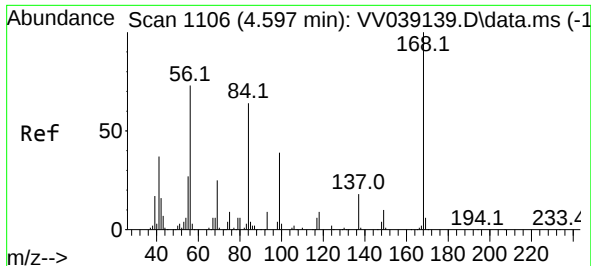

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 4.600 min Scan# 1106
Delta R.T. 0.003 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04




Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01


Tgt Ion:168 Resp: 467975
Ion Ratio Lower Upper
168 100
99 59.7 49.6 74.4



#5
Bromomethane
Concen: 0.342 ug/l
RT: 1.506 min Scan# 145
Delta R.T. 0.012 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04

Tgt Ion: 94 Resp: 1838
Ion Ratio Lower Upper
94 100
96 127.8 74.9 112.3#









#6
Chloroethane
Concen: Below Cal
RT: 1.564 min Scan# 1
Delta R.T. 0.006 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04




Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01


Tgt Ion: 64 Resp: 335
Ion Ratio Lower Upper
64 100
66 0.0 24.6 36.8#

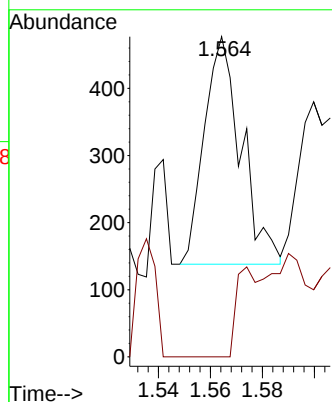

#10
Methyl Iodide
Concen: 0.561 ug/l
RT: 2.207 min Scan# 363
Delta R.T. 0.013 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04

Tgt Ion: 142 Resp: 3920
Ion Ratio Lower Upper
142 100
127 53.1 36.3 54.5
141 12.6 11.2 16.8


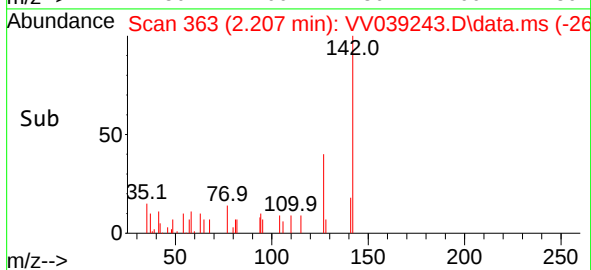






#11
Tert butyl alcohol
Concen: 0.892 ug/l
RT: 2.574 min Scan# 41
Delta R.T. 0.009 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04




Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01


Tgt Ion: 59 Resp: 1277
Ion Ratio Lower Upper
59 100
57 11.7 7.8 11.8

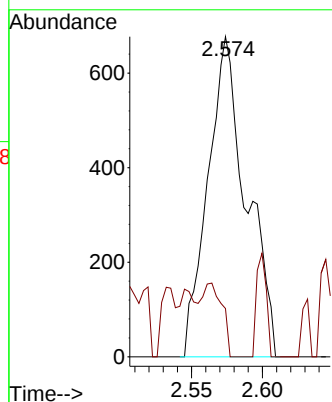

#13
Acrolein
Concen: 0.318 ug/l
RT: 2.014 min Scan# 303
Delta R.T. 0.006 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04

Tgt Ion: 56 Resp: 79
Ion Ratio Lower Upper
56 100
55 220.3 56.2 84.4#


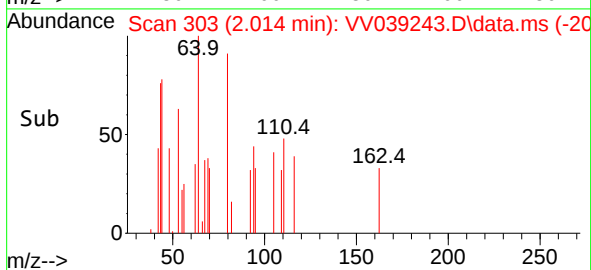
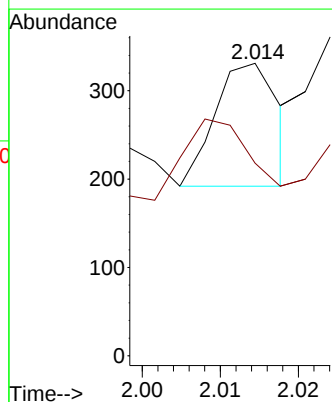





#15
Acrylonitrile
Concen: 0.300 ug/l
RT: 2.686 min Scan# 51
Delta R.T. 0.016 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04




Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01


Tgt Ion: 53 Resp: 1377
Ion Ratio Lower Upper
53 100
52 177.1 66.1 99.1#
51 28.4 28.5 42.7#

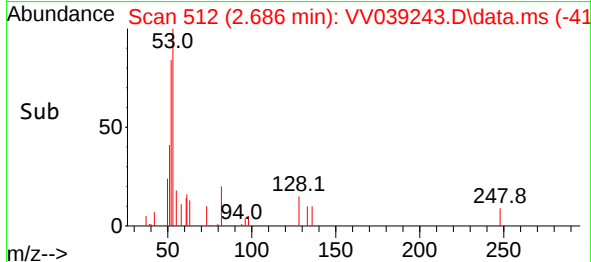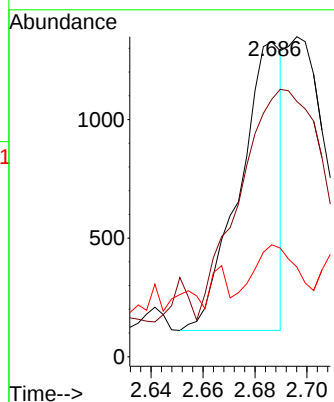

#16
Acetone
Concen: Below Cal
RT: 2.133 min Scan# 340
Delta R.T. 0.015 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04

Tgt Ion: 43 Resp: 3869
Ion Ratio Lower Upper
43 100
58 26.8 25.8 38.6



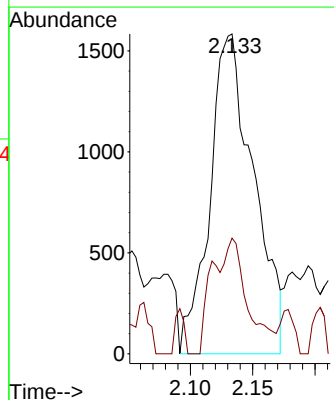
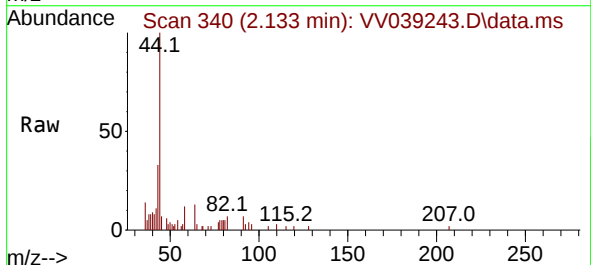




#17
Carbon Disulfide
Concen: 0.493 ug/l
RT: 2.256 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04




Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01


Tgt Ion: 76 Resp: 10633
Ion Ratio Lower Upper
76 100
78 6.6 7.4 11.0#



#20
Methylene Chloride
Concen: Below Cal
RT: 2.455 min Scan# 440
Delta R.T. -0.000 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04

Tgt Ion: 84 Resp: 2745
Ion Ratio Lower Upper
84 100
49 137.8 102.8 154.2
51 26.0 31.9 47.9#
86 64.4 51.2 76.8

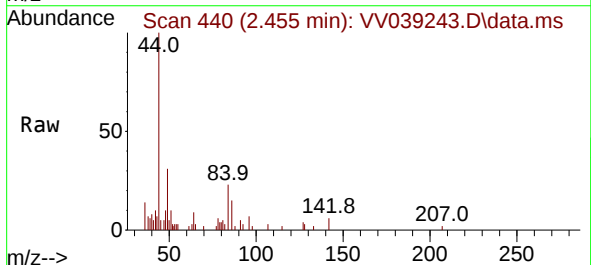

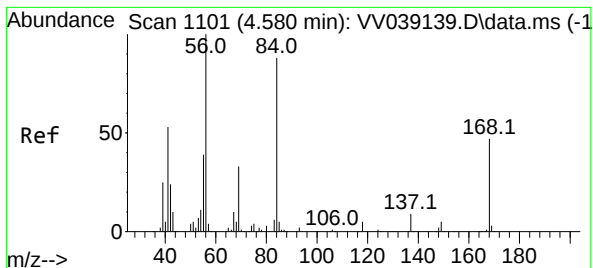

#31

Cyclohexane

Concen: 0.873 ug/l

RT: 4.590 min Scan# 1104

Delta R.T. 0.009 min

Lab File: VV039243.D

Acq: 03 Oct 2025 11:04

Instrument :

MSVOA_V

ClientSampleId :

VV1003MBL01





Tgt Ion: 56 Resp: 10545

Ion Ratio Lower Upper

56 100

69 196.3 26.2 39.2#

84 120.3 70.3 105.5#

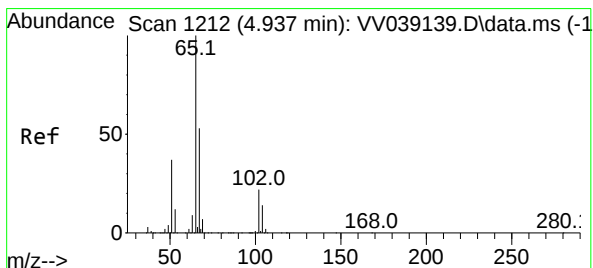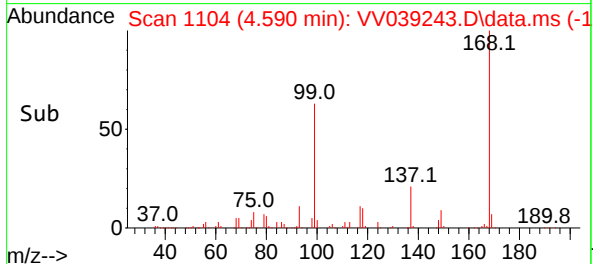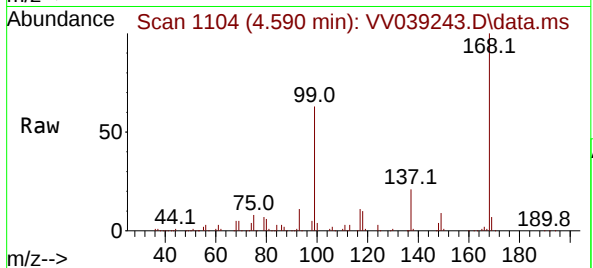

#33

1,2-Dichloroethane-d4

Concen: 59.237 ug/l

RT: 4.940 min Scan# 1213

Delta R.T. 0.003 min

Lab File: VV039243.D




Acq: 03 Oct 2025 11:04


Tgt Ion: 65 Resp: 401214

Ion Ratio Lower Upper

65 100

67 53.4 0.0 107.0


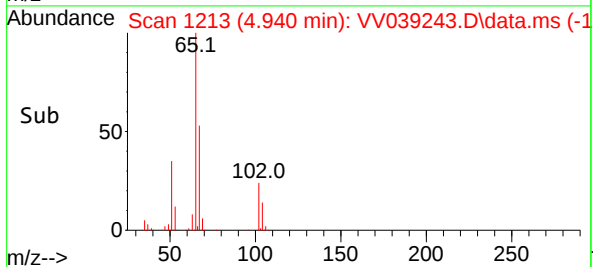

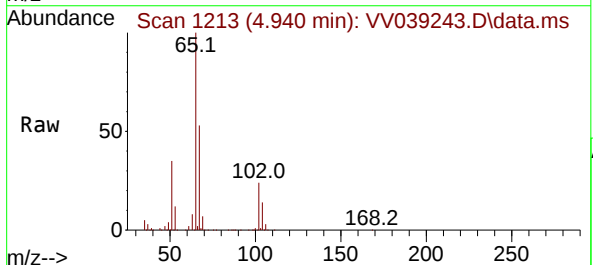




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 5.532 min Scan# 11
Delta R.T. 0.003 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04




Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01


Tgt Ion:	114	Resp:	930371
Ion	Ratio	Lower	Upper
114	100		
63	19.6	0.0	42.6
88	15.9	0.0	30.8

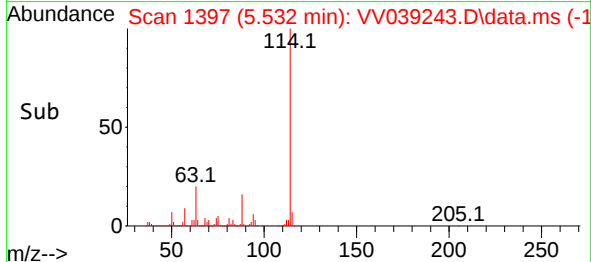

#35
Dibromofluoromethane
Concen: 47.907 ug/l
RT: 4.500 min Scan# 1076
Delta R.T. 0.003 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04

Tgt Ion:	113	Resp:	358319
Ion	Ratio	Lower	Upper
113	100		
111	103.9	82.4	123.6
192	18.7	13.8	20.8

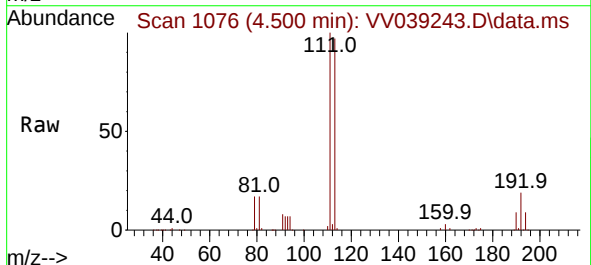



#36

1,1-Dichloropropene

Concen: 3.270 ug/l

RT: 4.603 min Scan# 1108

Delta R.T. -0.138 min

Lab File: VV039243.D

Acq: 03 Oct 2025 11:04

Instrument :

MSVOA_V

ClientSampleId :

VV1003MBL01





Tgt Ion: 75 Resp: 36983

Ion Ratio Lower Upper

75 100

110 9.1 18.1 54.1#

77 0.9 24.8 37.2#

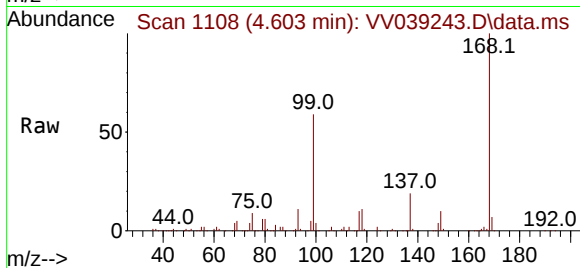

#38

Carbon Tetrachloride

Concen: 3.485 ug/l

RT: 4.600 min Scan# 1107

Delta R.T. -0.132 min

Lab File: VV039243.D

Acq: 03 Oct 2025 11:04




Tgt Ion: 117 Resp: 48161


Ion Ratio Lower Upper

117 100

119 7.4 77.2 115.8#

121 0.0 24.2 36.2#




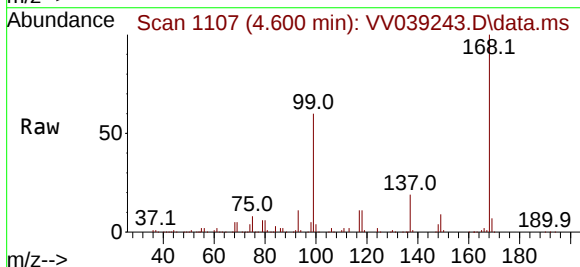




#41
Methacrylonitrile
Concen: 1.934 ug/l
RT: 4.156 min Scan# 968
Delta R.T. 0.003 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04




Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01


Tgt Ion: 41	Resp: 151
Ion Ratio	Lower Upper
41	100
39	270.9 42.2 63.2#
67	0.0 67.9 101.9#
52	53.0 26.7 40.1#

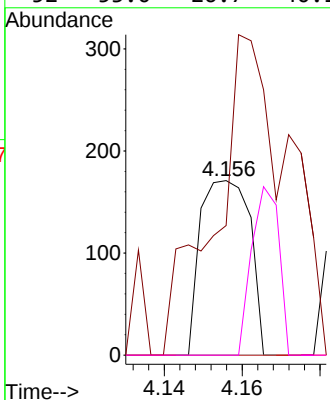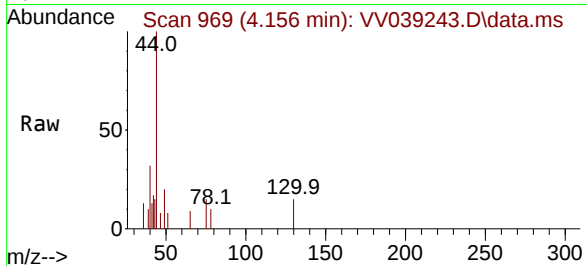

#49
1,4-Dioxane
Concen: 1.059 ug/l
RT: 6.355 min Scan# 1653
Delta R.T. 0.067 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04

Tgt Ion: 88	Resp: 145
Ion Ratio	Lower Upper
88	100
43	145.5 25.1 37.7#
58	0.0 53.6 80.4#



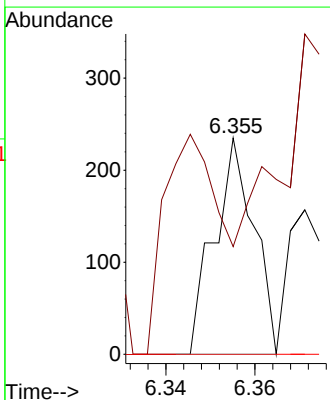
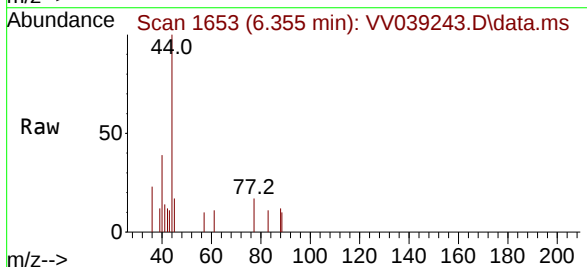




#50
Toluene-d8
Concen: 51.230 ug/l
RT: 7.236 min Scan# 1926
Delta R.T. 0.003 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04




Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01


Tgt Ion: 98 Resp: 1125382
Ion Ratio Lower Upper
98 100
100 64.2 52.2 78.2

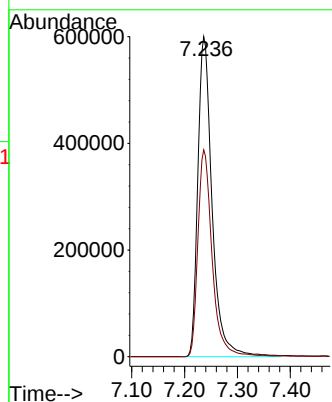

#58
2-Chloroethyl Vinyl ether
Concen: 9.633 ug/l
RT: 6.741 min Scan# 1773
Delta R.T. -0.068 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04

Tgt Ion: 63 Resp: 71
Ion Ratio Lower Upper
63 100
106 0.0 22.1 33.1#

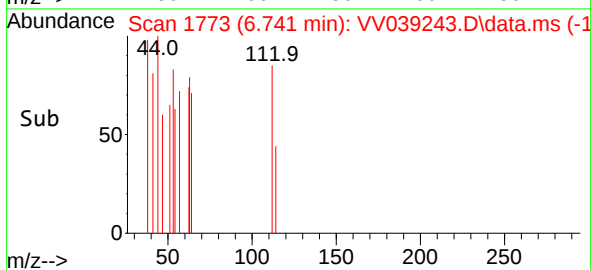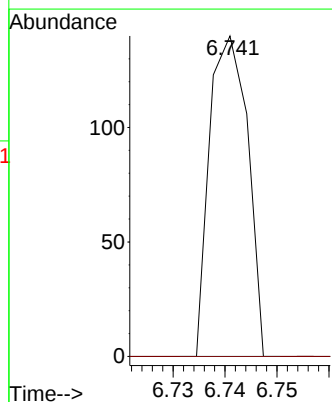



#59

2-Hexanone

Concen: 2.345 ug/l

RT: 8.259 min Scan# 2183

Delta R.T. 0.200 min

Lab File: VV039243.D

Acq: 03 Oct 2025 11:04

Instrument :

MSVOA_V

ClientSampleId :





VV1003MBL01

Tgt Ion: 43 Resp: 198

Ion Ratio Lower Upper

43 100

58 43.9 28.3 85.0

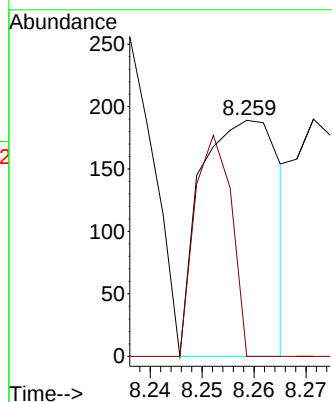

#62

4-Bromofluorobenzene

Concen: 39.673 ug/l

RT: 10.001 min Scan# 2787

Delta R.T. 0.003 min

Lab File: VV039243.D

Acq: 03 Oct 2025 11:04




Tgt Ion: 95 Resp: 358770


Ion Ratio Lower Upper

95 100

174 77.5 0.0 150.4

176 73.9 0.0 144.2









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 8.773 min Scan# 2405
Delta R.T. 0.000 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04




Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01


Tgt Ion:117 Resp: 902501
Ion Ratio Lower Upper
117 100
82 55.5 45.4 68.2
119 31.2 25.6 38.4

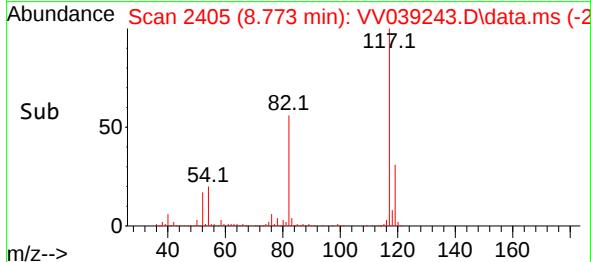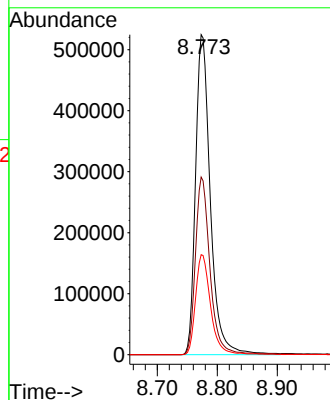

#70
Styrene
Concen: 1.571 ug/l
RT: 9.529 min Scan# 2640
Delta R.T. 0.045 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04

Tgt Ion:104 Resp: 279
Ion Ratio Lower Upper
104 100
78 108.2 39.8 59.6#
103 91.0 43.4 65.2#



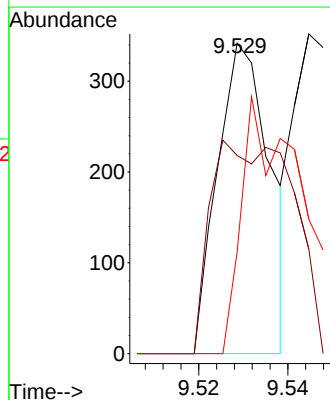



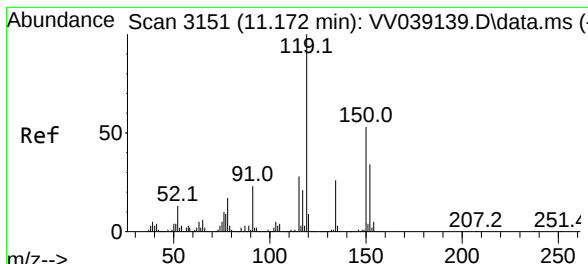

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 11.172 min Scan# 3151
 Delta R.T. -0.000 min
 Lab File: VV039243.D
 Acq: 03 Oct 2025 11:04




Instrument :
 MSVOA_V
 ClientSampleId :
 VV1003MBL01


Tgt Ion:152 Resp: 400925
 Ion Ratio Lower Upper
 152 100
 115 61.9 44.8 134.4
 150 159.1 0.0 353.8

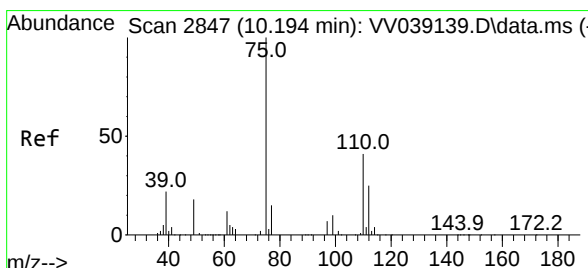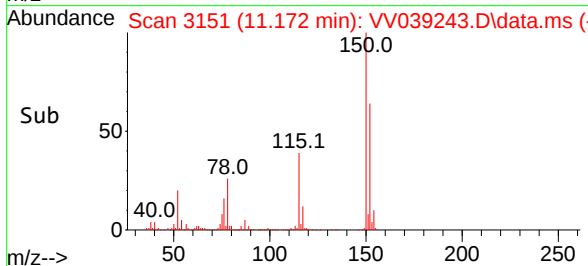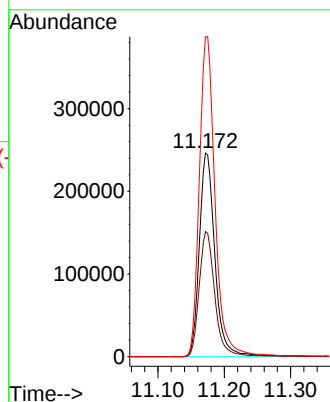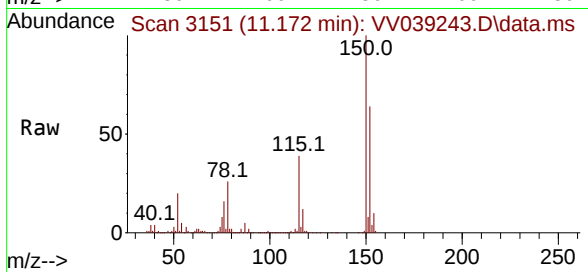

#76
 1,2,3-Trichloropropane
 Concen: 19.205 ug/l
 RT: 10.001 min Scan# 2787
 Delta R.T. -0.193 min
 Lab File: VV039243.D
 Acq: 03 Oct 2025 11:04

Tgt Ion: 75 Resp: 175312
 Ion Ratio Lower Upper
 75 100
 77 0.5 11.3 33.8#


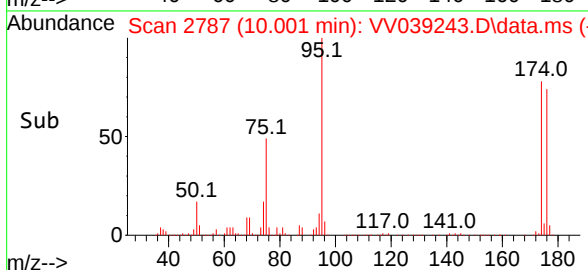
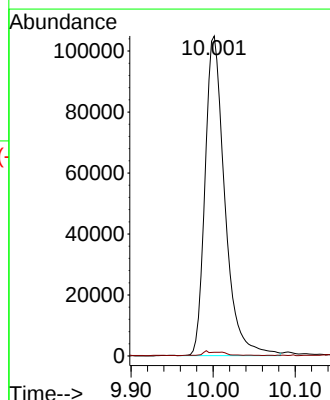
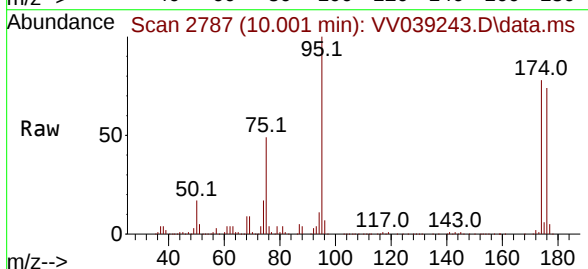




#79
2-Chlorotoluene
Concen: 0.214 ug/l
RT: 10.361 min Scan# 21
Delta R.T. 0.016 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04




Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01


Tgt Ion: 91 Resp: 4537
Ion Ratio Lower Upper
91 100
126 26.5 16.7 50.0

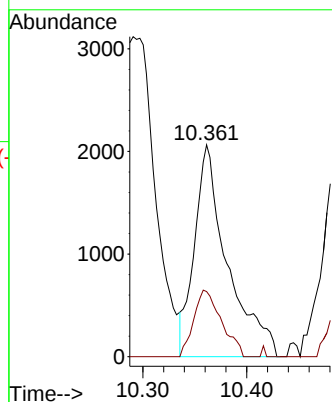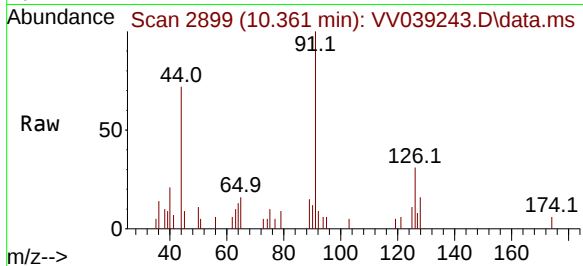

#81
trans-1,4-Dichloro-2-butene
Concen: 46.105 ug/l
RT: 10.001 min Scan# 2787
Delta R.T. 0.074 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04

Tgt Ion: 75 Resp: 175312
Ion Ratio Lower Upper
75 100
53 0.3 72.5 108.7#
89 0.0 37.2 55.8#



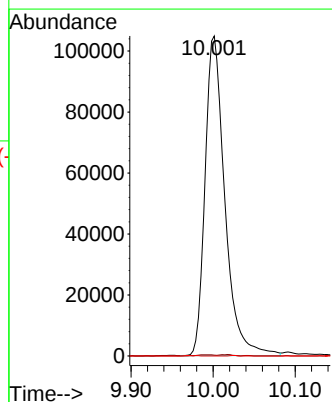
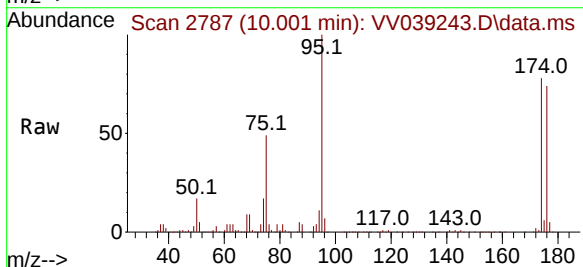




#82
4-Chlorotoluene
Concen: 0.201 ug/l
RT: 10.490 min Scan# 2939
Delta R.T. 0.029 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04




Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01


Tgt Ion: 91 Resp: 4935
Ion Ratio Lower Upper
91 100
126 22.6 14.5 43.6

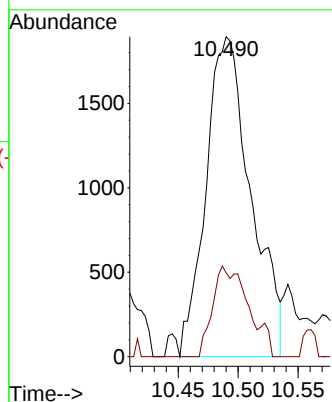

#87
1,3-Dichlorobenzene
Concen: 0.261 ug/l
RT: 11.127 min Scan# 3137
Delta R.T. 0.022 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04

Tgt Ion:146 Resp: 3983
Ion Ratio Lower Upper
146 100
111 39.9 20.9 62.8
148 64.9 31.8 95.3


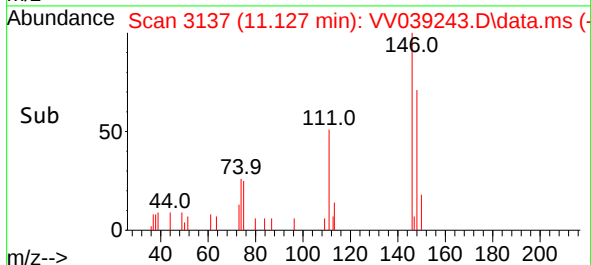






#88
 1,4-Dichlorobenzene
 Concen: 0.238 ug/l
 RT: 11.127 min Scan# 3158
 Delta R.T. -0.068 min
 Lab File: VV039243.D
 Acq: 03 Oct 2025 11:04




Instrument :
 MSVOA_V
 ClientSampleId :
 VV1003MBL01


Tgt Ion:146 Resp: 3983
 Ion Ratio Lower Upper
 146 100
 111 39.9 20.3 60.8
 148 64.9 31.4 94.2

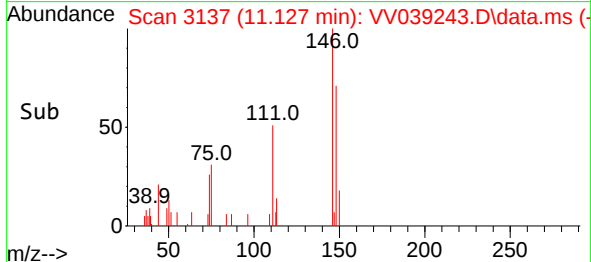

#90
 Hexachloroethane
 Concen: 0.260 ug/l
 RT: 11.821 min Scan# 3353
 Delta R.T. 0.003 min
 Lab File: VV039243.D
 Acq: 03 Oct 2025 11:04

Tgt Ion:117 Resp: 1703
 Ion Ratio Lower Upper
 117 100
 201 63.0 32.3 96.8


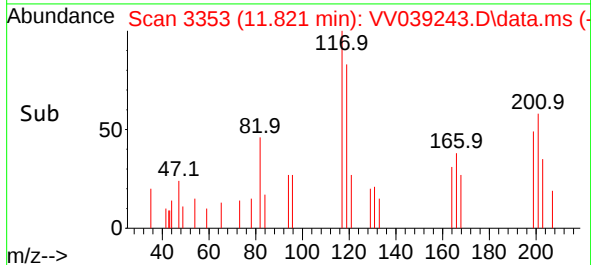






#91
1,2-Dichlorobenzene
Concen: 0.211 ug/l
RT: 11.586 min Scan# 311
Delta R.T. 0.019 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04




Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01


Tgt Ion:	146	Resp:	3005
Ion	Ratio	Lower	Upper
146	100		
111	38.9	21.5	64.5
148	56.0	31.9	95.7

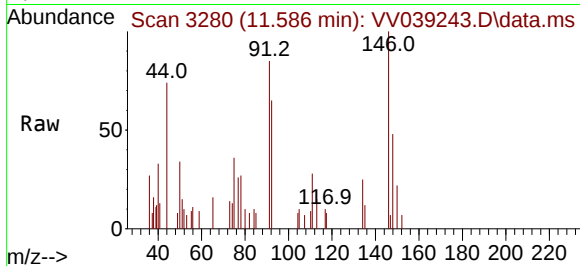

#92
1,2-Dibromo-3-Chloropropane
Concen: Below Cal
RT: 12.374 min Scan# 3525
Delta R.T. 0.025 min
Lab File: VV039243.D
Acq: 03 Oct 2025 11:04

Tgt Ion:	75	Resp:	166
Ion	Ratio	Lower	Upper
75	100		
155	0.0	38.6	115.8#
157	0.0	49.5	148.3#

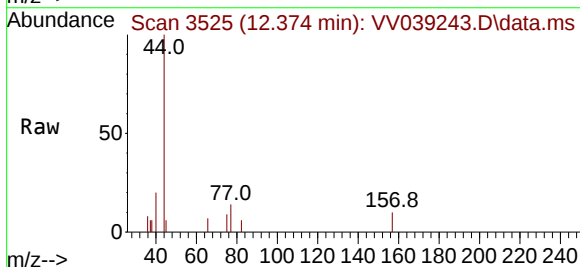



#93

1,2,4-Trichlorobenzene

Concen: 0.438 ug/l

RT: 13.201 min Scan# 3

Delta R.T. 0.015 min

Lab File: VV039243.D

Acq: 03 Oct 2025 11:04

Instrument :

MSVOA_V

ClientSampleId :

VV1003MBL01





Tgt Ion:180 Resp: 3584

Ion Ratio Lower Upper

180 100

182 79.7 47.1 141.4

145 30.4 16.3 48.8

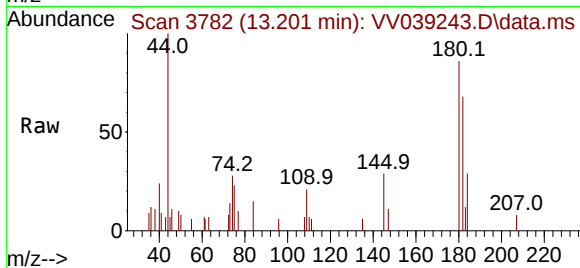

#94

Hexachlorobutadiene

Concen: 0.467 ug/l

RT: 13.374 min Scan# 3836

Delta R.T. 0.006 min

Lab File: VV039243.D

Acq: 03 Oct 2025 11:04




Tgt Ion:225 Resp: 1983


Ion Ratio Lower Upper

225 100

223 73.0 31.6 94.7

227 81.2 31.8 95.4

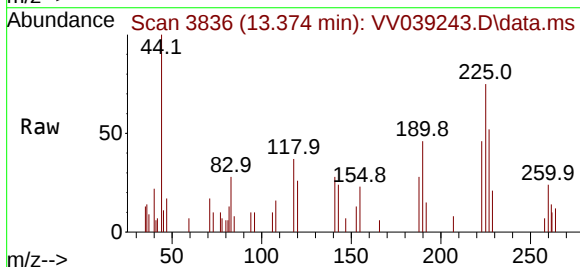

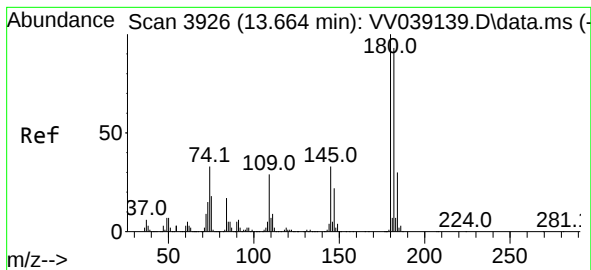

#96
 1,2,3-Trichlorobenzene
 Concen: 0.395 ug/l
 RT: 13.676 min Scan# 3930
 Delta R.T. 0.013 min
 Lab File: VV039243.D
 Acq: 03 Oct 2025 11:04

Instrument :
 MSVOA_V
 ClientSampleId :
 VV1003MBL01

Tgt Ion:180	Resp:	3306
Ion	Ratio	Lower Upper
180	100	
182	96.3	46.9 140.8
145	29.6	17.0 51.0

