

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100325\
Data File : VV039243.D
Acq On : 03 Oct 2025 11:04
Operator : SY/MD
Sample : VV1003MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M

Title : SW846 8260

Signal : TIC: VV039243.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.815	849	863	886	rBV3	18539	67187	2.30%	0.429%
2	4.503	1060	1077	1095	rBV	426644	1120942	38.43%	7.157%
3	4.600	1096	1107	1145	rVB	529497	1437096	49.27%	9.176%
4	4.940	1201	1213	1247	rBV	453952	1109783	38.05%	7.086%
5	5.532	1386	1397	1431	rBV	930091	2153455	73.84%	13.750%
6	7.236	1916	1927	1968	rBV	1544277	2916531	100.00%	18.623%
7	8.352	2263	2274	2285	rBV2	15724	30517	1.05%	0.195%
8	8.773	2395	2405	2440	rBV	1535233	2661546	91.26%	16.994%
9	10.001	2776	2787	2824	rBV	1024359	1742769	59.75%	11.128%
10	11.172	3140	3151	3187	rBV	1466461	2421396	83.02%	15.461%




Sum of corrected areas: 15661222

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100325\
Data File : VV039243.D
Acq On : 03 Oct 2025 11:04
Operator : SY/MD
Sample : VV1003MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

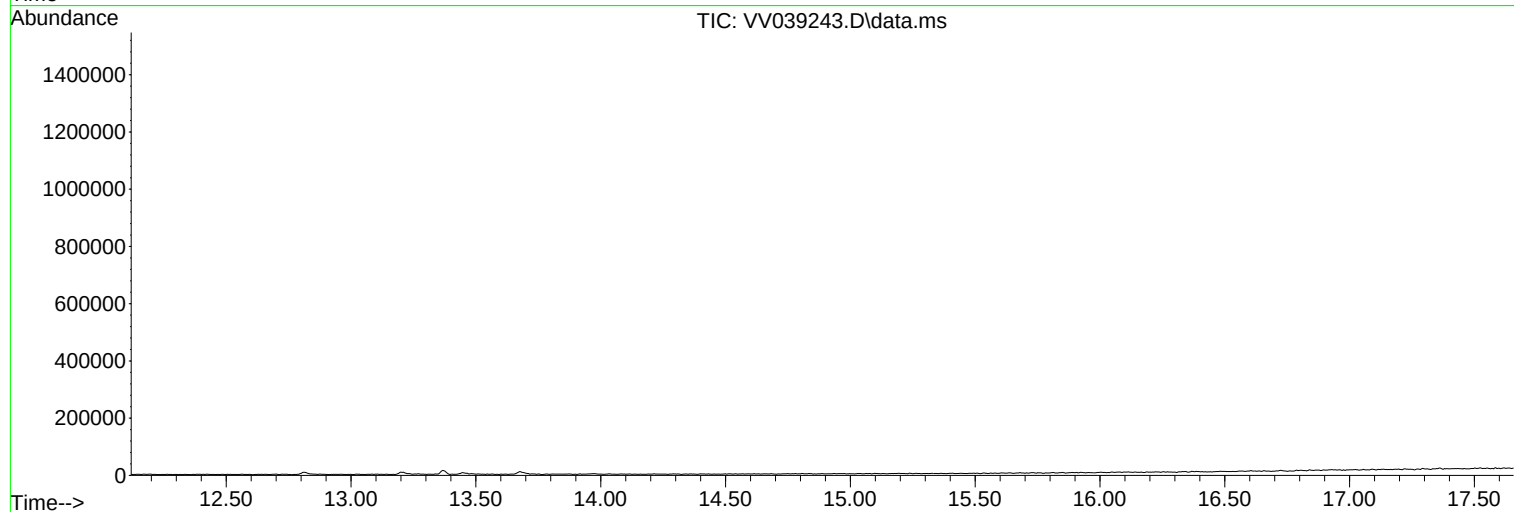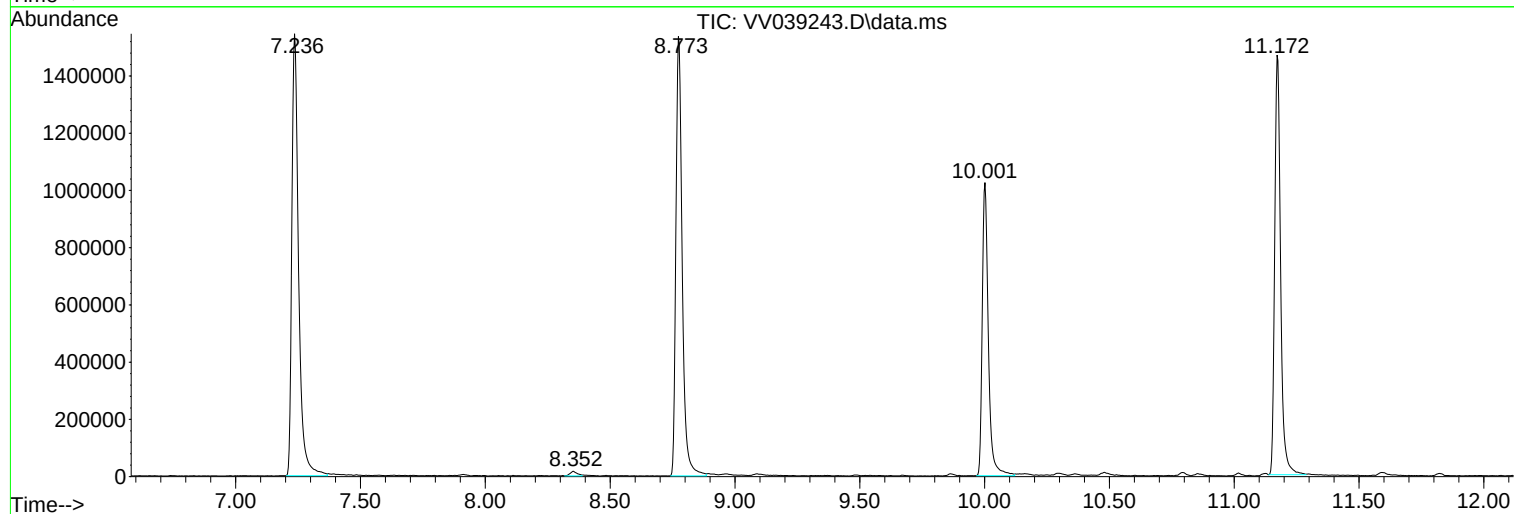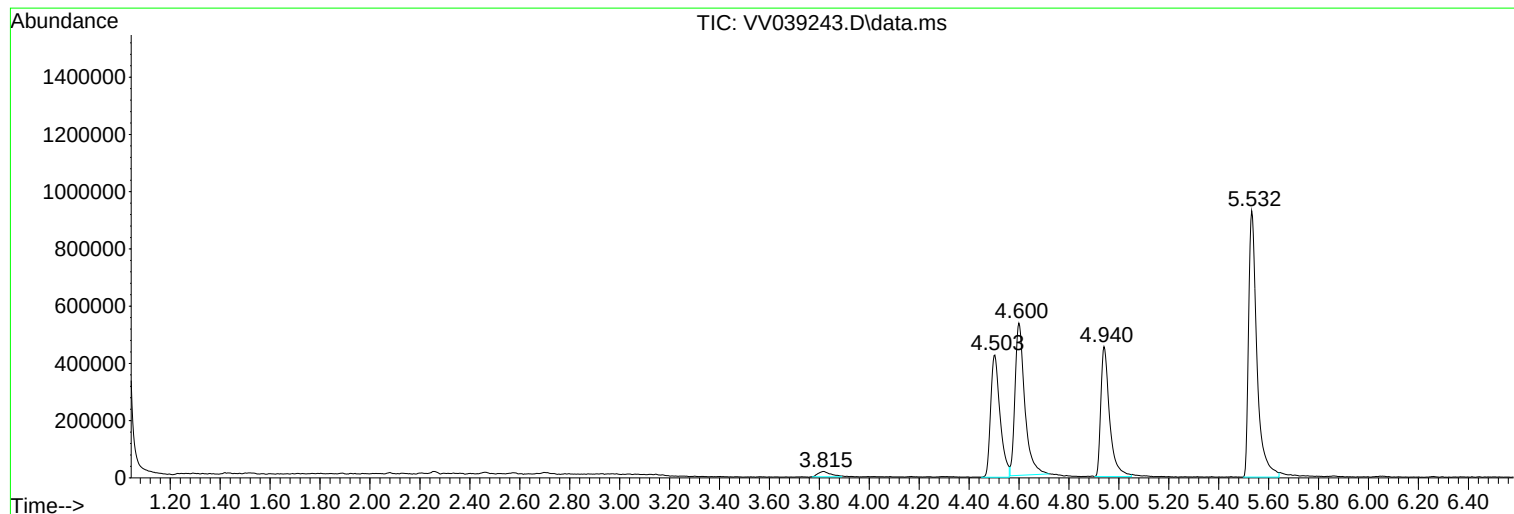

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100325\
Data File : VV039243.D
Acq On : 03 Oct 2025 11:04
Operator : SY/MD
Sample : VV1003MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100325\
Data File : VV039243.D
Acq On : 03 Oct 2025 11:04
Operator : SY/MD
Sample : VV1003MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VV1003MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc