

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV100325\  
Data File : VV039257.D  
Acq On : 03 Oct 2025 18:04  
Operator : SY/MD  
Sample : Q3201-02  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
MW14

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\82V092225W.M

Title : SW846 8260

Signal : TIC: VV039257.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.564       | 453           | 474         | 502          | rBV      | 5054410        | 11985485      | 6.74%           | 6.057%        |
| 2         | 2.712       | 502           | 520         | 618          | rVB3     | 60991347       | 177742157     | 100.00%         | 89.819%       |
| 3         | 5.011       | 1224          | 1235        | 1256         | rVB      | 776315         | 1878241       | 1.06%           | 0.949%        |
| 4         | 7.236       | 1905          | 1927        | 1963         | rBV      | 1064065        | 2052328       | 1.15%           | 1.037%        |
| 5         | 8.776       | 2395          | 2406        | 2443         | rBV      | 1270999        | 2176580       | 1.22%           | 1.100%        |
| 6         | 11.172      | 3139          | 3151        | 3176         | rBV      | 1260423        | 2054734       | 1.16%           | 1.038%        |




Sum of corrected areas: 197889525

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV100325\  
Data File : VV039257.D  
Acq On : 03 Oct 2025 18:04  
Operator : SY/MD  
Sample : Q3201-02  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
MW14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\82V092225W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

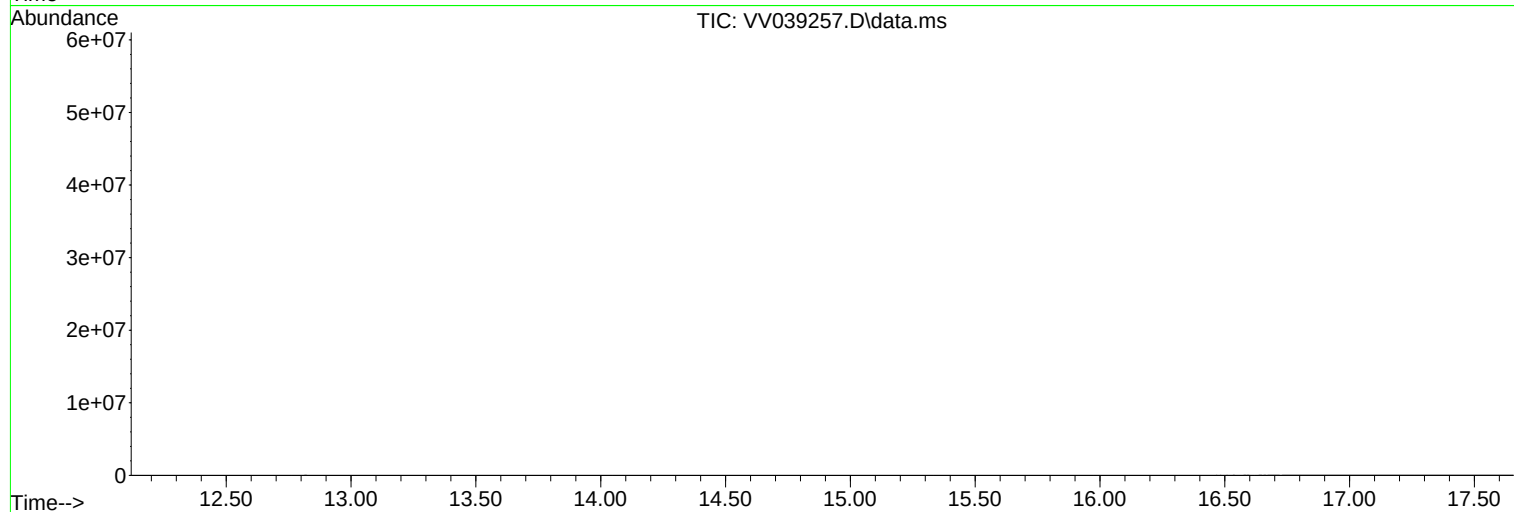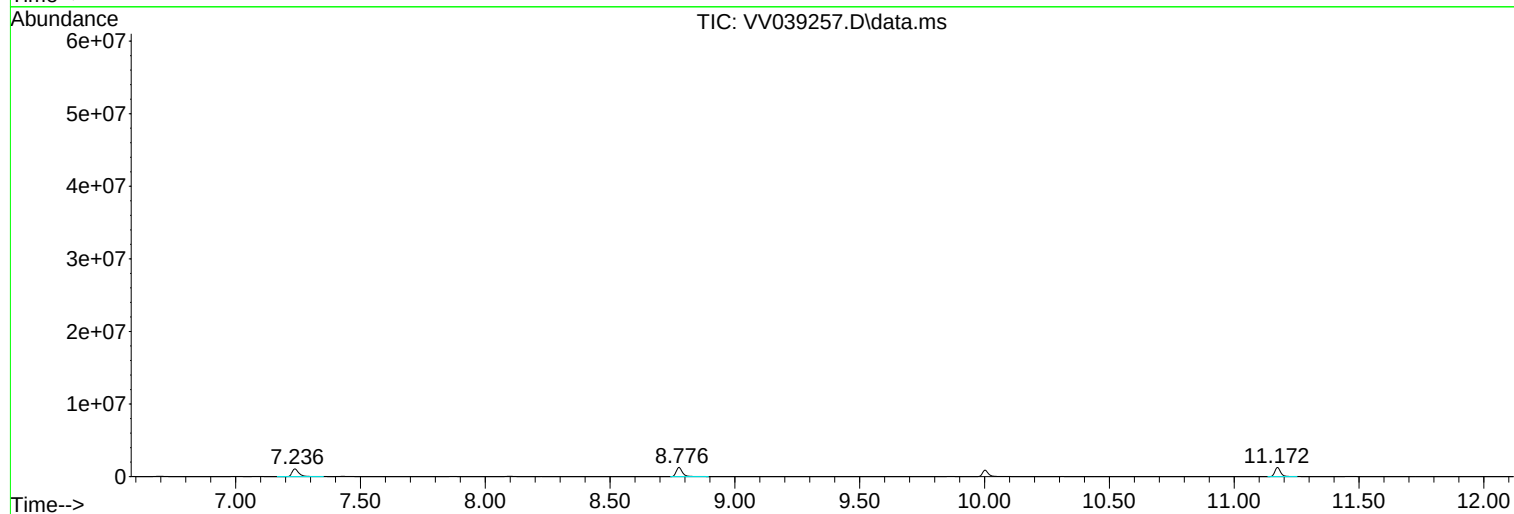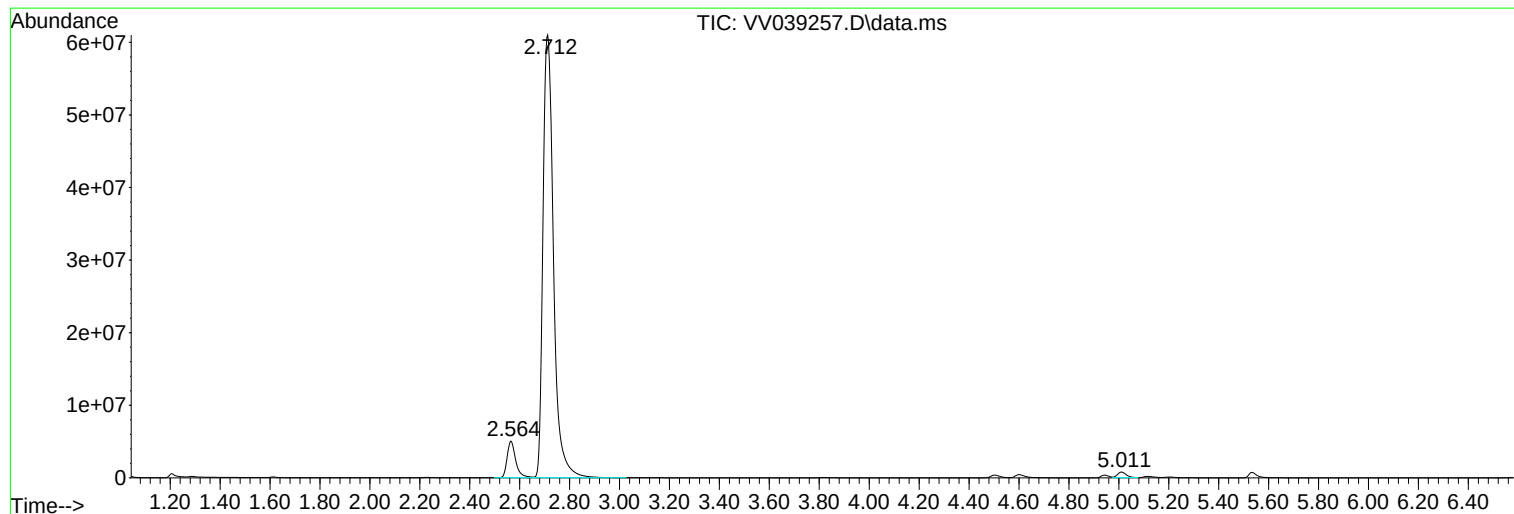

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV100325\  
Data File : VV039257.D  
Acq On : 03 Oct 2025 18:04  
Operator : SY/MD  
Sample : Q3201-02  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
MW14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\82V092225W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV100325\  
Data File : VV039257.D  
Acq On : 03 Oct 2025 18:04  
Operator : SY/MD  
Sample : Q3201-02  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
MW14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\82V092225W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----