

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100325\
 Data File : VV039262.D
 Acq On : 03 Oct 2025 19:56
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M

Title : SW846 8260

Signal : TIC: VV039262.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.423	111	119	126	rBV9	7096	15009	1.07%	0.171%
2	2.458	433	441	452	rBV3	26014	45656	3.25%	0.519%
3	3.815	846	863	884	rBV	79158	257612	18.36%	2.931%
4	4.503	1062	1077	1097	rBV	309550	824491	58.76%	9.380%
5	4.603	1097	1108	1142	rVB	268227	742263	52.90%	8.444%
6	4.944	1201	1214	1248	rBV	330430	846444	60.32%	9.630%
7	5.535	1385	1398	1437	rBV	444842	1061680	75.66%	12.078%
8	7.239	1915	1928	1956	rBV	613764	1212683	86.42%	13.796%
9	8.352	2262	2274	2290	rBV2	61104	124588	8.88%	1.417%
10	8.776	2396	2406	2442	rBV	789779	1403216	100.00%	15.964%
11	10.001	2776	2787	2815	rBV	562370	964772	68.75%	10.976%
12	11.175	3141	3152	3188	rBV	775773	1291530	92.04%	14.693%




Sum of corrected areas: 8789944

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100325\
Data File : VV039262.D
Acq On : 03 Oct 2025 19:56
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

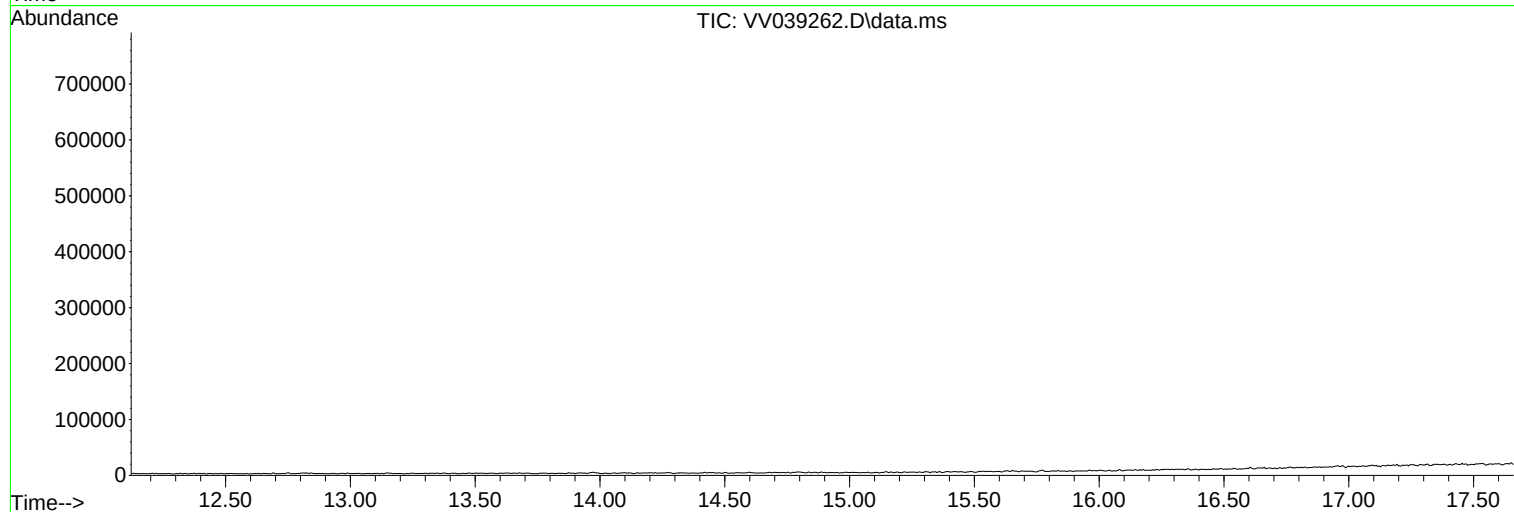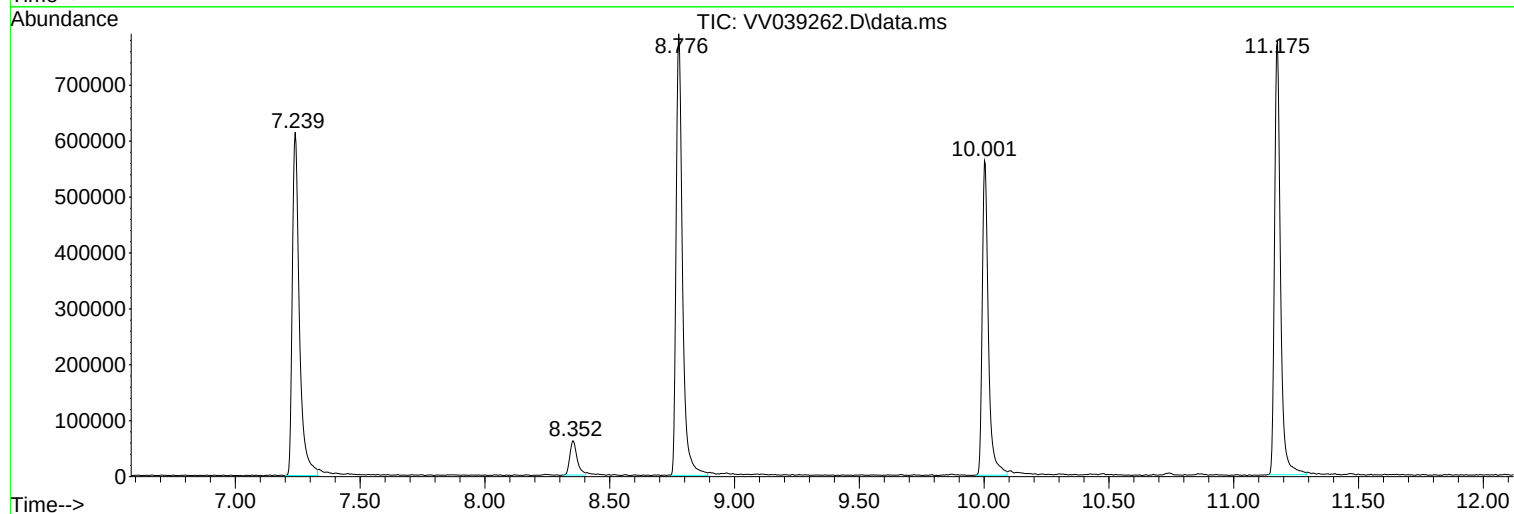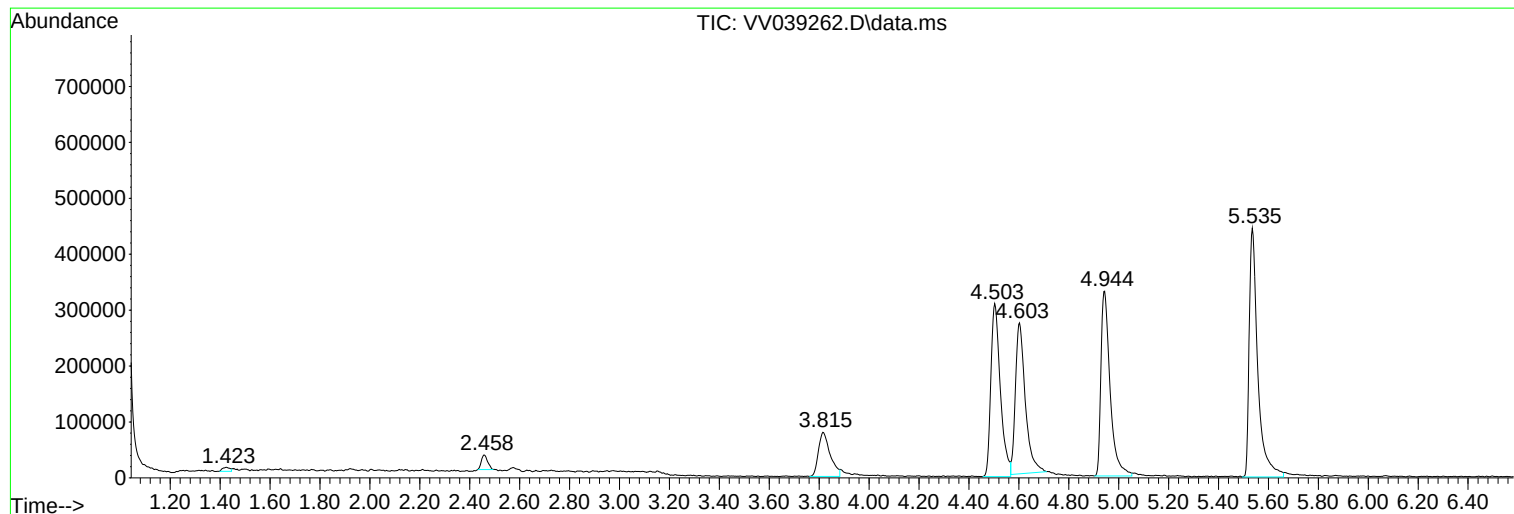

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100325\
Data File : VV039262.D
Acq On : 03 Oct 2025 19:56
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100325\
Data File : VV039262.D
Acq On : 03 Oct 2025 19:56
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc