

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100418\
 Data File : VV008068.D
 Acq On : 04 Oct 2018 18:18
 Operator : SY/MD
 Sample : J5258-04
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESN9

Quant Time: Oct 05 06:24:07 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 05 05:56:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	90158	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	85667	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	42083	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	18396	3.81	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.20%
7) Chloroethane-d5	1.59	69	17533	4.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.00%
11) 1,1-Dichloroethene-d2	2.14	63	30062	2.75	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.00%#
20) 2-Butanone-d5	3.97	46	68916	47.41	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.82%
24) Chloroform-d	4.41	84	48714	4.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.40%
26) 1,2-Dichloroethane-d4	5.09	65	26831	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.60%
32) Benzene-d6	5.10	84	91602	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
36) 1,2-Dichloropropane-d6	6.13	67	30627	4.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.40%
41) Toluene-d8	7.36	98	82912	3.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.60%
43) trans-1,3-Dichloropropene-	7.67	79	10148	4.06	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.20%
46) 2-Hexanone-d5	8.14	63	45303	41.11	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.22%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	21512	4.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	36909	4.53	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.60%


Target Compounds					Qvalue
13) Acetone	2.22	43	7559	7.136 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100418\
Data File : VV008068.D
Acq On : 04 Oct 2018 18:18
Operator : SY/MD
Sample : J5258-04
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESNN9

Quant Time: Oct 05 06:24:07 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 05 05:56:33 2018
Response via : Initial Calibration

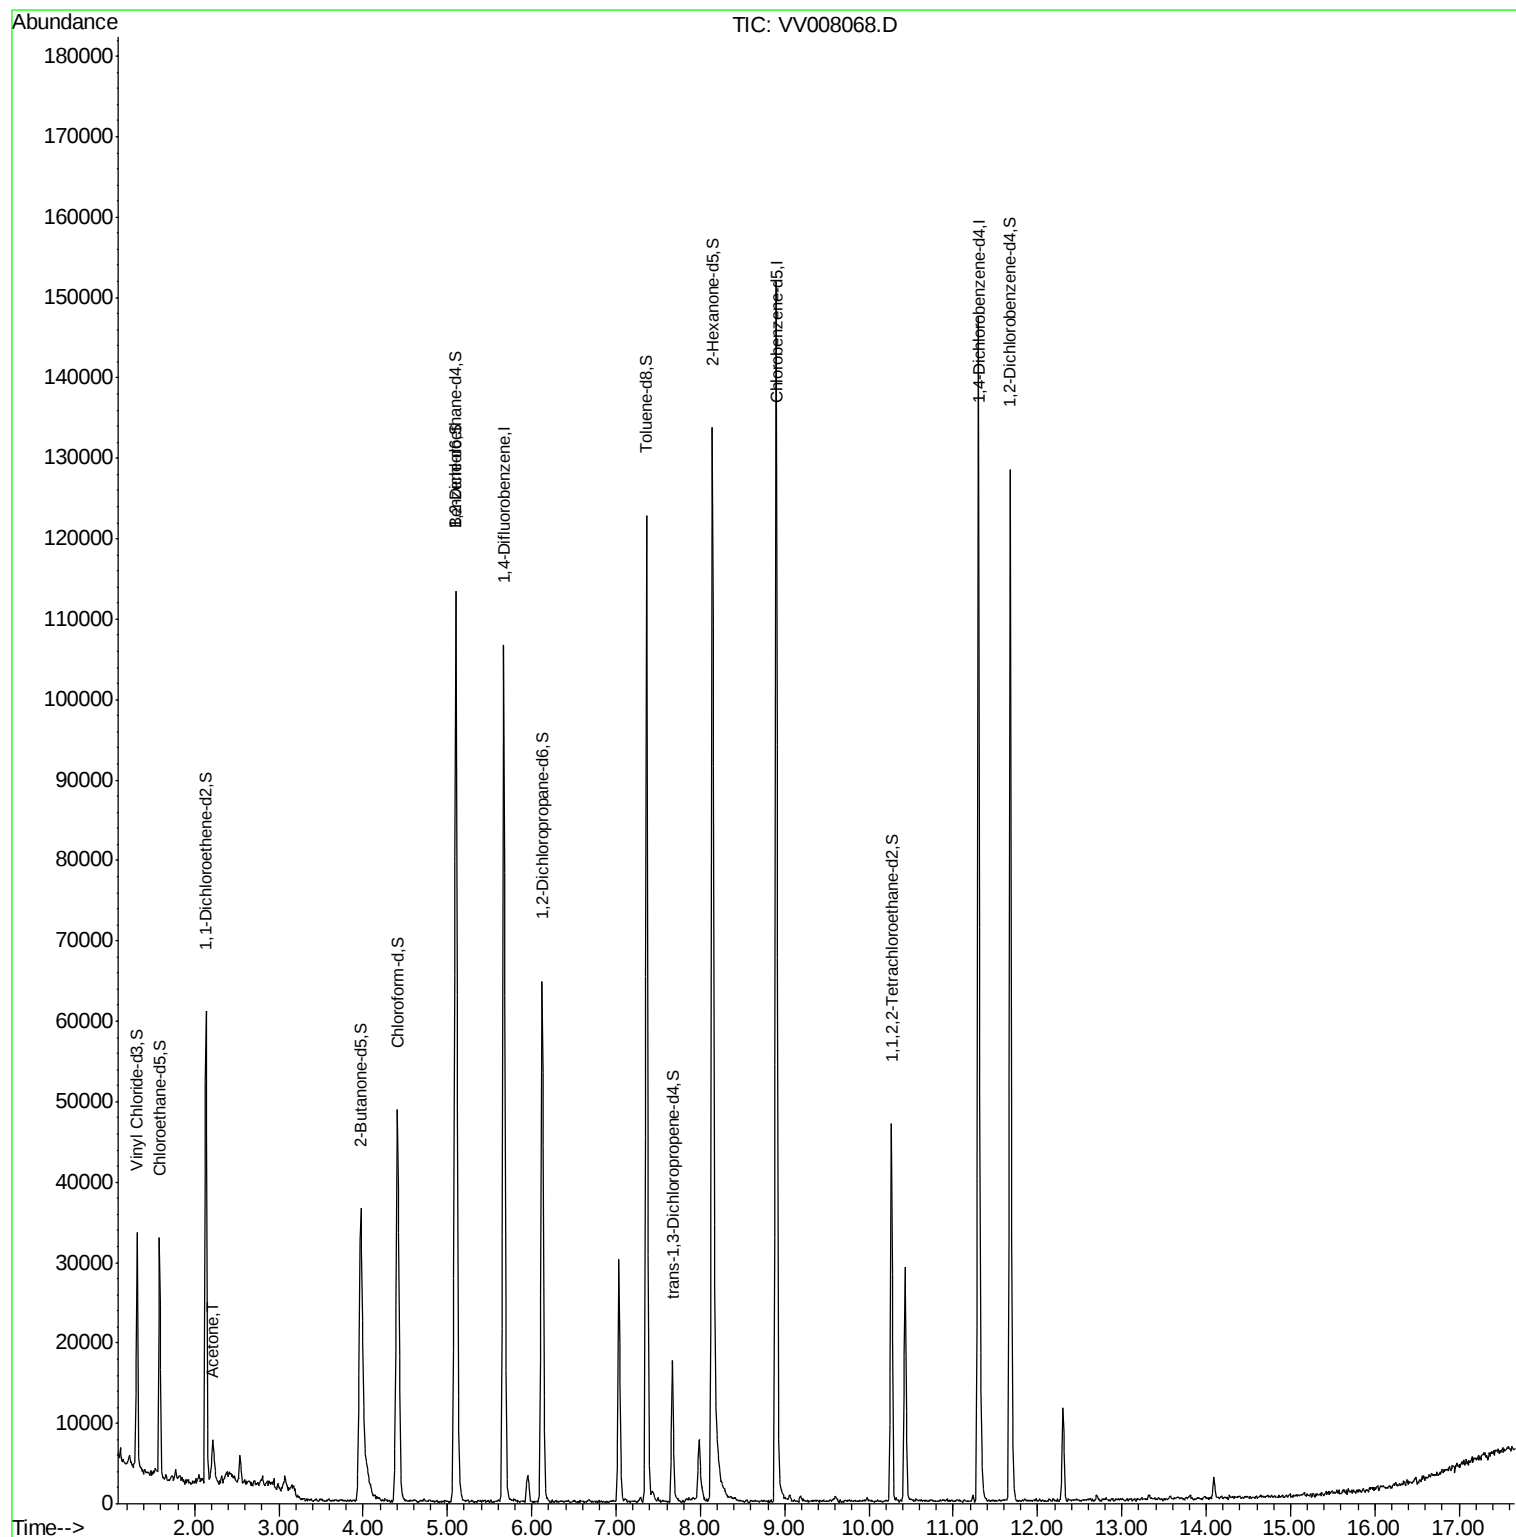

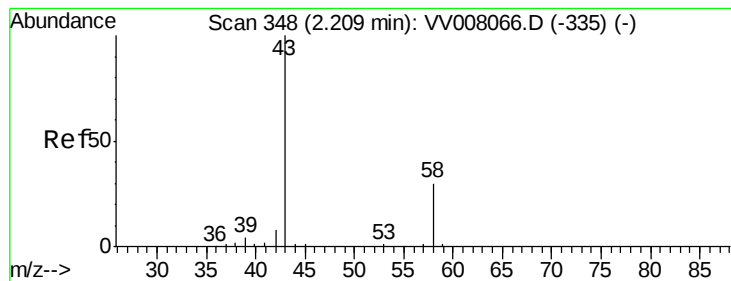

#13
 Acetone
 Concen: 7.136 ug/L
 RT: 2.22 min Scan# 350
 Delta R.T. 0.01 min
 Lab File: VV008068.D
 Acq: 04 Oct 2018 18:18

Instrument :
 MSVOA_V
 ClientSampleId :
 ESNN9

Tgt Ion: 43 Resp: 7559
 Ion Ratio Lower Upper
 43 100
 58 32.1 0.0 62.0

