

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100418\
 Data File : VV008060.D
 Acq On : 04 Oct 2018 14:07
 Operator : SY/MD
 Sample : J5246-02
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J70

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	63	72	89	rVB	30882	38072	12.71%	1.372%
2	1.431	100	106	114	rVB	17161	20139	6.72%	0.726%
3	1.586	147	154	169	rVB	30256	35778	11.94%	1.289%
4	2.135	315	325	337	rVB	64140	91400	30.51%	3.294%
5	2.203	338	346	348	rBV5	2450	3132	1.05%	0.113%
6	2.367	386	397	422	rVB	7990	27996	9.35%	1.009%
7	3.965	878	894	904	rBV	42908	112260	37.47%	4.046%
8	4.029	906	914	941	rVB	31628	99395	33.18%	3.582%
9	4.409	1016	1032	1053	rVB	51485	123049	41.08%	4.435%
10	5.100	1230	1247	1272	rBV2	117698	275743	92.05%	9.938%
11	5.669	1410	1424	1446	rBV	114858	222858	74.39%	8.032%
12	5.965	1503	1516	1533	rVB4	14387	28797	9.61%	1.038%
13	6.122	1553	1565	1584	rBV2	66348	134145	44.78%	4.835%
14	7.036	1837	1849	1862	rBV	30416	53836	17.97%	1.940%
15	7.364	1935	1951	1969	rBV	131005	227636	75.99%	8.204%
16	7.669	2036	2046	2062	rBV	18405	30622	10.22%	1.104%
17	7.984	2131	2144	2152	rBV2	11400	21461	7.16%	0.773%
18	8.142	2181	2193	2234	rBV2	146446	299569	100.00%	10.797%
19	8.900	2412	2429	2447	rBV	161877	266920	89.10%	9.620%
20	9.183	2506	2517	2525	rBV4	2469	4160	1.39%	0.150%
21	10.267	2843	2854	2866	rBV	50521	79210	26.44%	2.855%
22	10.428	2889	2904	2922	rBV	32135	54642	18.24%	1.969%
23	11.299	3163	3175	3202	rVB	154588	261725	87.37%	9.433%
24	11.675	3281	3292	3313	rVB	133802	219724	73.35%	7.919%
25	12.302	3476	3487	3497	rBV2	16172	26620	8.89%	0.959%
26	14.093	4030	4044	4055	rBV2	4750	7661	2.56%	0.276%
27	16.768	4870	4876	4888	rVB3	6439	8021	2.68%	0.289%


Sum of corrected areas: 2774571

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100418\
Data File : VV008060.D
Acq On : 04 Oct 2018 14:07
Operator : SY/MD
Sample : J5246-02
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J70

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

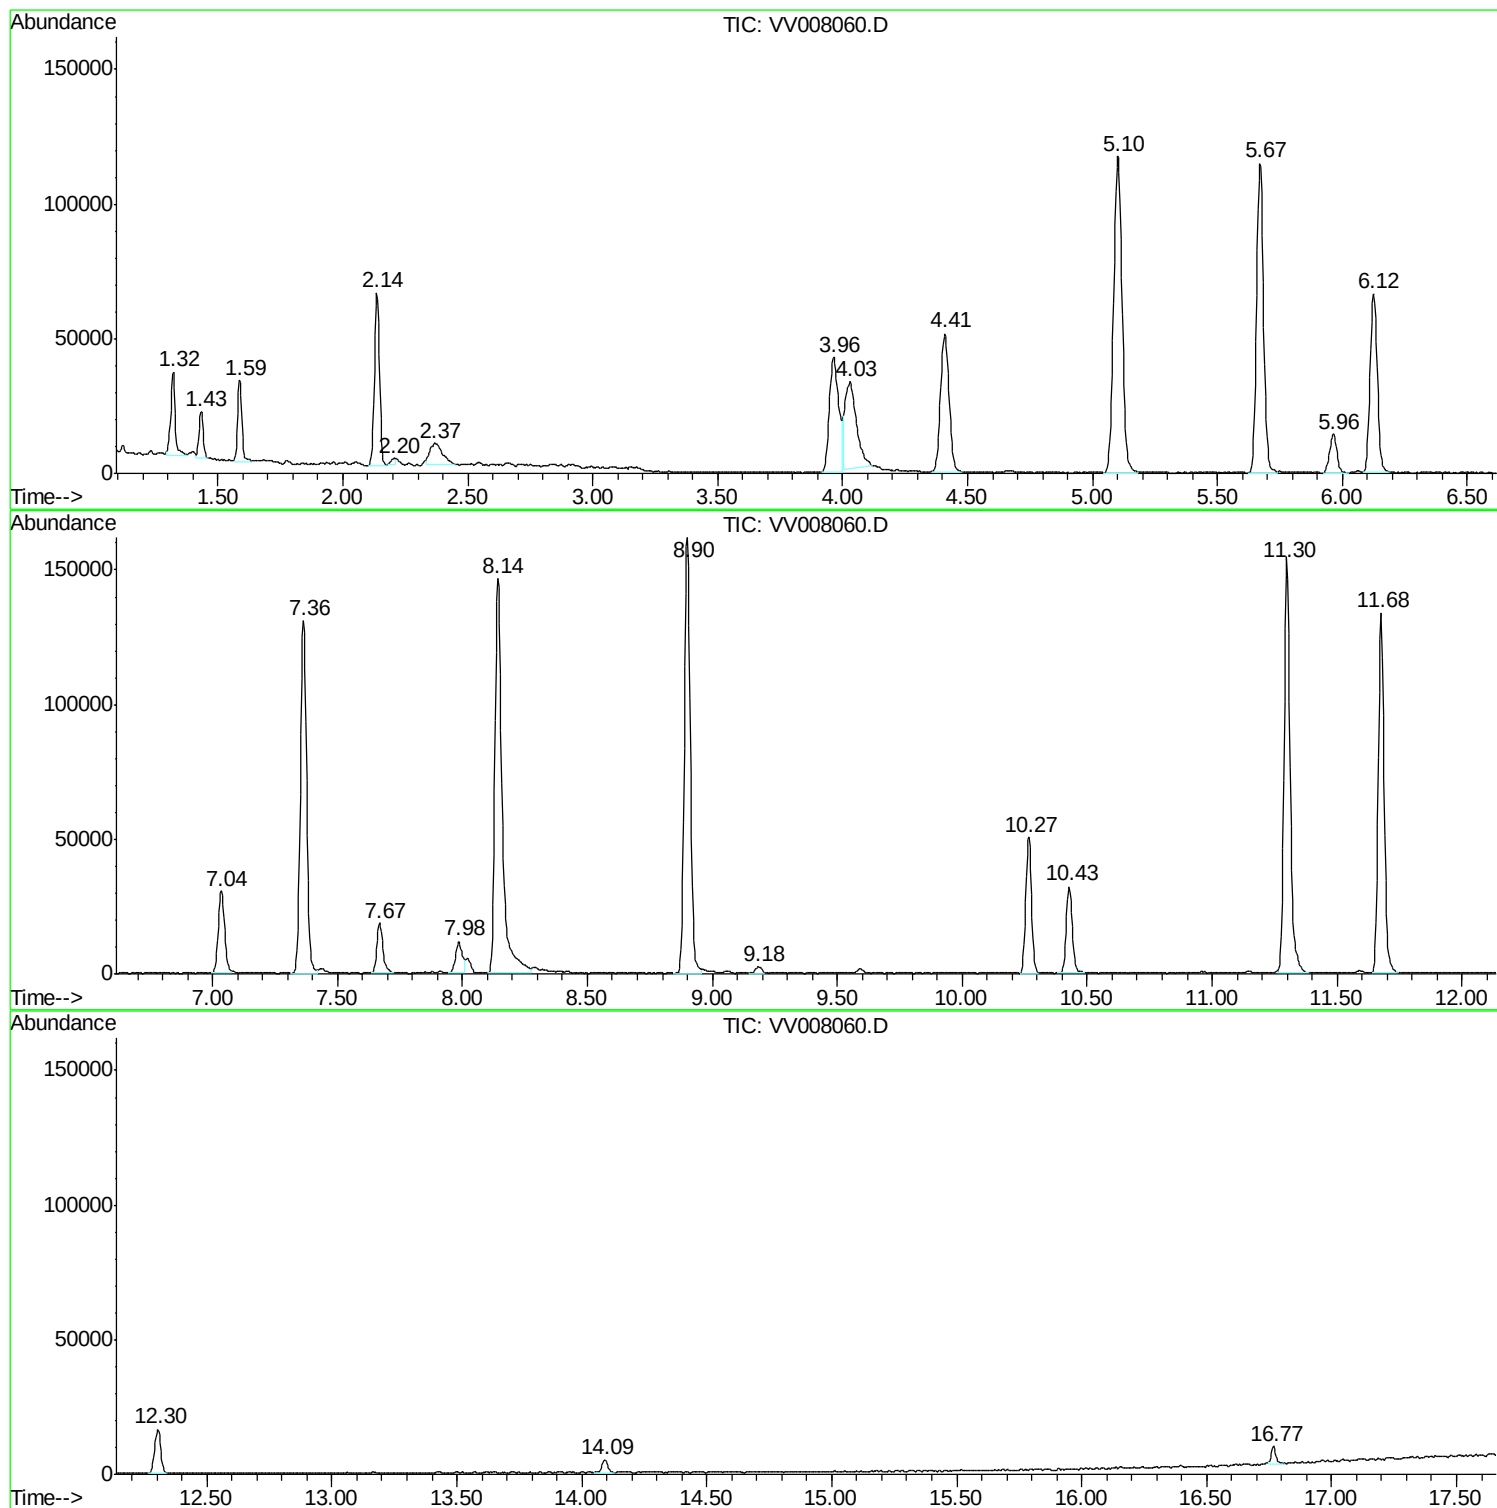

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100418\
Data File : VV008060.D
Acq On : 04 Oct 2018 14:07
Operator : SY/MD
Sample : J5246-02
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J70










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.37	0.63 ug/L	27996	1,4-Difluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	43
2		Formamide	45	CH3NO	000075-12-7	7
3		Methyltartronic acid	134	C4H6O5	000595-98-2	4
4		L-Lactic acid	90	C3H6O3	000079-33-4	4
5		Isopropyl Alcohol	60	C3H8O	000067-63-0	4

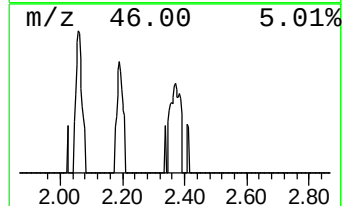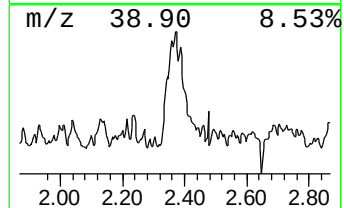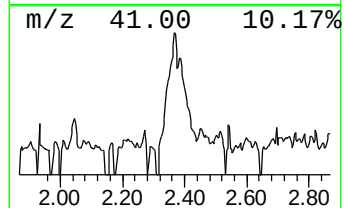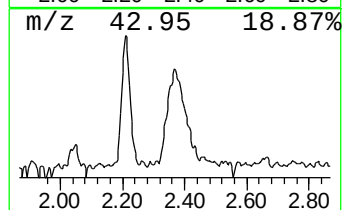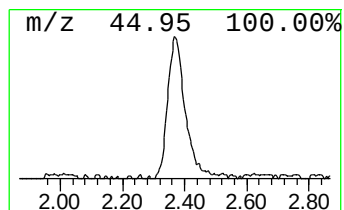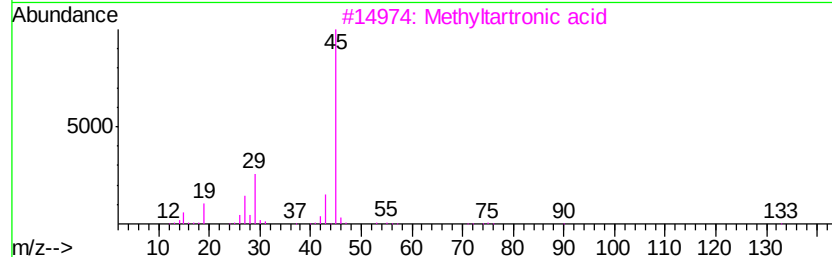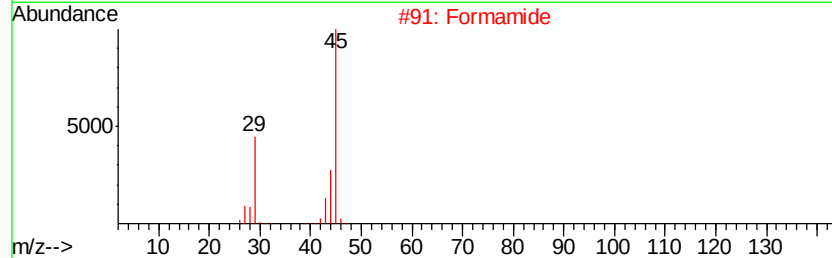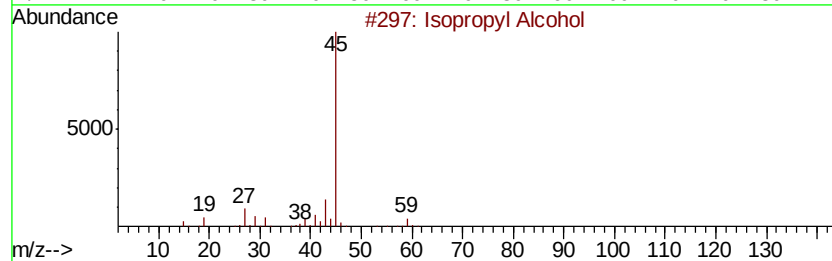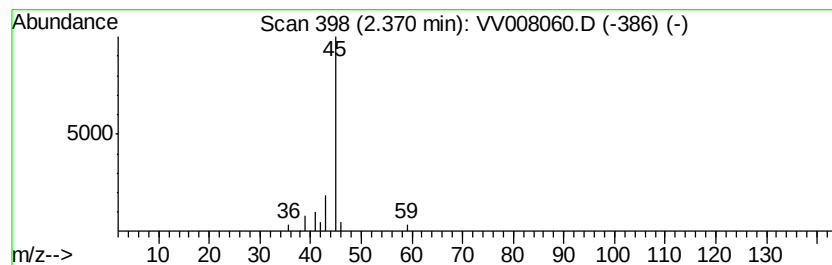

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100418\
Data File : VV008060.D
Acq On : 04 Oct 2018 14:07
Operator : SY/MD
Sample : J5246-02
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J70

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.37	0.6	ug/L	27996	1	5.67	222858	5.0