


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100418\
Data File : VV008054.D
Acq On : 04 Oct 2018 10:44
Operator : SY/MD
Sample : BFB81
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB81

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Oct 08 02:28:16 2018

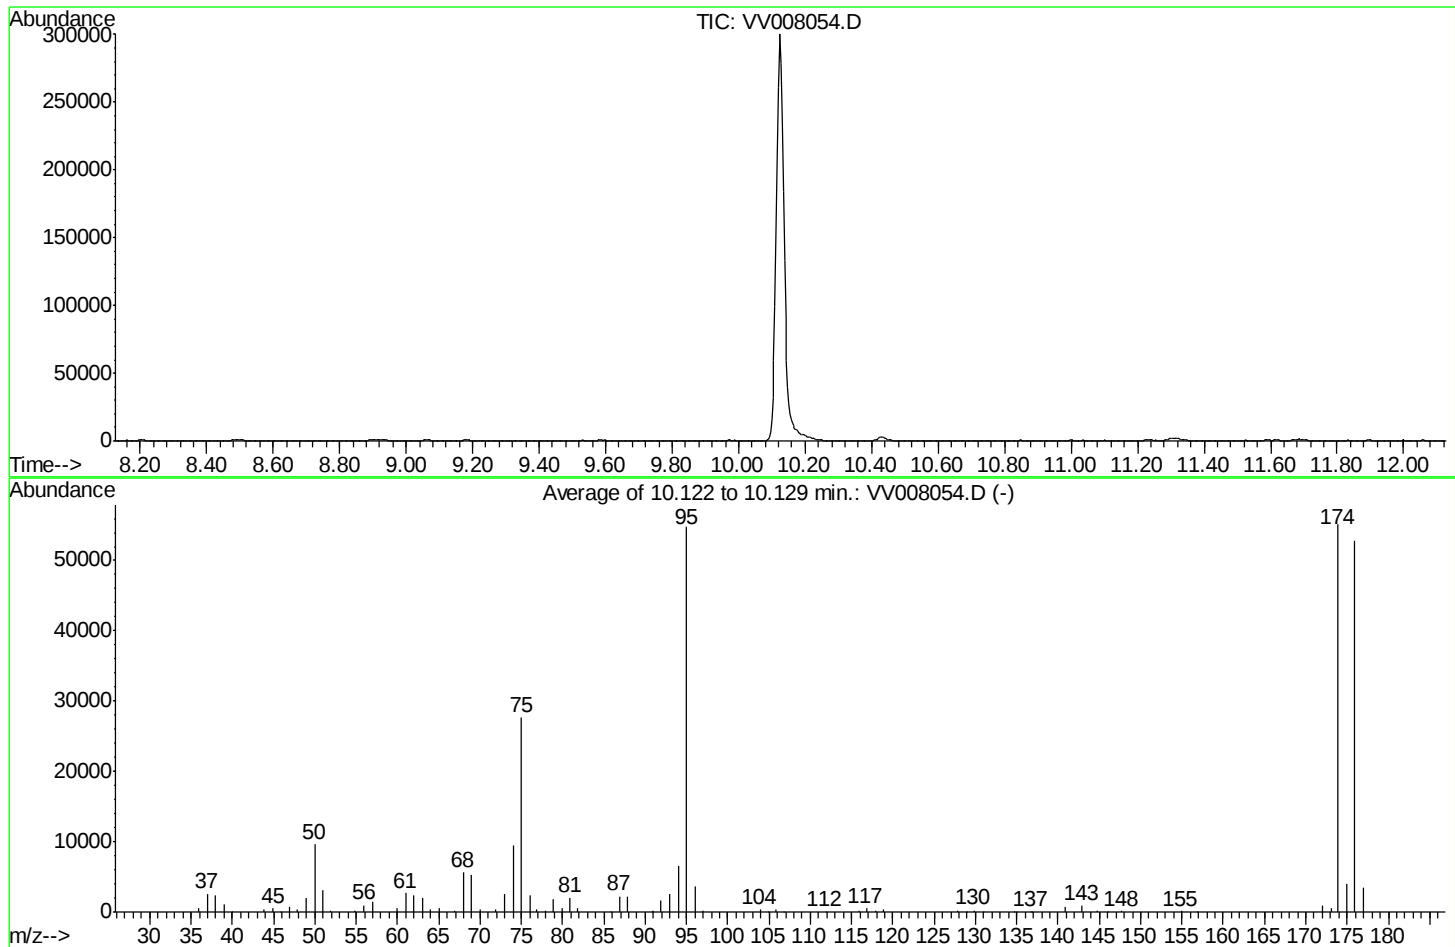

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	9615	PASS
75	95	30	80	50.3	27602	PASS
95	95	100	100	100.0	54906	PASS
96	95	5	9	6.7	3656	PASS
173	174	0.00	2	1.2	641	PASS
174	95	50	120	100.5	55157	PASS
175	174	5	9	7.3	4044	PASS
176	174	95	101	95.8	52856	PASS
177	176	5	9	6.5	3415	PASS

m/z	Abundance
35.90	559.0
37.00	2618.0
37.90	2317.0
39.00	1086.0
40.00	169.0
43.90	622.0
44.90	471.0
46.90	649.0
47.90	317.0
49.00	2180.0
50.00	10040.0
51.00	3376.0
51.90	184.0
54.90	153.0
56.00	925.0
57.00	1506.0
60.00	546.0
61.00	2788.0
61.90	2514.0
63.00	2029.0
64.00	311.0
65.00	494.0
66.90	179.0
68.00	5769.0
69.00	5444.0
70.00	463.0
71.90	411.0
73.00	2518.0
74.00	9707.0
75.00	28176.0
76.00	2482.0
76.90	414.0
77.90	265.0
78.90	2002.0
79.90	642.0
80.90	2018.0
81.80	484.0
86.90	2273.0
87.90	2084.0
90.80	213.0
91.00	216.0
92.00	1707.0
92.90	2626.0
94.00	6857.0
95.00	56024.0
96.00	3843.0
97.00	124.0
103.90	312.0
104.90	132.0
105.90	286.0
115.90	225.0
116.80	463.0
117.90	212.0
118.90	314.0
127.80	175.0
128.90	129.0
129.80	261.0
130.90	105.0
135.00	110.0
136.70	131.0
140.80	661.0
142.90	882.0
144.80	245.0
147.70	146.0
154.90	117.0
172.00	897.0
173.90	54840.0
174.90	4065.0
175.90	52432.0
176.90	3427.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
35.90	517.0
37.00	2661.0
37.90	2368.0
39.00	1106.0
40.00	180.0
43.90	584.0
44.90	487.0
45.90	103.0
46.90	662.0
47.90	287.0
49.00	2116.0
50.00	9848.0
51.00	3279.0
51.90	157.0
54.90	141.0
56.00	945.0
57.00	1548.0
60.00	539.0
61.00	2822.0
62.00	2555.0
63.00	2137.0
64.00	340.0
65.10	483.0
66.90	196.0
68.00	5789.0
69.00	5494.0
70.00	449.0
71.90	366.0
73.00	2570.0
74.00	9860.0
75.00	28560.0
76.00	2505.0
76.90	372.0
77.90	258.0
78.90	1957.0
79.90	614.0
80.90	2098.0
81.80	484.0
85.90	111.0
86.90	2294.0
87.90	2249.0
91.00	239.0
92.00	1675.0
92.90	2681.0
94.00	6806.0
95.00	56592.0
96.00	3733.0
97.10	154.0
104.00	337.0
104.90	126.0
105.80	314.0
106.80	108.0
115.90	239.0
116.80	498.0
117.80	230.0
118.90	305.0
127.80	190.0
128.90	112.0
129.80	268.0
134.70	114.0
136.70	133.0
140.80	688.0
142.90	964.0
144.80	199.0
147.80	127.0
154.90	150.0
156.90	105.0
171.90	917.0
173.10	950.0
173.90	56888.0
174.90	4151.0
175.90	54704.0
176.90	3532.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
35.90	411.0
37.00	2411.0
37.90	2253.0
39.00	1021.0
40.00	163.0
43.90	516.0
45.00	474.0
46.90	621.0
47.80	269.0
49.00	1888.0
50.00	8958.0
51.00	2911.0
51.90	129.0
54.90	136.0
55.90	884.0
57.00	1450.0
60.00	480.0
61.00	2568.0
62.00	2323.0
63.00	2006.0
63.90	306.0
65.00	465.0
66.80	178.0
68.00	5274.0
69.00	4963.0
70.00	398.0
71.90	294.0
72.90	2361.0
74.00	9066.0
75.00	26072.0
76.00	2326.0
76.90	317.0
77.90	234.0
78.90	1723.0
79.90	534.0
80.90	1948.0
81.80	495.0
85.90	123.0
86.90	2032.0
87.90	2048.0
90.90	228.0
91.90	1513.0
93.00	2526.0
94.00	6298.0
95.00	52104.0
96.00	3392.0
97.10	158.0
103.90	293.0
105.80	291.0
106.80	111.0
111.80	103.0
115.90	221.0
116.80	439.0
117.80	244.0
118.80	295.0
127.80	198.0
129.80	258.0
134.70	124.0
136.90	115.0
140.80	655.0
142.90	888.0
144.80	141.0
145.90	101.0
147.80	114.0
155.00	152.0
156.90	122.0
171.90	902.0
173.00	974.0
173.90	53744.0
174.90	3916.0
175.90	51432.0
176.90	3288.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
40.10	103.0
43.80	273.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81