
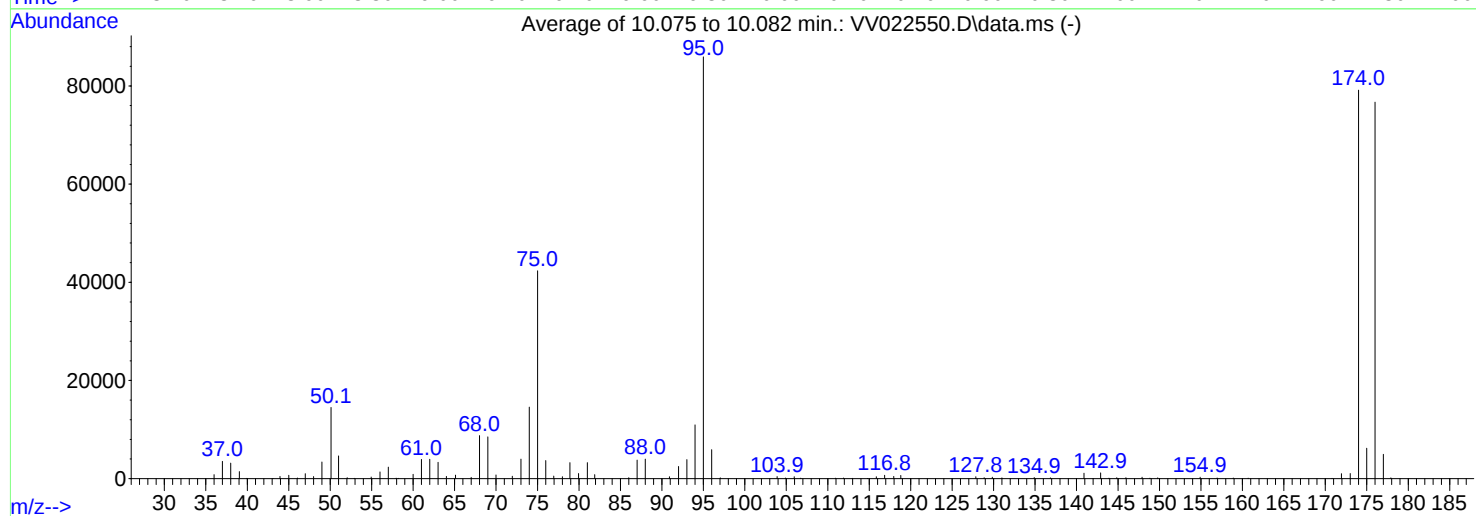


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100421\
 Data File : VV022550.D
 Acq On : 04 Oct 2021 09:24
 Operator : SY/MD
 Sample : BFB208
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB208

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Oct 06 07:50:25 2021

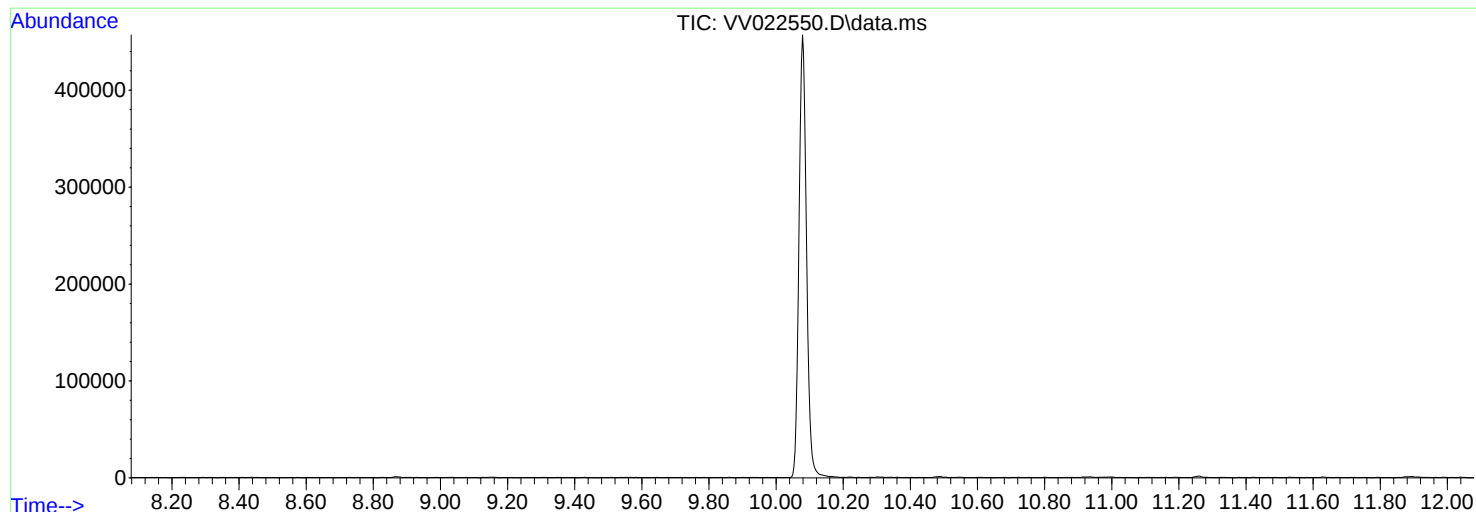

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	14494	PASS
75	95	30	80	49.3	42333	PASS
95	95	100	100	100.0	85928	PASS
96	95	5	9	6.9	5889	PASS
173	174	0.00	2	1.3	1044	PASS
174	95	50	120	92.1	79152	PASS
175	174	5	9	7.8	6182	PASS
176	174	95	105	96.9	76707	PASS
177	176	5	10	6.5	4951	PASS

m/z	Abundance
40.00	120.0
43.90	286.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
36.00	738.0
37.00	3516.0
38.00	3130.0
39.00	1434.0
39.90	209.0
43.10	114.0
44.00	719.0
45.00	708.0
46.00	125.0
47.00	1025.0
48.00	393.0
49.00	3323.0
50.10	14228.0
51.00	4732.0
52.10	222.0
54.90	249.0
56.00	1352.0
57.00	2335.0
57.90	127.0
60.00	842.0
61.00	3986.0
62.00	3871.0
63.00	3153.0
64.00	484.0
65.10	659.0
67.00	284.0
68.00	8516.0
69.00	8482.0
70.00	701.0
72.00	453.0
73.00	4150.0
74.00	14243.0
75.00	41936.0
76.00	3625.0
77.00	470.0
78.00	369.0
78.90	3109.0
79.90	1085.0
81.00	3127.0
81.90	792.0
86.00	204.0
87.00	3535.0
88.00	3952.0
90.90	418.0
92.00	2359.0
93.00	3819.0
94.00	10746.0
95.00	84112.0
96.00	5763.0
97.00	152.0
103.90	386.0
104.90	125.0
106.00	375.0
106.70	107.0
111.00	118.0
111.90	121.0
112.90	139.0
115.90	381.0
116.90	675.0
118.00	430.0
118.80	646.0
127.90	327.0
128.80	162.0
129.80	317.0
131.00	155.0
134.90	184.0
136.80	145.0
140.90	1035.0
142.00	115.0
142.90	1134.0
144.90	201.0
146.00	217.0
147.90	281.0
148.90	116.0
149.80	148.0
154.90	236.0
156.90	127.0
158.90	157.0
170.80	119.0
171.90	1028.0
173.00	1026.0
174.00	75144.0
175.00	6081.0
176.00	73776.0
177.00	4603.0
177.90	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
36.00	897.0
37.00	3672.0
38.00	3193.0
39.00	1482.0
39.90	210.0
44.00	759.0
45.00	693.0
46.00	136.0
47.00	1064.0
48.00	438.0
49.00	3491.0
50.10	15102.0
51.00	4771.0
52.00	207.0
52.90	116.0
54.90	331.0
56.00	1429.0
57.00	2369.0
58.00	127.0
60.00	910.0
61.00	4072.0
62.00	4065.0
63.00	3431.0
64.00	436.0
65.10	735.0
67.00	289.0
68.00	9137.0
69.00	8856.0
70.00	768.0
71.90	520.0
73.00	4090.0
74.00	15058.0
75.00	43736.0
76.00	3777.0
76.90	536.0
78.00	402.0
78.90	3379.0
80.00	1120.0
81.00	3377.0
81.90	872.0
86.00	203.0
87.00	3946.0
88.00	4109.0
90.90	415.0
92.00	2579.0
93.00	3995.0
94.00	11409.0
95.00	88904.0
96.00	6079.0
97.00	167.0
103.90	460.0
104.90	139.0
105.90	412.0
106.70	106.0
110.90	116.0
111.90	145.0
113.00	110.0
115.80	407.0
116.90	691.0
117.90	484.0
118.80	653.0
127.90	411.0
128.90	199.0
129.90	301.0
131.00	167.0
134.90	232.0
136.80	159.0
140.90	1128.0
142.90	1216.0
143.90	140.0
144.80	188.0
146.00	203.0
147.90	313.0
148.90	119.0
149.80	176.0
154.90	299.0
157.00	153.0
158.90	153.0
160.70	124.0
170.80	118.0
171.90	1049.0
173.00	1083.0
174.00	82032.0
175.00	6432.0
176.00	79752.0
177.00	5094.0
177.90	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
36.00	841.0
37.00	3400.0
38.00	3147.0
39.10	1408.0
40.00	187.0
44.00	723.0
45.00	652.0
46.10	144.0
47.00	937.0
48.00	435.0
49.00	3374.0
50.10	14153.0
51.00	4390.0
52.00	198.0
52.90	118.0
55.00	390.0
56.00	1326.0
57.00	2316.0
58.20	175.0
60.00	928.0
61.00	3648.0
62.00	3865.0
63.00	3411.0
64.00	423.0
65.10	762.0
67.00	248.0
68.00	8643.0
69.00	8231.0
70.00	765.0
71.90	516.0
73.00	3663.0
74.00	14447.0
75.00	41328.0
76.00	3604.0
76.90	541.0
78.00	392.0
78.90	3261.0
80.00	966.0
81.00	3268.0
81.90	839.0
86.00	203.0
87.00	3902.0
88.00	3858.0
90.90	387.0
92.00	2475.0
93.00	3841.0
94.00	10752.0
95.00	84768.0
96.00	5825.0
97.10	187.0
103.90	468.0
104.90	163.0
105.90	428.0
106.80	107.0
110.90	112.0
111.90	139.0
114.80	114.0
115.80	397.0
116.80	680.0
117.90	442.0
118.80	626.0
127.80	435.0
128.90	201.0
129.90	291.0
131.00	156.0
134.90	272.0
136.90	175.0
140.90	1132.0
142.90	1199.0
143.90	155.0
144.80	175.0
145.80	176.0
147.90	297.0
148.80	102.0
149.80	160.0
154.90	319.0
157.00	151.0
158.90	108.0
160.70	128.0
172.00	967.0
173.00	1022.0
174.00	80280.0
175.00	6032.0
176.00	76592.0
177.00	5155.0
177.90	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208