

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032220.D
 Acq On : 04 Oct 2023 11:02
 Operator : SY/MD
 Sample : 04708-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJS7

Quant Time: Oct 05 01:39:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 05 01:37:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	95958	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	95065	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	44778	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	40157	5.146	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.000%
7) Chloroethane-d5	1.532	69	34097	5.382	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.600%
11) 1,1-Dichloroethene-d2	2.060	65	17041	5.178	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	103.600%
20) 2-Butanone-d5	3.802	46	95061	48.152	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.300%
24) Chloroform-d	4.252	84	70243	5.102	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.000%
26) 1,2-Dichloroethane-d4	4.947	65	34935	5.357	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.200%
32) Benzene-d6	4.963	84	141556	5.061	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.200%
36) 1,2-Dichloropropane-d6	5.992	67	47225	5.095	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.000%
41) Toluene-d8	7.249	98	123773	4.839	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.800%
43) trans-1,3-Dichloroprop...	7.561	79	15349	4.674	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.400%
46) 2-Hexanone-d5	8.030	63	70104	45.368	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.740%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	31539	4.865	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.400%
66) 1,2-Dichlorobenzene-d4	11.564	152	44781	5.389	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.800%
Target Compounds						
					Qvalue	
13) Acetone	2.130	43	2709	1.780	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032220.D
Acq On : 04 Oct 2023 11:02
Operator : SY/MD
Sample : 04708-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJS7

Quant Time: Oct 05 01:39:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 05 01:37:52 2023
Response via : Initial Calibration

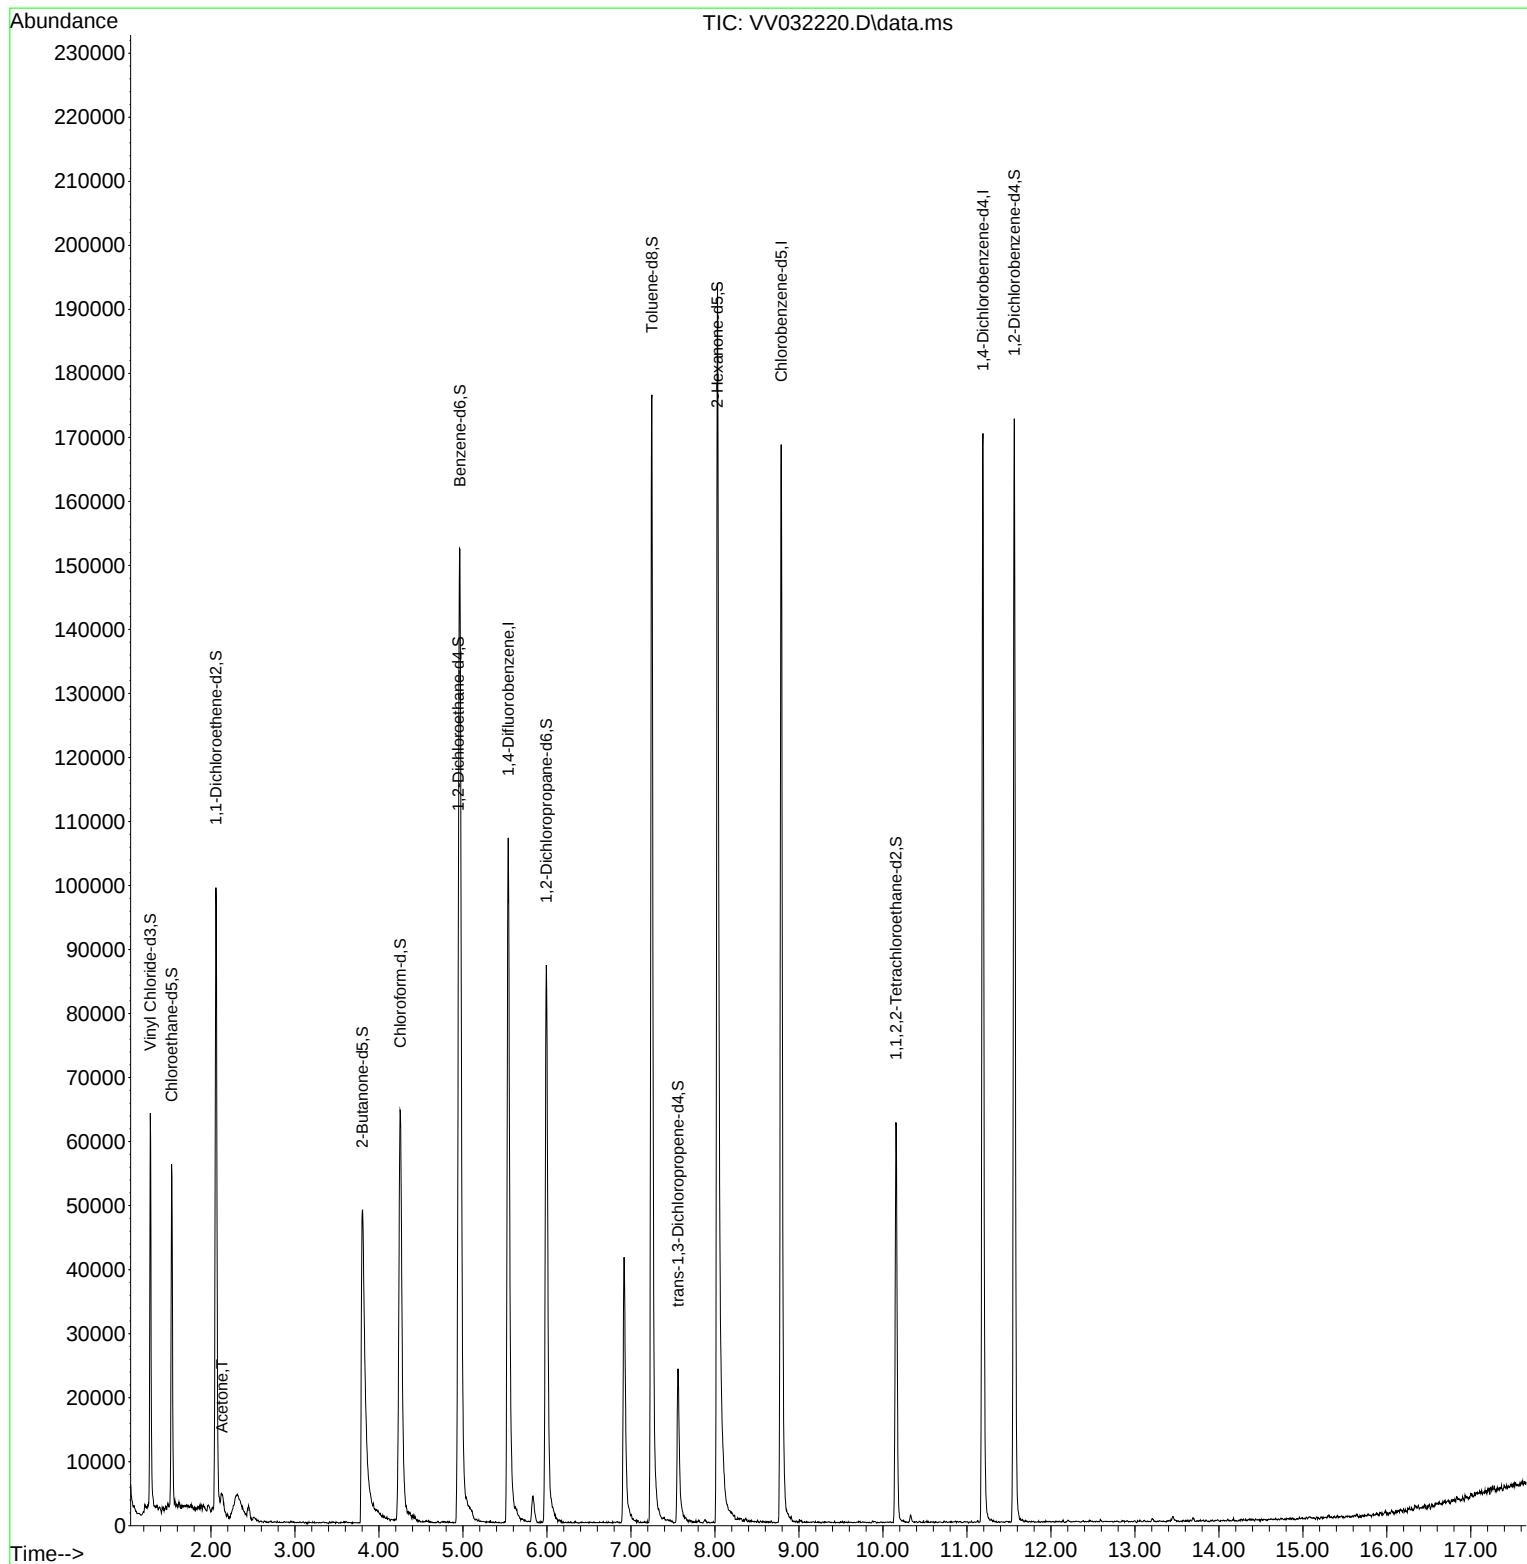

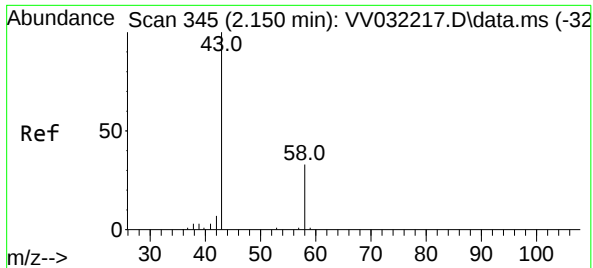

#13
 Acetone
 Concen: 1.780 ug/L
 RT: 2.130 min Scan# 31
 Delta R.T. -0.019 min
 Lab File: VV032220.D
 Acq: 04 Oct 2023 11:02

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJS7

Tgt Ion: 43 Resp: 2709
 Ion Ratio Lower Upper
 43 100
 58 34.8 0.0 66.0

