

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032227.D
 Acq On : 04 Oct 2023 14:17
 Operator : SY/MD
 Sample : VIBLK321
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK321

Quant Time: Oct 05 01:41:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 05 01:37:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	100697	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	99207	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	47158	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	38231	4.668	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.400%
7) Chloroethane-d5	1.532	69	33199	4.994	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.800%
11) 1,1-Dichloroethene-d2	2.060	65	16116	4.666	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	93.400%
20) 2-Butanone-d5	3.818	46	98636	47.611	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.220%
24) Chloroform-d	4.256	84	69034	4.778	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
26) 1,2-Dichloroethane-d4	4.947	65	34494	5.041	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.800%
32) Benzene-d6	4.966	84	140514	4.814	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.200%
36) 1,2-Dichloropropane-d6	5.995	67	46925	4.852	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.000%
41) Toluene-d8	7.249	98	120839	4.527	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.600%
43) trans-1,3-Dichloroprop...	7.561	79	16132	4.707	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.200%
46) 2-Hexanone-d5	8.034	63	75269	46.677	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.360%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	32893	4.862	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.200%
66) 1,2-Dichlorobenzene-d4	11.564	152	44737	5.112	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.200%
Target Compounds						Qvalue
34) Trichloroethene	5.841	95	2812	0.295	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032227.D
Acq On : 04 Oct 2023 14:17
Operator : SY/MD
Sample : VIBLK321
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK321


Quant Time: Oct 05 01:41:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 05 01:37:52 2023
Response via : Initial Calibration

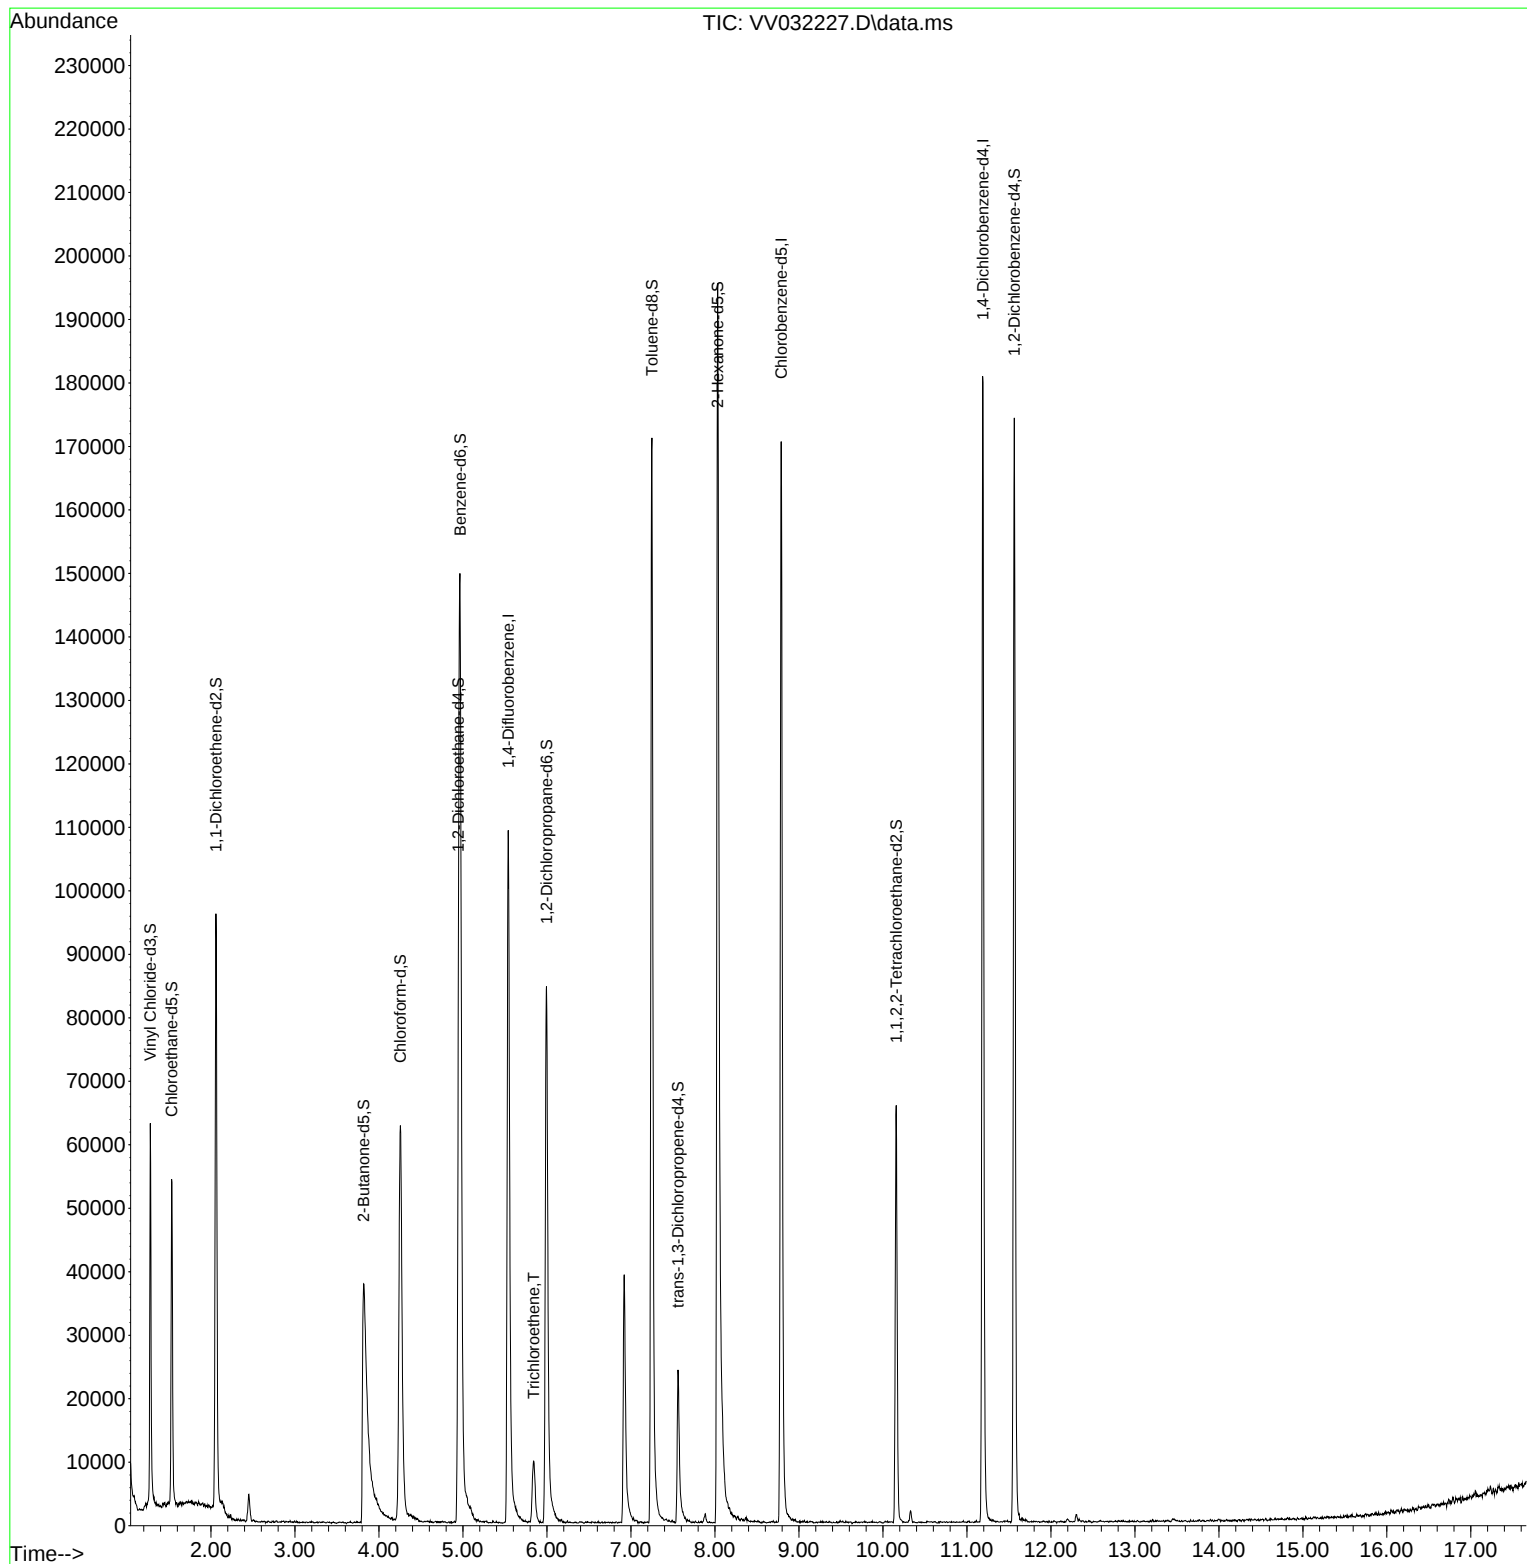

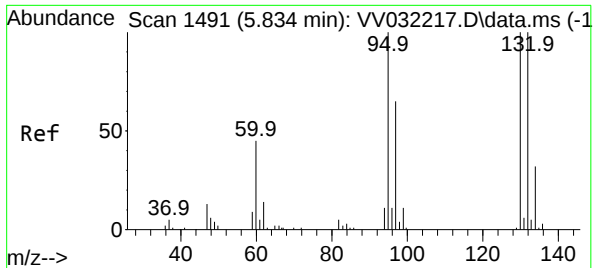

#34
 Trichloroethene
 Concen: 0.295 ug/L
 RT: 5.841 min Scan# 1493
 Delta R.T. 0.006 min
 Lab File: VV032227.D
 Acq: 04 Oct 2023 14:17

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK321

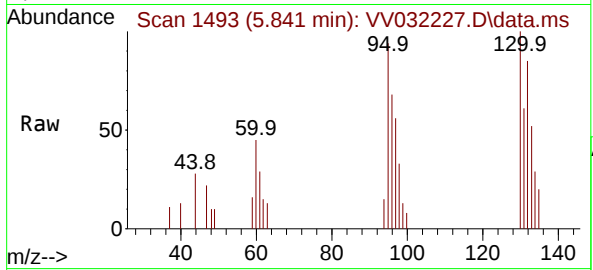

Tgt Ion: 95 Resp: 2812

Ion	Ratio	Lower	Upper
95	100		
97	60.1	45.7	84.9
132	90.4	70.3	130.5
130	106.9	69.6	129.2

