

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032218.D
 Acq On : 04 Oct 2023 10:12
 Operator : SY/MD
 Sample : VV1004WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK362

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032218.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	85	rBV	58793	62427	16.37%	1.993%
2	1.532	145	153	166	rBV	50831	58731	15.40%	1.875%
3	2.057	306	316	330	rBV	93125	135311	35.49%	4.320%
4	2.449	428	438	450	rVB	8098	13590	3.56%	0.434%
5	2.966	590	599	612	rVB5	2144	4859	1.27%	0.155%
6	3.822	855	865	907	rBV2	30948	136464	35.79%	4.357%
7	4.253	981	999	1026	rBV	60236	160276	42.03%	5.117%
8	4.960	1203	1219	1249	rBV2	149308	381306	100.00%	12.173%
9	5.539	1386	1399	1435	rBV	110499	240065	62.96%	7.664%
10	5.834	1478	1491	1505	rBV5	3602	7772	2.04%	0.248%
11	5.992	1527	1540	1562	rBV	81824	178826	46.90%	5.709%
12	6.918	1818	1828	1855	rBV	39024	79406	20.82%	2.535%
13	7.246	1916	1930	1968	rBV	169867	314139	82.39%	10.029%
14	7.561	2019	2028	2052	rBV	22016	44134	11.57%	1.409%
15	8.034	2165	2175	2210	rBV	182774	379077	99.42%	12.102%
16	8.789	2399	2410	2434	rBV	175326	295690	77.55%	9.440%
17	10.159	2824	2836	2852	rBV	59418	96482	25.30%	3.080%
18	11.188	3145	3156	3177	rBV	176254	280250	73.50%	8.947%
19	11.564	3261	3273	3296	rBV	165844	263493	69.10%	8.412%




Sum of corrected areas: 3132298

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032218.D
Acq On : 04 Oct 2023 10:12
Operator : SY/MD
Sample : VV1004WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK362

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

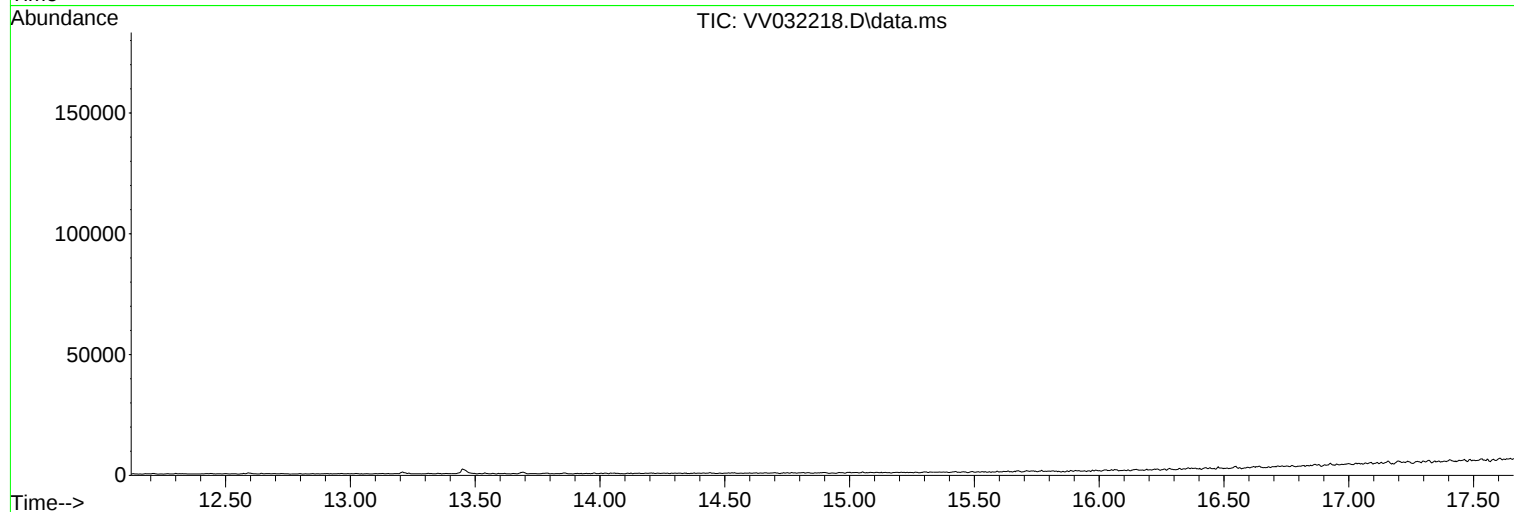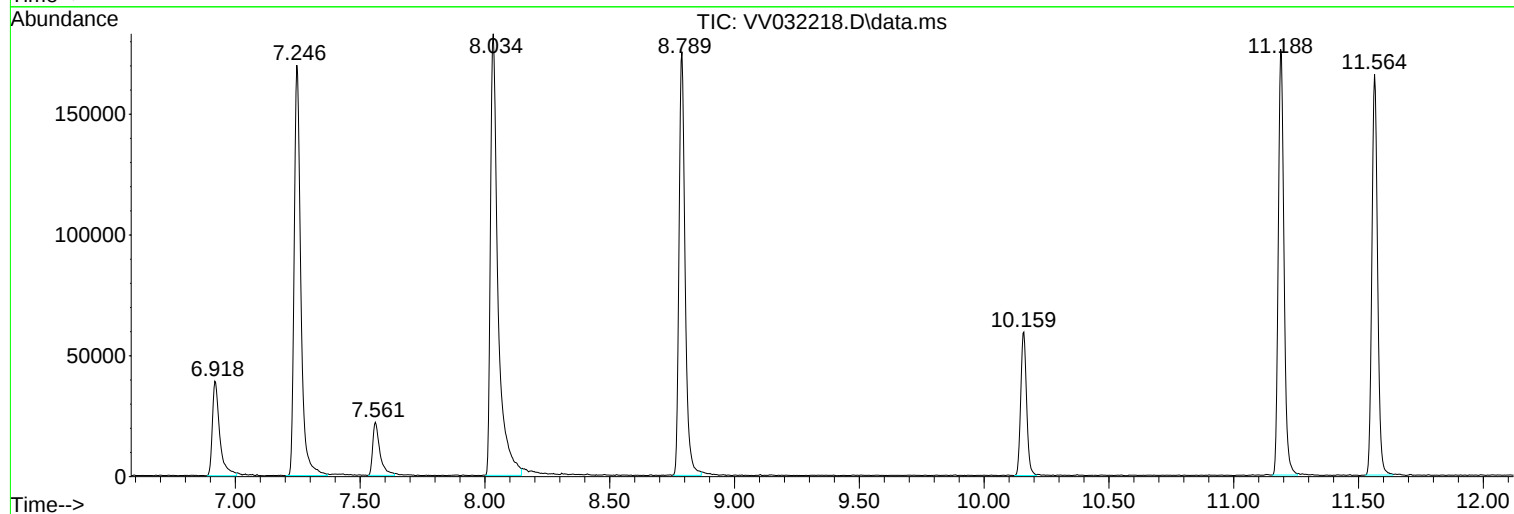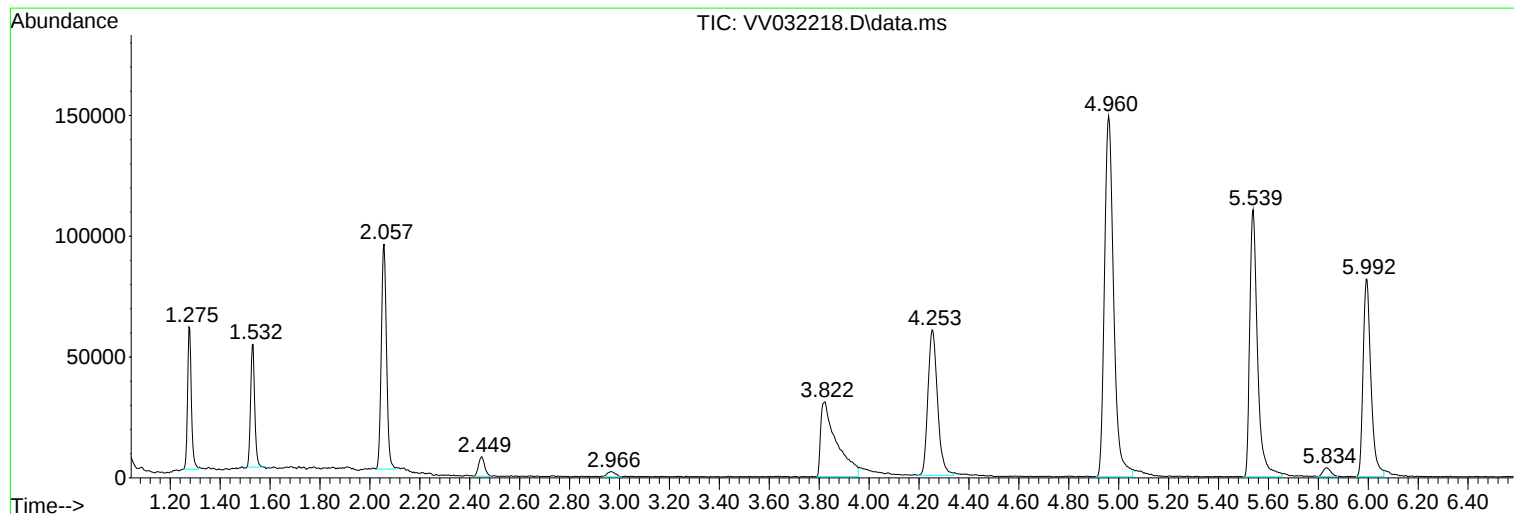

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032218.D
Acq On : 04 Oct 2023 10:12
Operator : SY/MD
Sample : VV1004WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK362

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032218.D
Acq On : 04 Oct 2023 10:12
Operator : SY/MD
Sample : VV1004WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK362

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc