

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032221.D
 Acq On : 04 Oct 2023 11:27
 Operator : SY/MD
 Sample : 04708-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJU2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	93	rBV	624551	674566	38.91%	4.320%
2	1.532	146	153	168	rVB	52921	60949	3.52%	0.390%
3	2.069	306	320	346	rBV2	494603	776659	44.80%	4.973%
4	2.449	426	438	458	rBV	189022	316577	18.26%	2.027%
5	2.696	503	515	540	rBV	169337	298909	17.24%	1.914%
6	3.815	849	863	907	rBV2	283036	752064	43.38%	4.816%
7	4.252	984	999	1029	rBV	62295	164199	9.47%	1.051%
8	4.516	1061	1081	1106	rBV	94361	245297	14.15%	1.571%
9	4.738	1134	1150	1173	rBV2	53261	131583	7.59%	0.843%
10	4.963	1204	1220	1228	rBV2	154084	371589	21.43%	2.380%
11	5.040	1229	1244	1276	rVB2	171238	603124	34.79%	3.862%
12	5.539	1388	1399	1423	rBV	119058	249007	14.36%	1.595%
13	5.834	1479	1491	1528	rBV	216525	454489	26.22%	2.910%
14	5.992	1528	1540	1560	rBV	86693	181385	10.46%	1.162%
15	6.095	1560	1572	1593	rVV	155420	311129	17.95%	1.992%
16	6.918	1818	1828	1846	rBV2	41179	79117	4.56%	0.507%
17	7.246	1919	1930	1943	rBV	178967	318664	18.38%	2.041%
18	7.320	1943	1953	1985	rVB	228940	413684	23.86%	2.649%
19	7.561	2019	2028	2047	rBV	24376	45775	2.64%	0.293%
20	7.773	2082	2094	2114	rBV	104048	187080	10.79%	1.198%
21	7.908	2120	2136	2164	rBV	484614	841042	48.51%	5.386%
22	8.030	2164	2174	2213	rVV	201308	394146	22.73%	2.524%
23	8.815	2413	2418	2448	rVB	458491	759383	43.80%	4.863%
24	8.950	2448	2460	2487	rVV	539165	861612	49.70%	5.517%
25	9.075	2487	2499	2538	rVB	985941	1562824	90.15%	10.008%
26	9.497	2611	2630	2674	rBV2	926773	1733675	100.00%	11.102%
27	10.159	2825	2836	2853	rBV	63858	102966	5.94%	0.659%
28	11.210	3144	3163	3185	rBV2	826224	1554645	89.67%	9.955%
29	11.577	3261	3277	3298	rBV3	274906	646514	37.29%	4.140%
30	13.201	3771	3782	3806	rBV	340068	523554	30.20%	3.353%




Sum of corrected areas: 15616207

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032221.D
Acq On : 04 Oct 2023 11:27
Operator : SY/MD
Sample : 04708-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJU2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

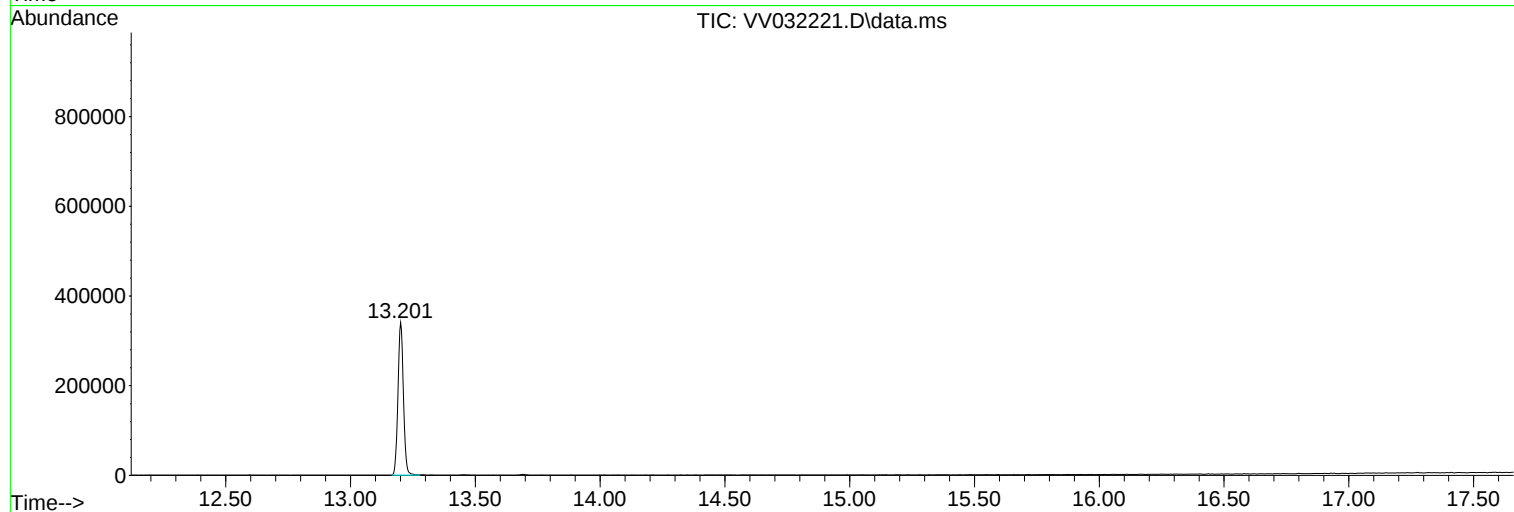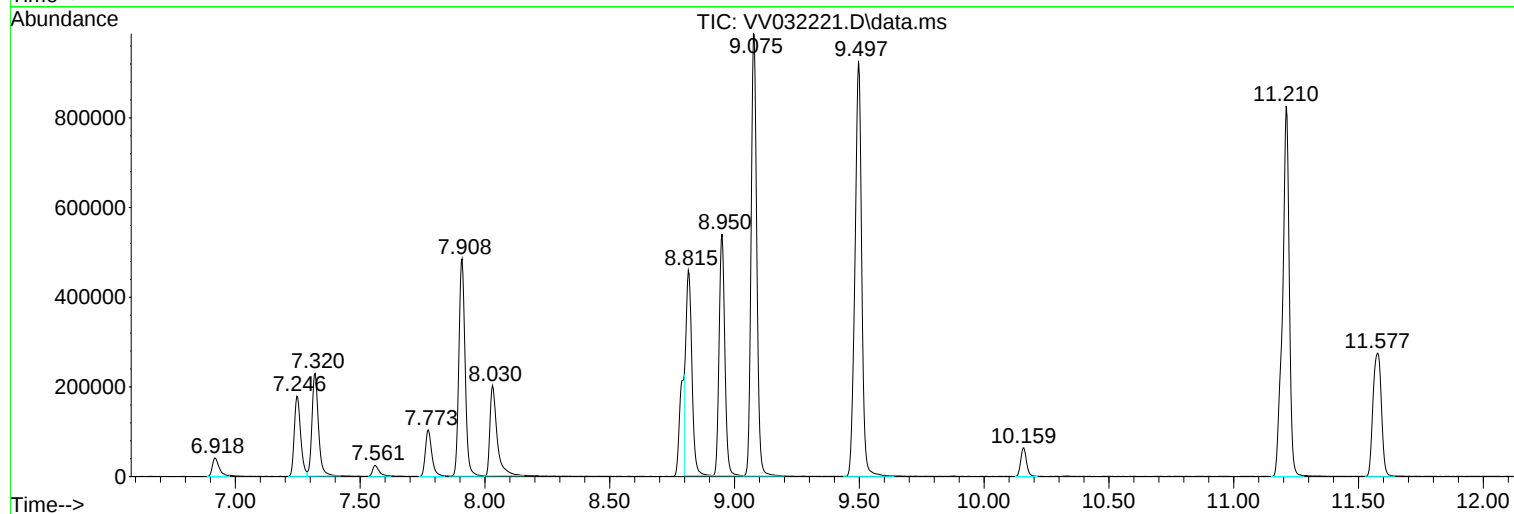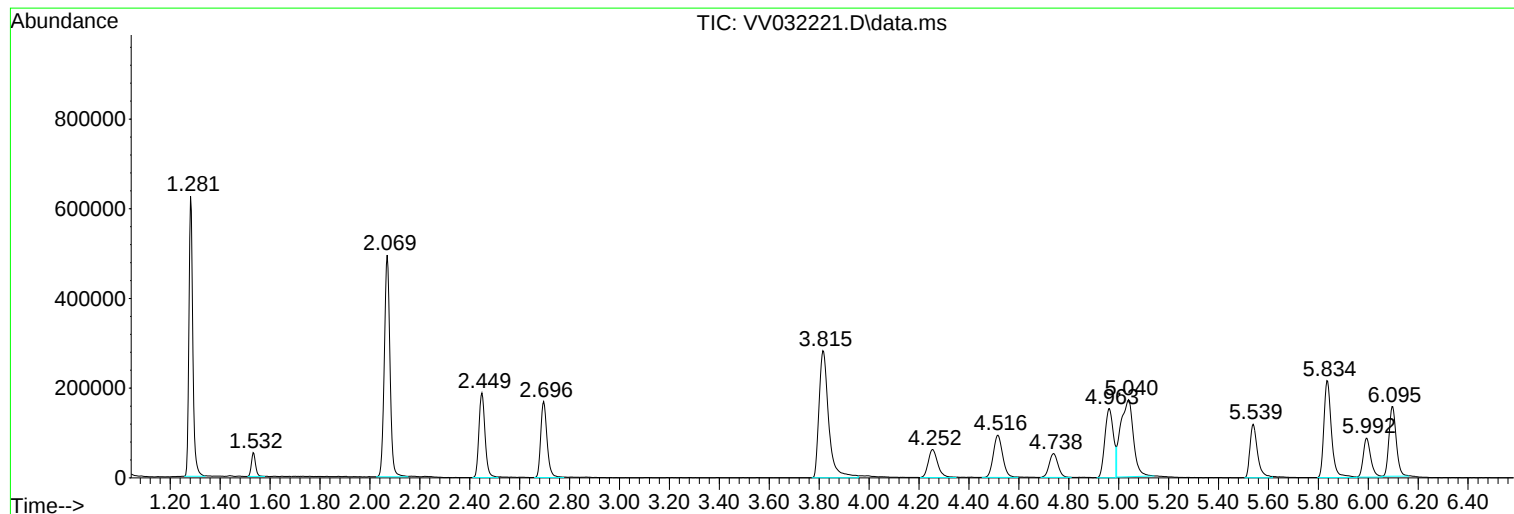

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032221.D
Acq On : 04 Oct 2023 11:27
Operator : SY/MD
Sample : 04708-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJU2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032221.D
Acq On : 04 Oct 2023 11:27
Operator : SY/MD
Sample : 04708-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJU2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc