

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032223.D
 Acq On : 04 Oct 2023 12:40
 Operator : SY/MD
 Sample : 04708-07DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJU2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032223.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	67	75	94	rVB2	166754	181896	30.06%	3.185%
2	1.532	145	153	169	rVB	52178	61553	10.17%	1.078%
3	2.066	307	319	337	rBV3	150950	260366	43.02%	4.559%
4	2.449	427	438	455	rBV	51429	87101	14.39%	1.525%
5	2.699	505	516	537	rBV	32441	59189	9.78%	1.036%
6	3.818	853	864	908	rBV2	82990	266164	43.98%	4.661%
7	4.256	983	1000	1027	rBV	61380	161494	26.69%	2.828%
8	4.516	1065	1081	1102	rBV2	18139	45705	7.55%	0.800%
9	4.744	1136	1152	1167	rBV3	9432	24370	4.03%	0.427%
10	4.963	1203	1220	1233	rBV2	151276	384806	63.59%	6.739%
11	5.539	1386	1399	1432	rBV	144942	308558	50.99%	5.403%
12	5.841	1481	1493	1528	rVB4	41451	93876	15.51%	1.644%
13	5.992	1528	1540	1563	rBV	84628	185264	30.61%	3.244%
14	6.101	1563	1574	1591	rVB2	28810	61331	10.13%	1.074%
15	6.921	1819	1829	1854	rBV	39434	79491	13.14%	1.392%
16	7.249	1918	1931	1946	rBV	176498	318363	52.61%	5.575%
17	7.323	1946	1954	1973	rVB	40227	77482	12.80%	1.357%
18	7.561	2017	2028	2056	rBV	22783	47273	7.81%	0.828%
19	7.776	2086	2095	2117	rVB	18966	35459	5.86%	0.621%
20	7.908	2125	2136	2156	rBV	91743	159323	26.33%	2.790%
21	8.034	2164	2175	2213	rBV	186630	399571	66.03%	6.997%
22	8.789	2399	2410	2440	rBV2	234761	525485	86.83%	9.202%
23	8.950	2450	2460	2482	rVB	96736	157091	25.96%	2.751%
24	9.079	2488	2500	2521	rBV	170264	276300	45.66%	4.838%
25	9.500	2614	2631	2659	rBV2	146530	298088	49.26%	5.220%
26	10.159	2825	2836	2855	rBV	64586	103447	17.09%	1.812%
27	11.191	3146	3157	3184	rBV2	255673	605170	100.00%	10.598%
28	11.564	3260	3273	3297	rBV2	188574	351795	58.13%	6.161%
29	13.204	3773	3783	3803	rBV	60577	94474	15.61%	1.654%




Sum of corrected areas: 5710485

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032223.D
Acq On : 04 Oct 2023 12:40
Operator : SY/MD
Sample : 04708-07DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJU2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

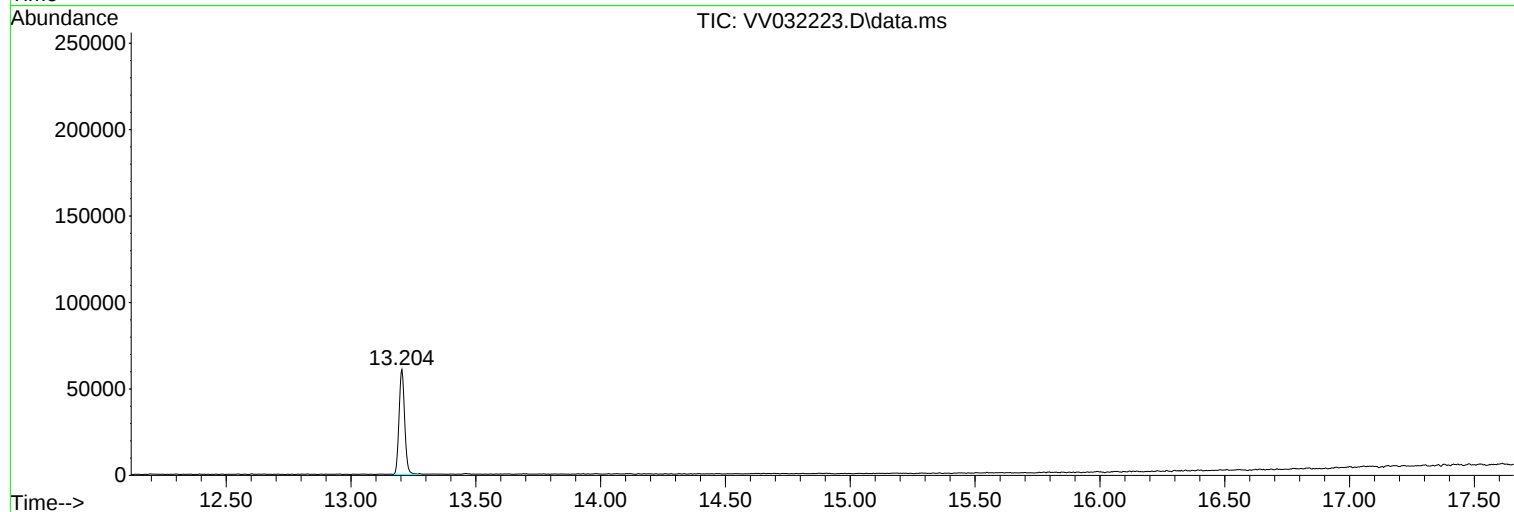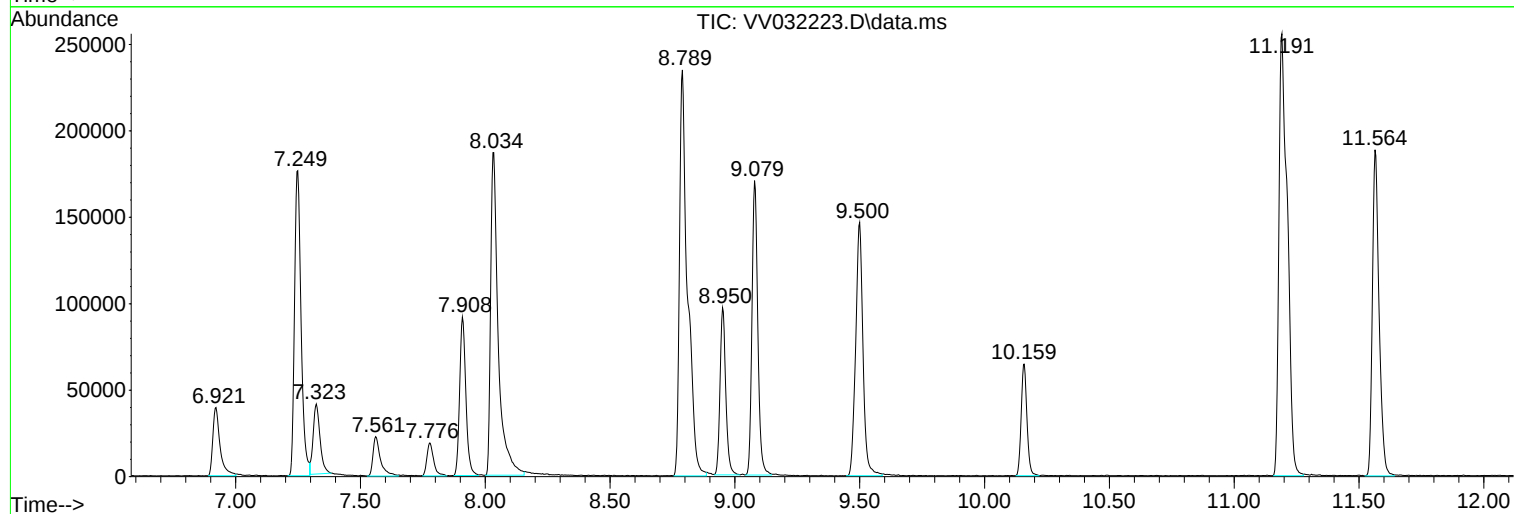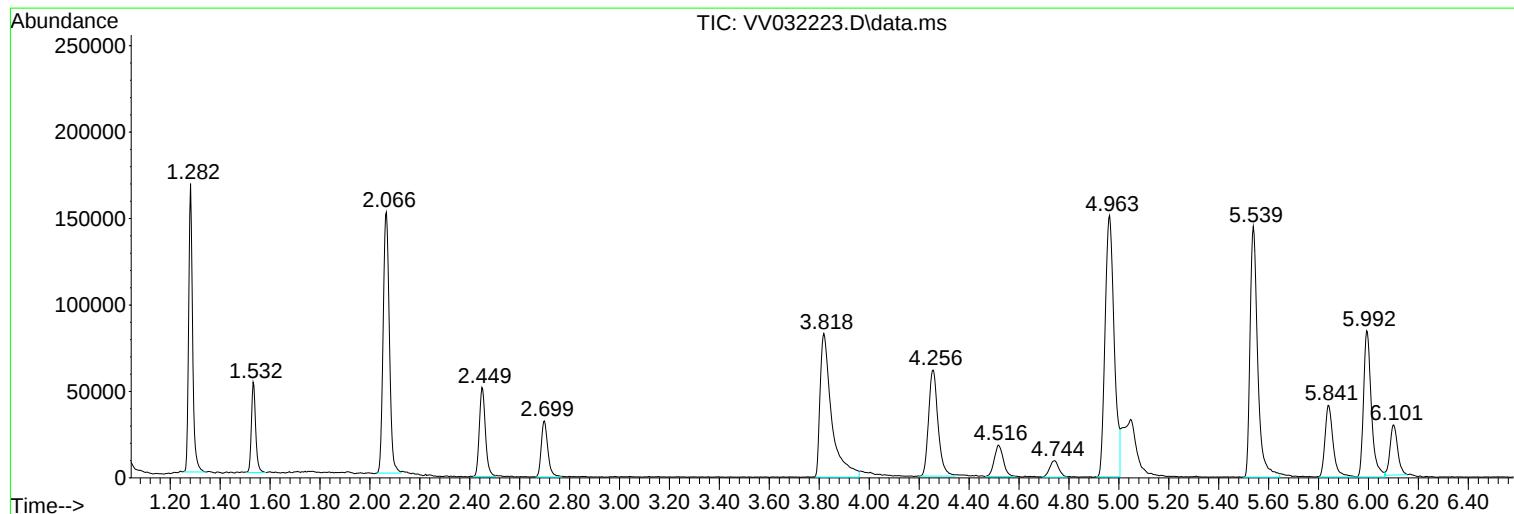

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032223.D
Acq On : 04 Oct 2023 12:40
Operator : SY/MD
Sample : 04708-07DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJU2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032223.D
Acq On : 04 Oct 2023 12:40
Operator : SY/MD
Sample : 04708-07DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJU2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc