

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032230.D
 Acq On : 04 Oct 2023 15:28
 Operator : SY/MD
 Sample : 04708-02DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJR7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	26	rVB3	4070	5081	1.32%	0.149%
2	1.278	67	74	90	rVB	54194	59823	15.59%	1.758%
3	1.532	145	153	163	rBV	47358	55881	14.56%	1.642%
4	2.060	307	317	333	rBV	85113	125070	32.59%	3.675%
5	2.449	427	438	450	rBV	22060	36687	9.56%	1.078%
6	3.815	853	863	900	rBV	40624	148757	38.76%	4.371%
7	4.256	982	1000	1026	rBV2	57358	151067	39.36%	4.439%
8	4.963	1204	1220	1257	rBV3	137834	365264	95.16%	10.733%
9	5.539	1388	1399	1421	rBV	103539	221078	57.60%	6.496%
10	5.838	1479	1492	1525	rBV	172051	362600	94.47%	10.655%
11	5.995	1529	1541	1582	rVB	79066	175002	45.59%	5.142%
12	6.921	1818	1829	1861	rBV	35984	74071	19.30%	2.177%
13	7.249	1919	1931	1954	rBV	157858	290476	75.68%	8.536%
14	7.561	2019	2028	2052	rBV2	20292	41737	10.87%	1.226%
15	8.034	2164	2175	2213	rBV	178192	383825	100.00%	11.279%
16	8.789	2399	2410	2433	rBV	163409	282206	73.52%	8.293%
17	10.159	2825	2836	2852	rBV	58967	95382	24.85%	2.803%
18	11.191	3143	3157	3179	rBV	174791	275573	71.80%	8.098%
19	11.564	3262	3273	3291	rBV	158054	253473	66.04%	7.448%




Sum of corrected areas: 3403053

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032230.D
Acq On : 04 Oct 2023 15:28
Operator : SY/MD
Sample : 04708-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJR7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

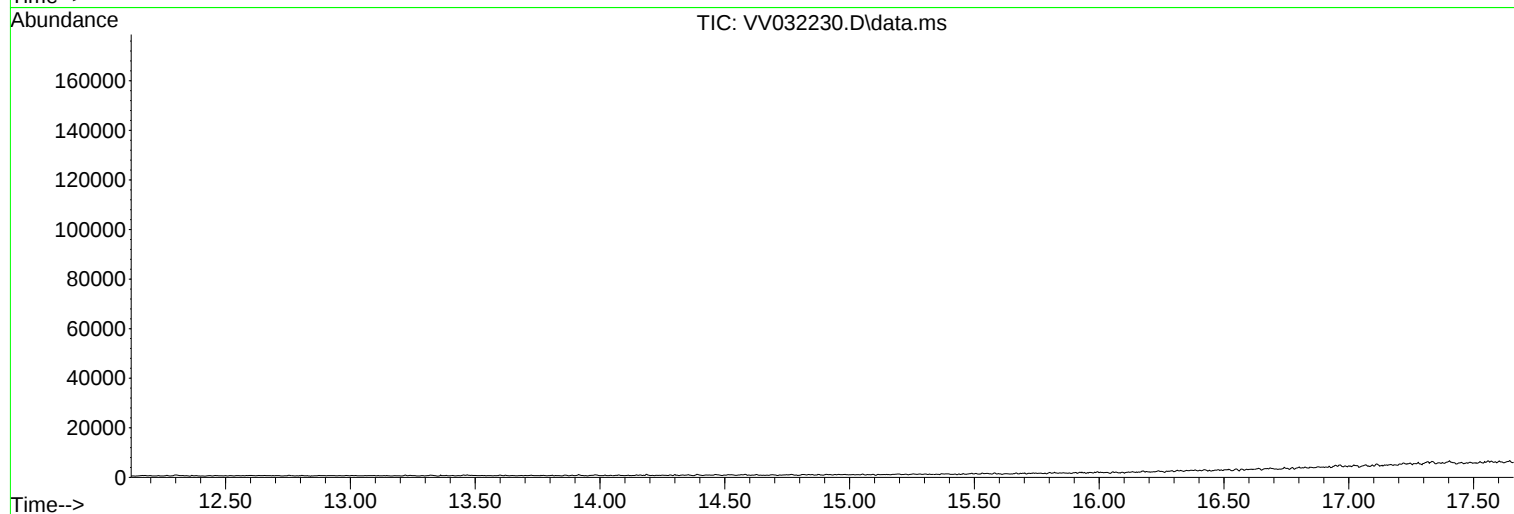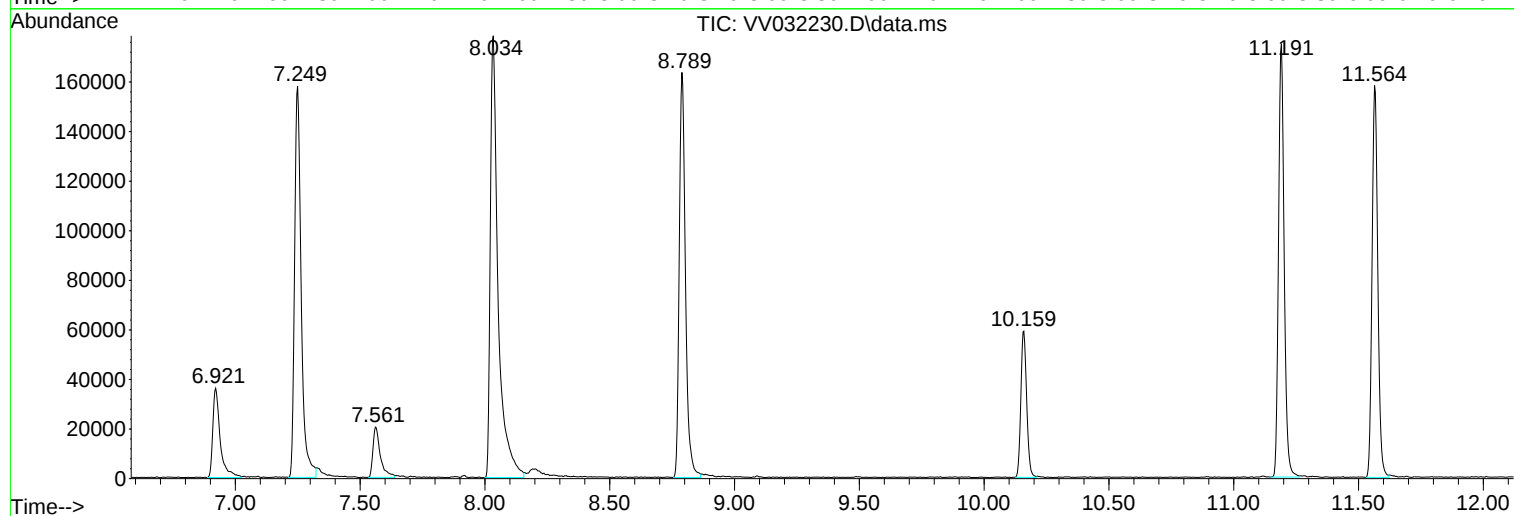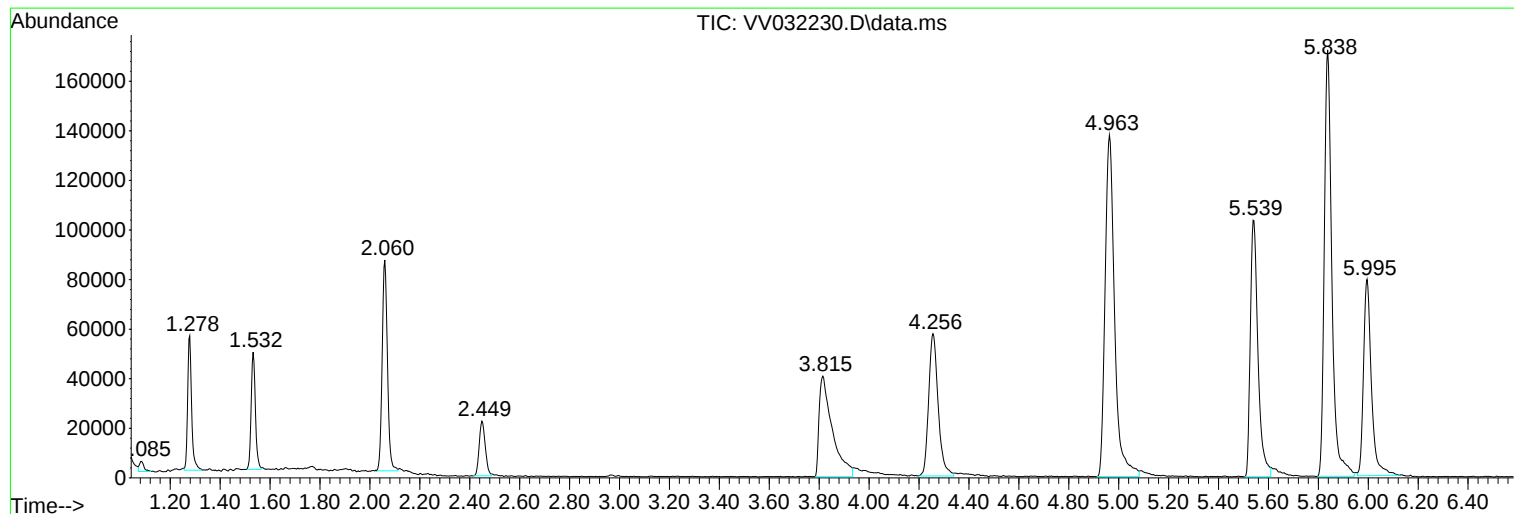

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032230.D
Acq On : 04 Oct 2023 15:28
Operator : SY/MD
Sample : 04708-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJR7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032230.D
Acq On : 04 Oct 2023 15:28
Operator : SY/MD
Sample : 04708-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJR7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc