

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032231.D
 Acq On : 04 Oct 2023 15:53
 Operator : SY/MD
 Sample : 04741-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032231.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	86	rBV	54360	58387	14.76%	1.756%
2	1.532	145	153	167	rVB	48651	57007	14.41%	1.715%
3	2.060	306	317	333	rBV	87324	128936	32.60%	3.878%
4	3.806	851	860	891	rBV	44298	145577	36.81%	4.379%
5	4.256	983	1000	1030	rBV2	63436	191256	48.35%	5.753%
6	4.960	1204	1219	1245	rBV2	142116	366955	92.77%	11.038%
7	5.539	1386	1399	1423	rBV	108178	228251	57.71%	6.866%
8	5.841	1482	1493	1505	rBV8	4336	10538	2.66%	0.317%
9	5.995	1528	1541	1577	rBV2	80212	181149	45.80%	5.449%
10	6.439	1667	1679	1703	rBV	26345	54662	13.82%	1.644%
11	6.918	1816	1828	1858	rBV	36746	76531	19.35%	2.302%
12	7.249	1918	1931	1968	rBV	164377	305002	77.11%	9.175%
13	7.561	2016	2028	2043	rBV	22352	42150	10.66%	1.268%
14	7.912	2121	2137	2159	rBV	48382	87703	22.17%	2.638%
15	8.031	2164	2174	2208	rBV	187682	395535	100.00%	11.898%
16	8.182	2211	2221	2244	rVB2	25654	49766	12.58%	1.497%
17	8.789	2399	2410	2445	rBV	167462	292270	73.89%	8.792%
18	9.674	2676	2685	2694	rBV2	5570	8868	2.24%	0.267%
19	10.159	2821	2836	2851	rBV	61356	100580	25.43%	3.025%
20	11.191	3146	3157	3178	rBV	173874	280459	70.91%	8.436%
21	11.564	3263	3273	3298	rBV	163546	262857	66.46%	7.907%




Sum of corrected areas: 3324439

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032231.D
Acq On : 04 Oct 2023 15:53
Operator : SY/MD
Sample : 04741-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

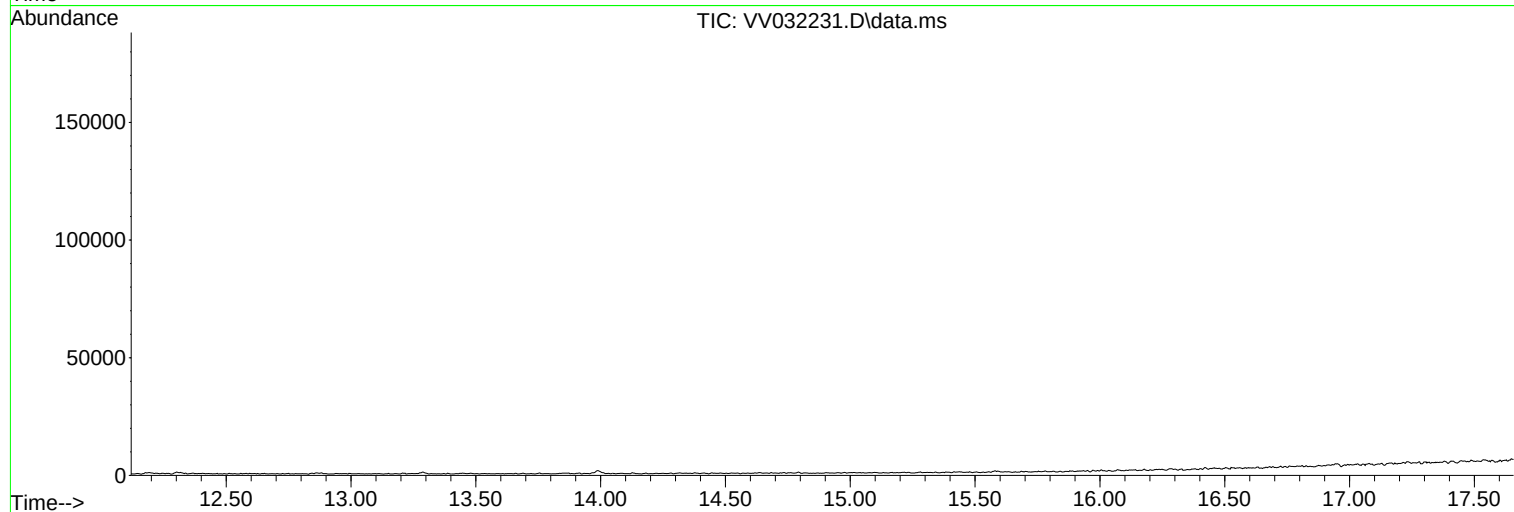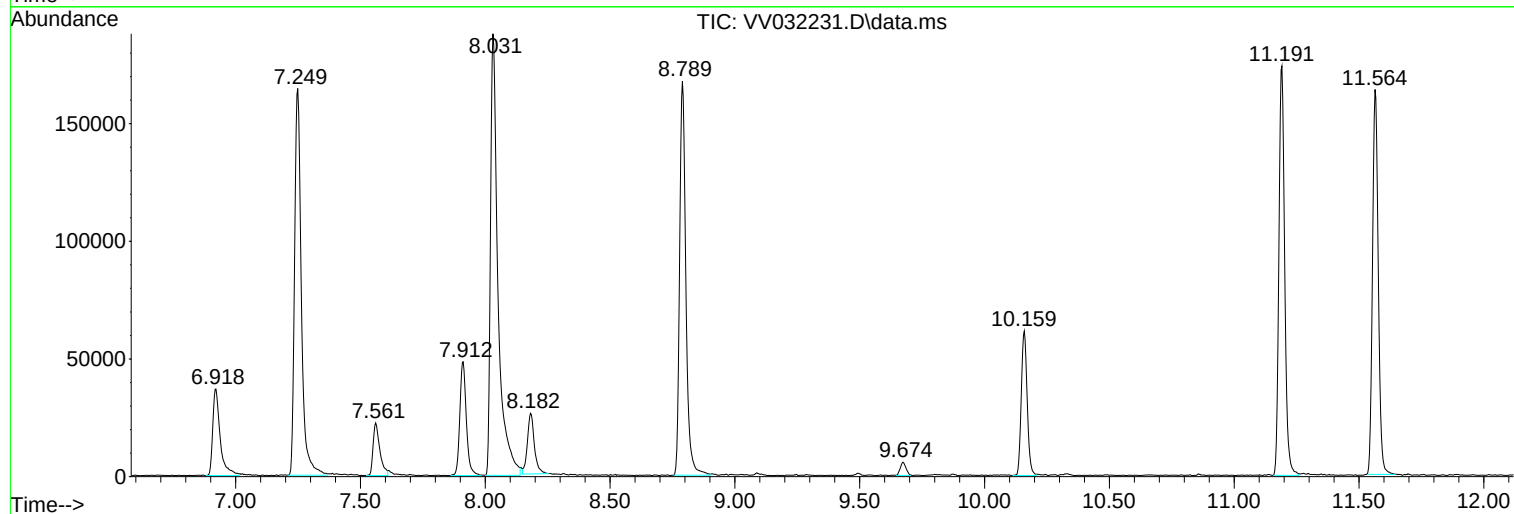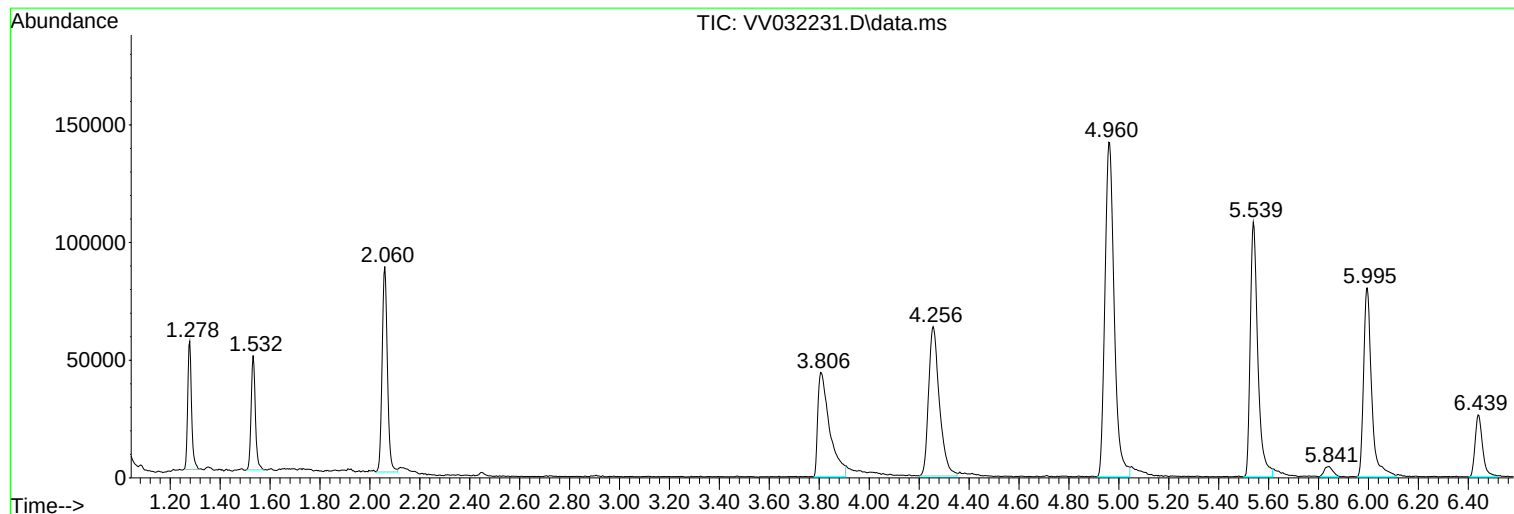

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032231.D
Acq On : 04 Oct 2023 15:53
Operator : SY/MD
Sample : 04741-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032231.D
Acq On : 04 Oct 2023 15:53
Operator : SY/MD
Sample : 04741-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc