

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032232.D
 Acq On : 04 Oct 2023 16:16
 Operator : SY/MD
 Sample : 04741-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rVB	53237	56333	14.45%	1.834%
2	1.532	145	153	164	rBV	48308	55295	14.18%	1.800%
3	2.059	306	317	330	rBV	85063	125024	32.06%	4.069%
4	3.809	851	861	902	rBV	46002	150145	38.51%	4.887%
5	4.256	983	1000	1023	rBV	58921	155676	39.93%	5.067%
6	4.963	1204	1220	1247	rBV2	140307	361693	92.76%	11.773%
7	5.538	1387	1399	1421	rBV	102699	220098	56.45%	7.164%
8	5.834	1482	1491	1511	rVB6	3907	8962	2.30%	0.292%
9	5.995	1529	1541	1559	rBV	79538	171026	43.86%	5.567%
10	6.442	1670	1680	1698	rBV2	4957	10161	2.61%	0.331%
11	6.921	1819	1829	1850	rBV	36477	73245	18.78%	2.384%
12	7.249	1919	1931	1958	rBV	158787	292317	74.97%	9.515%
13	7.561	2019	2028	2045	rBV	21741	41667	10.69%	1.356%
14	7.911	2128	2137	2155	rVB	17744	32556	8.35%	1.060%
15	8.034	2165	2175	2212	rBV	181950	389916	100.00%	12.692%
16	8.181	2213	2221	2238	rVB2	9104	18828	4.83%	0.613%
17	8.789	2399	2410	2446	rBV	167164	287129	73.64%	9.346%
18	10.159	2825	2836	2860	rBV	59139	96266	24.69%	3.133%
19	11.191	3145	3157	3175	rBV	170227	268556	68.88%	8.741%
20	11.564	3261	3273	3293	rBV	160321	257346	66.00%	8.376%




Sum of corrected areas: 3072239

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032232.D
Acq On : 04 Oct 2023 16:16
Operator : SY/MD
Sample : 04741-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

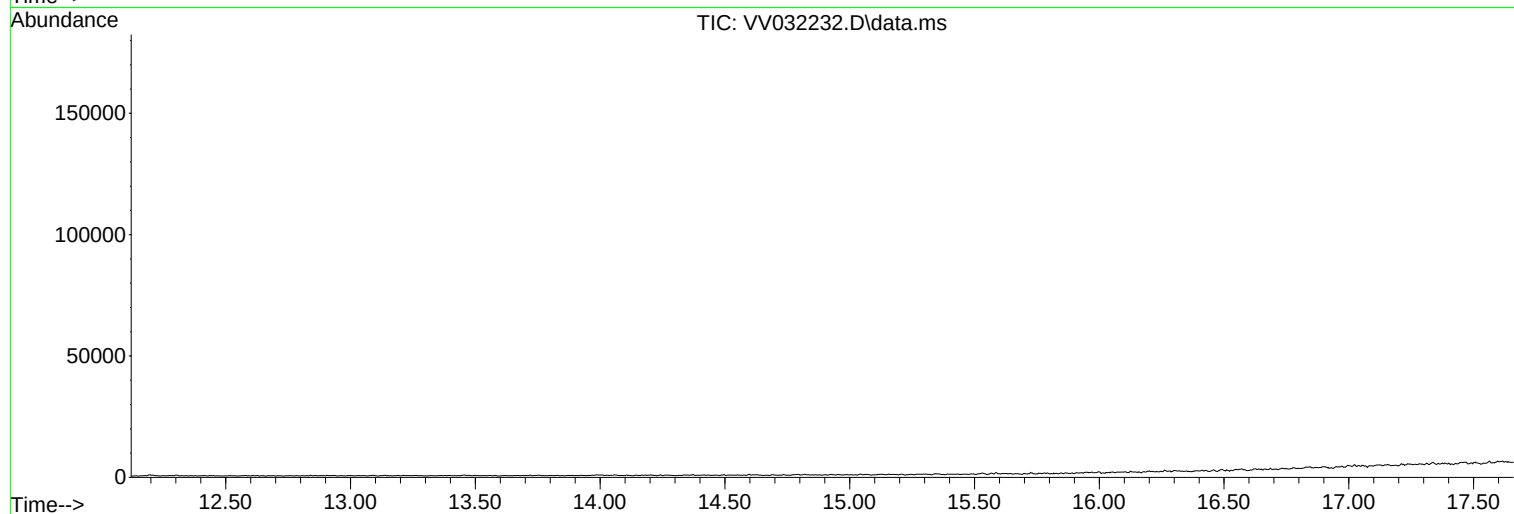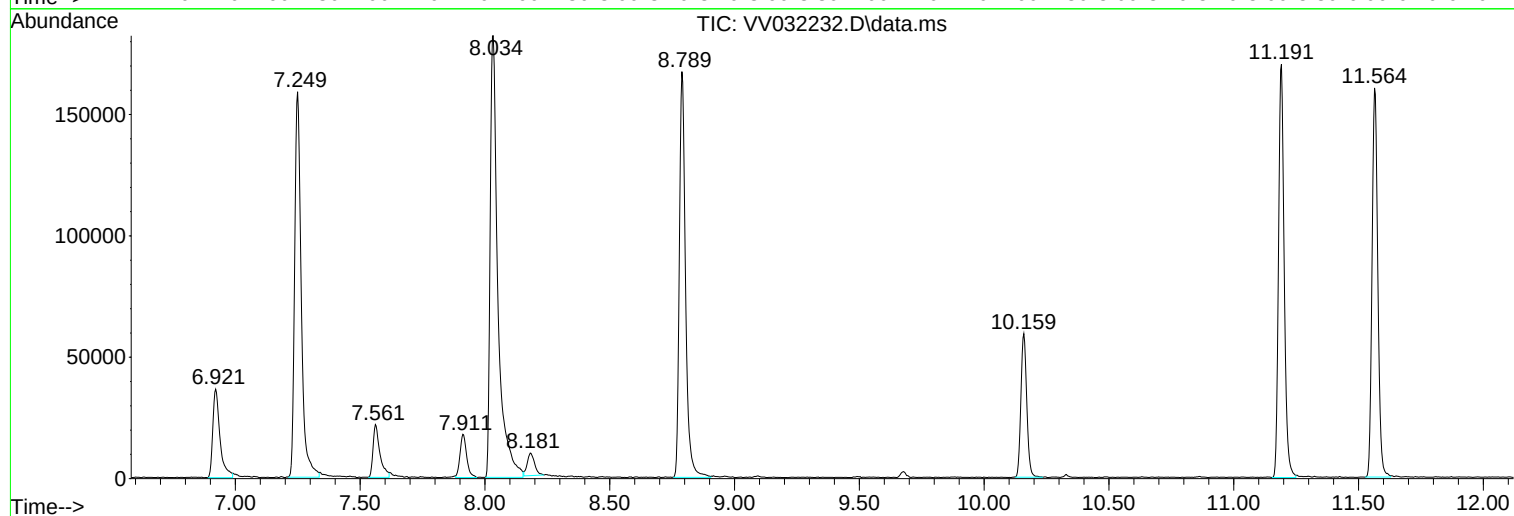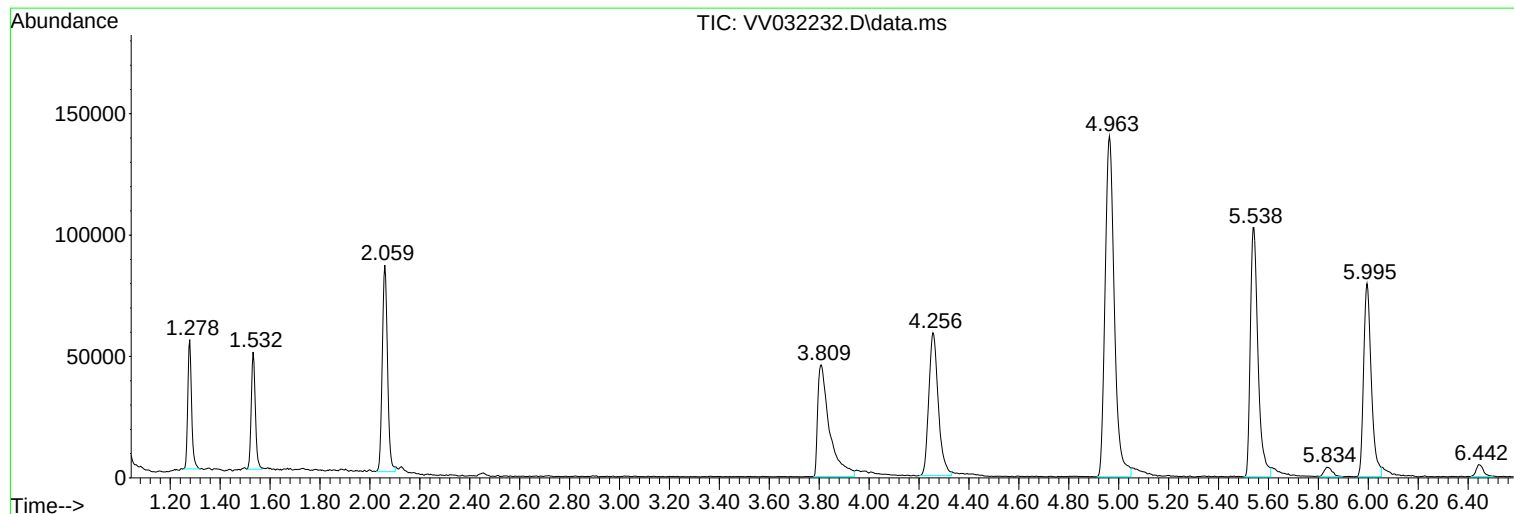

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032232.D
Acq On : 04 Oct 2023 16:16
Operator : SY/MD
Sample : 04741-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032232.D
Acq On : 04 Oct 2023 16:16
Operator : SY/MD
Sample : 04741-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc