

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032233.D
 Acq On : 04 Oct 2023 16:39
 Operator : SY/MD
 Sample : 04741-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	93	rBV	53785	59410	14.56%	1.865%
2	1.532	145	153	163	rBV	49385	57514	14.09%	1.805%
3	2.060	307	317	332	rBV	87485	128953	31.60%	4.047%
4	3.812	852	862	895	rBV2	43719	150300	36.83%	4.717%
5	4.256	981	1000	1024	rBV	62688	173532	42.52%	5.446%
6	4.963	1204	1220	1244	rBV2	144935	371458	91.03%	11.658%
7	5.539	1388	1399	1420	rBV	99352	212279	52.02%	6.662%
8	5.841	1481	1493	1510	rVB8	4298	9907	2.43%	0.311%
9	5.995	1528	1541	1561	rBV2	83042	179728	44.04%	5.641%
10	6.442	1668	1680	1697	rBV	11920	24798	6.08%	0.778%
11	6.921	1817	1829	1856	rBV	37222	77310	18.95%	2.426%
12	7.249	1919	1931	1961	rBV	163356	305088	74.76%	9.575%
13	7.561	2019	2028	2051	rBV2	22418	44753	10.97%	1.405%
14	7.911	2127	2137	2158	rVB3	23274	43279	10.61%	1.358%
15	8.034	2163	2175	2211	rBV	191668	408071	100.00%	12.807%
16	8.185	2213	2222	2242	rVB	15648	30897	7.57%	0.970%
17	8.789	2400	2410	2434	rBV	159881	272382	66.75%	8.549%
18	9.673	2678	2685	2696	rVB2	3710	5950	1.46%	0.187%
19	10.159	2822	2836	2859	rVB	62456	100647	24.66%	3.159%
20	11.191	3145	3157	3176	rBV	164796	263582	64.59%	8.273%
21	11.564	3261	3273	3292	rBV	166953	266350	65.27%	8.360%




Sum of corrected areas: 3186188

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032233.D
Acq On : 04 Oct 2023 16:39
Operator : SY/MD
Sample : 04741-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

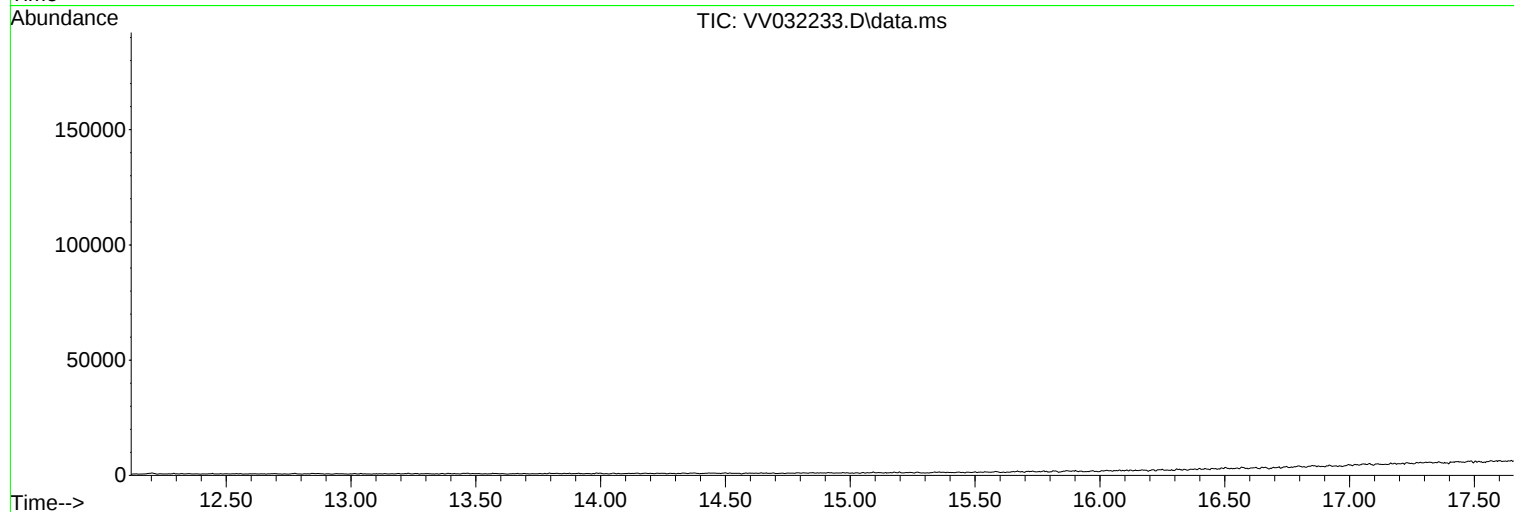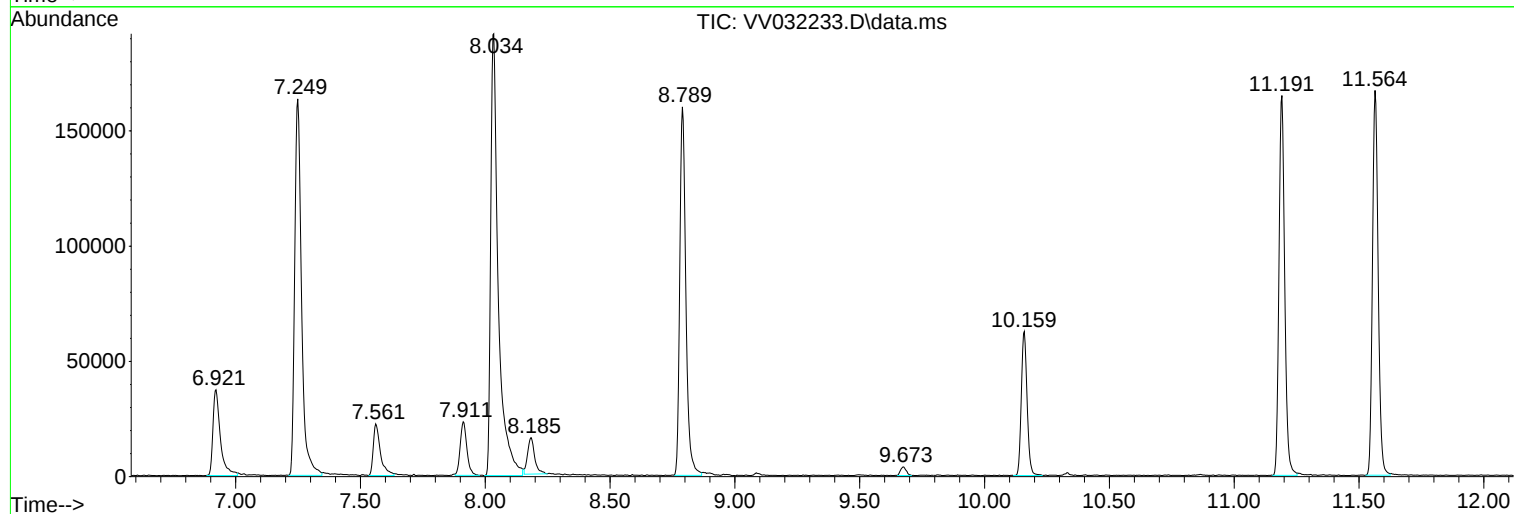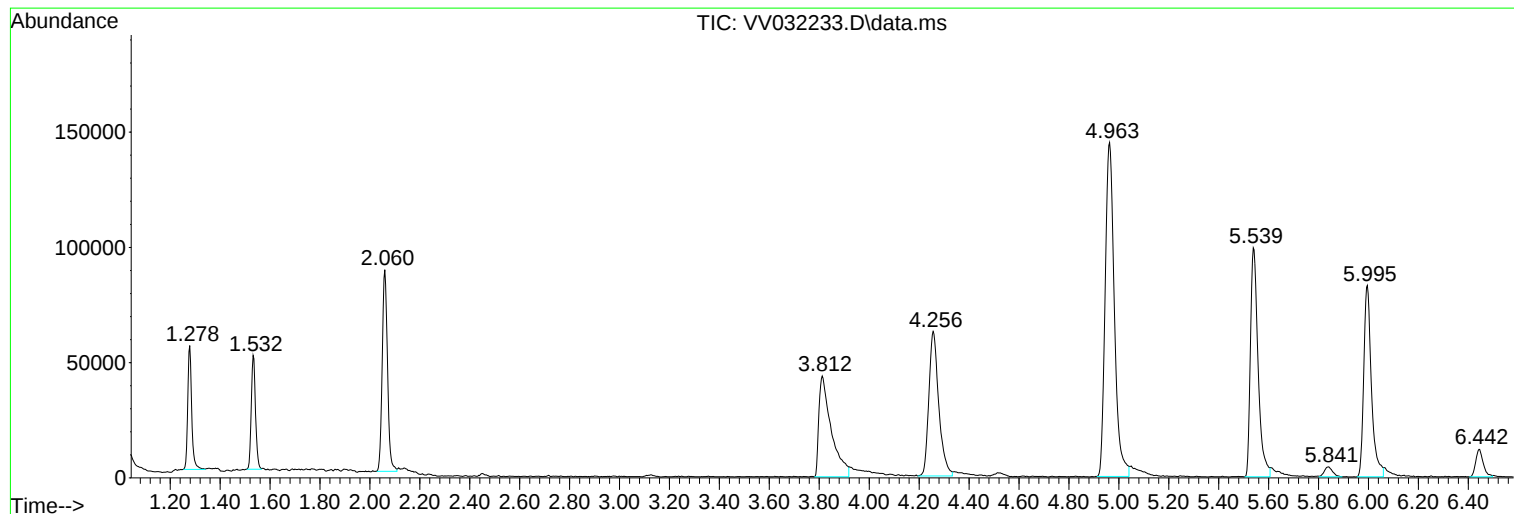

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032233.D
Acq On : 04 Oct 2023 16:39
Operator : SY/MD
Sample : 04741-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032233.D
Acq On : 04 Oct 2023 16:39
Operator : SY/MD
Sample : 04741-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------