

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032235.D
 Acq On : 04 Oct 2023 17:28
 Operator : SY/MD
 Sample : 04741-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032235.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	88	rVB	53017	57461	14.14%	1.852%
2	1.532	146	153	163	rBV	49373	56253	13.84%	1.813%
3	2.060	307	317	331	rBV	85445	125007	30.76%	4.028%
4	3.812	853	862	890	rBV	40530	142727	35.12%	4.599%
5	4.256	981	1000	1029	rBV3	59528	160438	39.47%	5.170%
6	4.963	1205	1220	1241	rBV2	142981	365486	89.92%	11.778%
7	5.539	1387	1399	1424	rBV	99960	216562	53.28%	6.979%
8	5.841	1482	1493	1506	rVB6	3864	8359	2.06%	0.269%
9	5.995	1528	1541	1577	rBV2	82735	186160	45.80%	5.999%
10	6.921	1817	1829	1846	rBV2	36718	73094	17.98%	2.355%
11	7.249	1918	1931	1967	rBV	160295	303502	74.67%	9.780%
12	7.561	2017	2028	2051	rBV2	22226	44419	10.93%	1.431%
13	7.912	2119	2137	2156	rBV2	21661	39993	9.84%	1.289%
14	8.034	2165	2175	2214	rBV	188205	406440	100.00%	13.097%
15	8.185	2214	2222	2234	rVB5	4852	10289	2.53%	0.332%
16	8.789	2399	2410	2436	rBV	161341	276896	68.13%	8.923%
17	10.159	2824	2836	2853	rBV	63236	100219	24.66%	3.229%
18	11.191	3146	3157	3177	rBV	167641	265001	65.20%	8.539%
19	11.564	3261	3273	3291	rBV	168130	264933	65.18%	8.537%




Sum of corrected areas: 3103239

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032235.D
Acq On : 04 Oct 2023 17:28
Operator : SY/MD
Sample : 04741-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

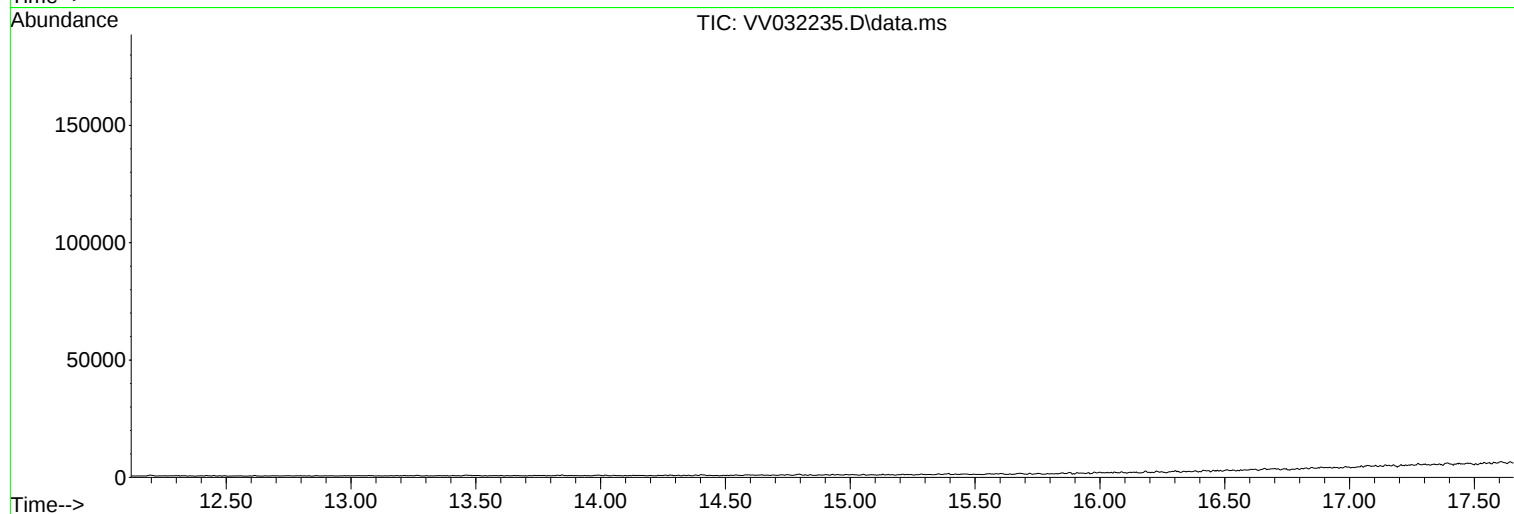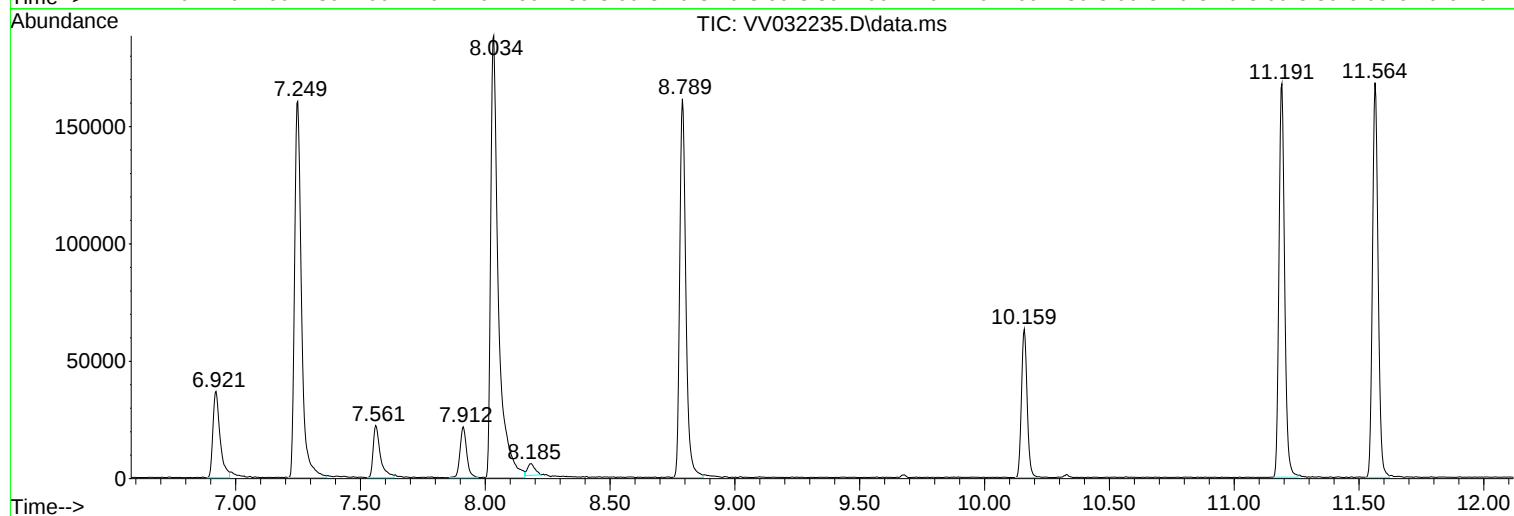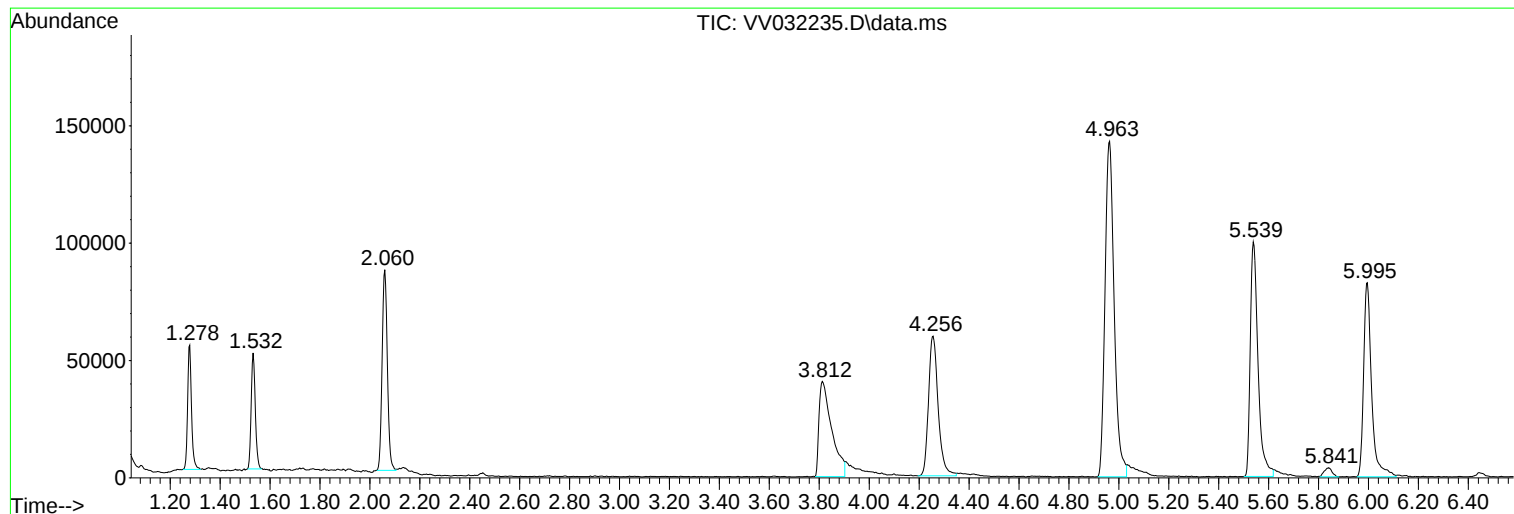

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032235.D
Acq On : 04 Oct 2023 17:28
Operator : SY/MD
Sample : 04741-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032235.D
Acq On : 04 Oct 2023 17:28
Operator : SY/MD
Sample : 04741-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc