

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032236.D
 Acq On : 04 Oct 2023 17:53
 Operator : SY/MD
 Sample : 04741-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ6

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rVB	51652	55185	14.67%	1.831%
2	1.532	145	153	166	rBV	47372	55661	14.79%	1.847%
3	2.060	307	317	330	rBV	81116	118963	31.61%	3.947%
4	3.812	852	862	901	rBV2	42914	148228	39.39%	4.918%
5	4.256	983	1000	1027	rBV	56698	156528	41.60%	5.193%
6	4.960	1204	1219	1244	rBV2	135279	347778	92.42%	11.539%
7	5.539	1386	1399	1422	rBV	101370	214455	56.99%	7.115%
8	5.828	1481	1489	1506	rVB9	3323	8058	2.14%	0.267%
9	5.995	1527	1541	1565	rBV2	77828	170998	45.44%	5.674%
10	6.442	1666	1680	1691	rBV3	7485	14869	3.95%	0.493%
11	6.921	1816	1829	1858	rBV2	34905	73081	19.42%	2.425%
12	7.249	1919	1931	1961	rBV	151834	283554	75.35%	9.408%
13	7.561	2018	2028	2048	rBV	20010	39884	10.60%	1.323%
14	7.912	2119	2137	2153	rBV2	18522	36478	9.69%	1.210%
15	8.034	2165	2175	2206	rBV	176219	376298	100.00%	12.485%
16	8.185	2213	2222	2234	rVB	10894	20051	5.33%	0.665%
17	8.789	2399	2410	2437	rBV	162853	277861	73.84%	9.219%
18	10.159	2825	2836	2857	rBV	58477	94473	25.11%	3.135%
19	10.329	2881	2889	2898	rBV2	3749	5300	1.41%	0.176%
20	11.191	3142	3157	3177	rBV	167967	266290	70.77%	8.835%
21	11.564	3263	3273	3290	rBV	158566	249977	66.43%	8.294%




Sum of corrected areas: 3013970

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032236.D
Acq On : 04 Oct 2023 17:53
Operator : SY/MD
Sample : 04741-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

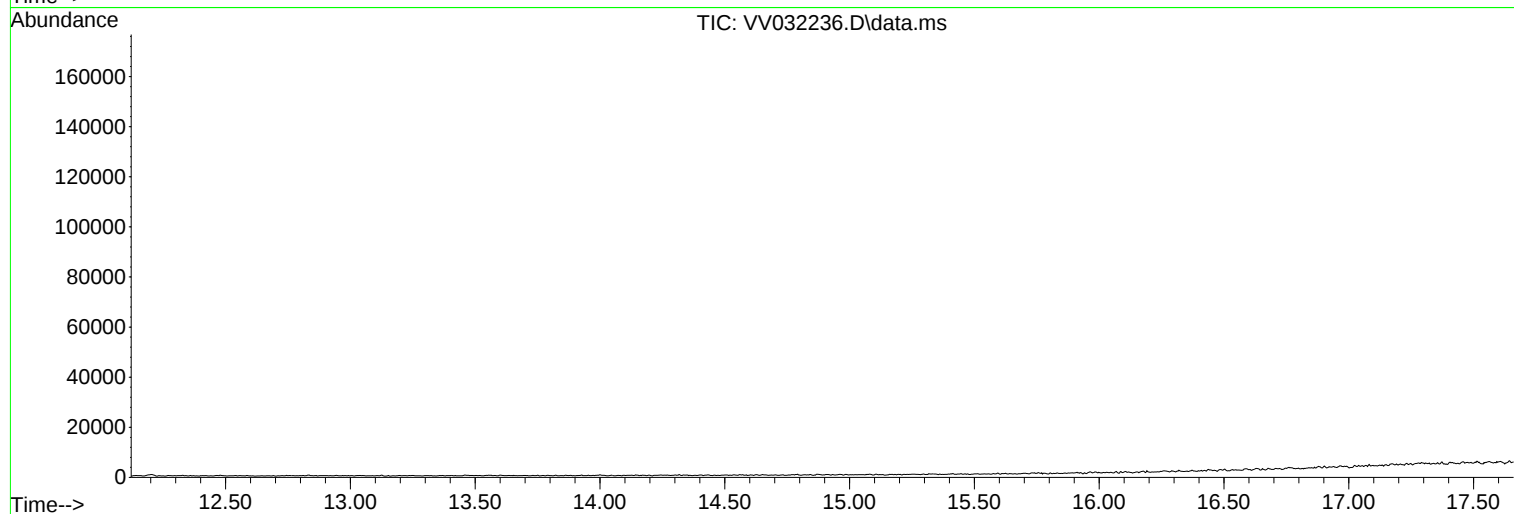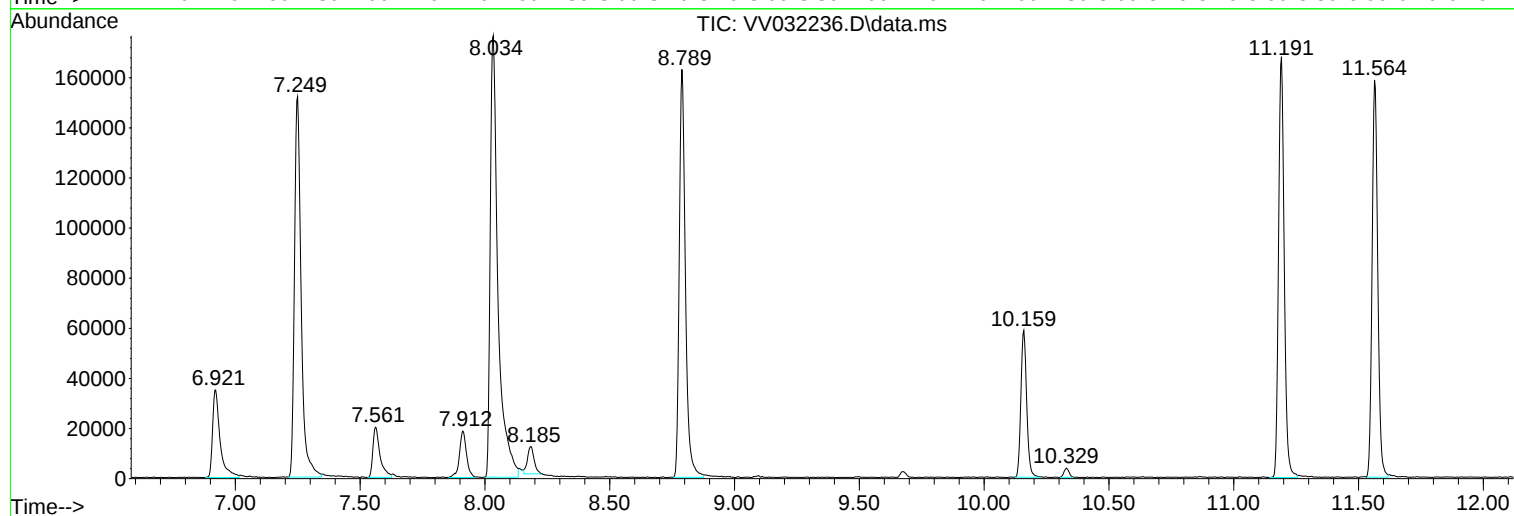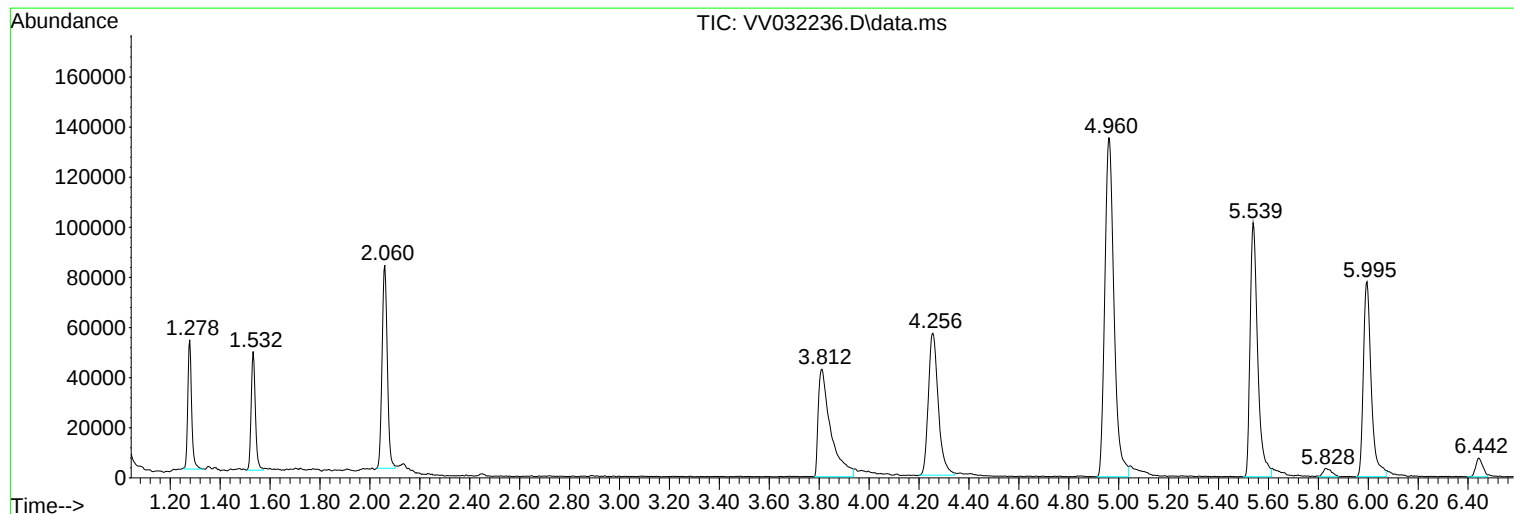

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032236.D
Acq On : 04 Oct 2023 17:53
Operator : SY/MD
Sample : 04741-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032236.D
Acq On : 04 Oct 2023 17:53
Operator : SY/MD
Sample : 04741-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc